


LB120343

7470A

INSTRUMENT ID: CV1

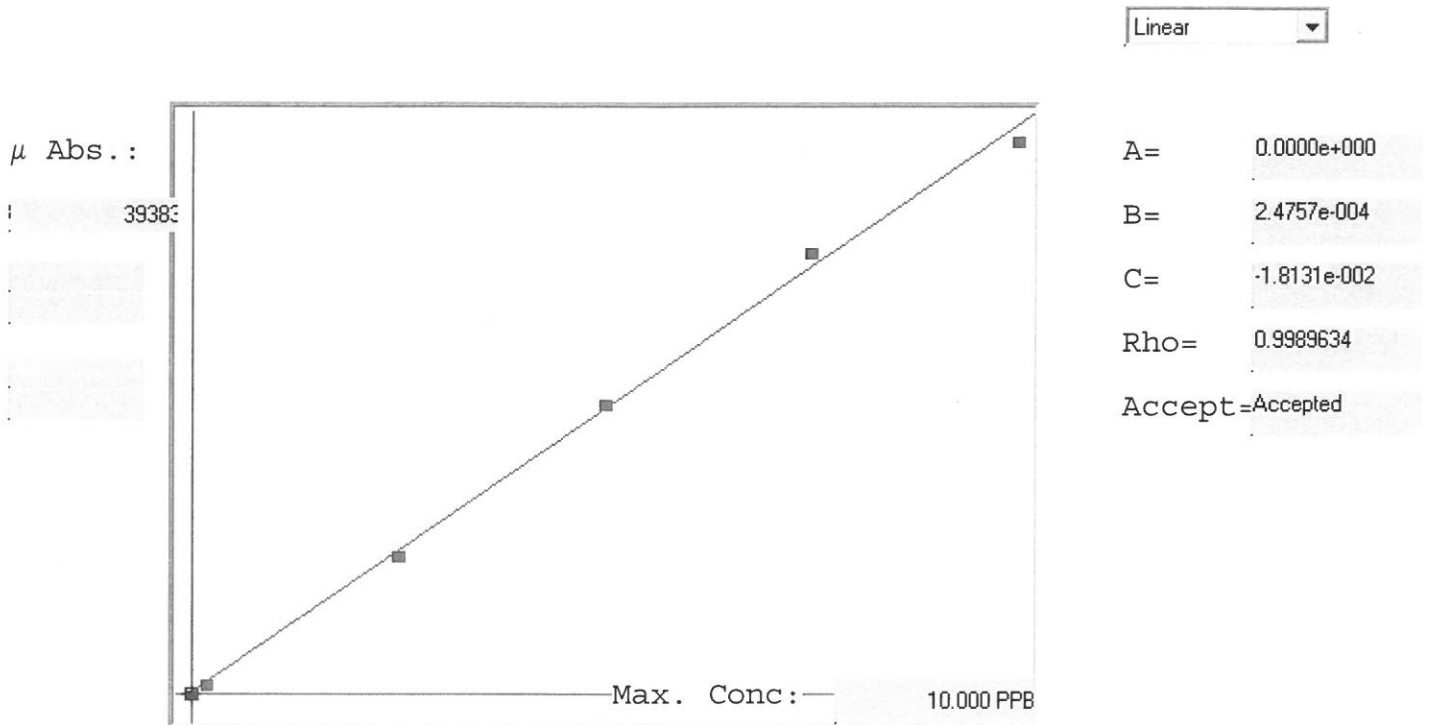

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/01
0.0	0.000	-0.040	-0.040	-87	0.000	-87					-13
0.2	0.200	0.175	-0.025	782	0.0 %	782					-3
2.5	2.500	2.437	-0.063	9915	0.0 %	9915					-3
5.0	5.000	5.117	0.117	20743	0.0 %	20743					2
7.5	7.500	7.778	0.278	31492	0.0 %	31492					4
10.0	10.000	9.732	-0.268	39383	0.0 %	39383					-3

LB120343 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 May 2022 10:03:36

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-87	-	0.0000	7470A	PPB	25 May 2022 10:08:56	S	Std
0.2 - 1	50.2	782	-	0.2000	7470A	PPB	25 May 2022 10:11:13	S	Std
2.5 - 1	52.5	9915	-	2.5000	7470A	PPB	25 May 2022 10:13:31	S	Std
5.0 - 1	55	20743	-	5.0000	7470A	PPB	25 May 2022 10:15:47	S	Std
7.5 - 1	57.5	31492	-	7.5000	7470A	PPB	25 May 2022 10:18:04	S	Std
10.0 - 1	510	39383	-	10.0000	7470A	PPB	25 May 2022 10:23:05	S	Std
ICV44 - 1	ICV44	15142	3.7306	-	7470A	PPB	25 May 2022 10:26:45	U	SMPL
ICB44 - 1	ICB44	50	-0.0058	-	7470A	PPB	25 May 2022 10:28:59	U	SMPL
CCV56 - 1	CCV56	18931	4.6687	-	7470A	PPB	25 May 2022 10:31:14	U	SMPL
CCB56 - 1	CCB56	41	-0.0080	-	7470A	PPB	25 May 2022 10:33:29	U	SMPL
CRA - 1	CRA	819	0.1846	-	7470A	PPB	25 May 2022 10:35:44	U	SMPL
HighStd - 1	HighStd	39073	9.6552	-	7470A	PPB	25 May 2022 10:37:58	U	SMPL
ChkStd - 1	ChkStd	27619	6.8196	-	7470A	PPB	25 May 2022 10:40:14	U	SMPL
PB145082BL - 1	PBW	-89	-0.0402	-	7470A	PPB	25 May 2022 10:42:31	U	SMPL
PB145082BS - 1	LCSW	14281	3.5174	-	7470A	PPB	25 May 2022 10:44:47	U	SMPL
N2981-21 - 1	TGMP-1	381	0.0762	-	7470A	PPB	25 May 2022 10:51:51	U	SMPL
N2981-21DUP - 1	TGMP-1DUP	365	0.0722	-	7470A	PPB	25 May 2022 10:54:07	U	SMPL
N2981-21MS - 1	TGMP-1MS	14778	3.6405	-	7470A	PPB	25 May 2022 10:56:25	U	SMPL
N2981-21MSD - 1	TGMP-1MSD	14408	3.5489	-	7470A	PPB	25 May 2022 10:58:42	U	SMPL
N2981-22 - 1	TGMP-3	176	0.0254	-	7470A	PPB	25 May 2022 11:00:57	U	SMPL
CCV57 - 1	CCV57	19412	4.7877	-	7470A	PPB	25 May 2022 11:03:13	U	SMPL
CCB57 - 1	CCB57	26	-0.0117	-	7470A	PPB	25 May 2022 11:05:28	U	SMPL
N2981-23 - 1	TGMP-4	2078	0.4963	-	7470A	PPB	25 May 2022 11:07:44	U	SMPL
N2981-24 - 1	TGMP-2	764	0.1710	-	7470A	PPB	25 May 2022 11:10:00	U	SMPL
N3006-01 - 1	220511095-01	1662	0.3933	-	7470A	PPB	25 May 2022 11:12:15	U	SMPL
N3008-01 - 1	220511036-05	22869	5.6436	-	7470A	PPB	25 May 2022 11:14:31	U	SMPL
N3011-01 - 1	220511032-03	7785	1.9092	-	7470A	PPB	25 May 2022 11:16:46	U	SMPL
N3012-01 - 1	220511032-02	2085	0.4981	-	7470A	PPB	25 May 2022 11:19:03	U	SMPL
N3017-01 - 1	220512093-01	29	-0.0110	-	7470A	PPB	25 May 2022 11:21:19	U	SMPL
N3018-01 - 1	220512035-01	56	-0.0043	-	7470A	PPB	25 May 2022 11:23:36	U	SMPL
N3019-01 - 1	220511048-01	3085	0.7456	-	7470A	PPB	25 May 2022 11:25:53	U	SMPL
N3020-01 - 1	220511031-01	2493	0.5991	-	7470A	PPB	25 May 2022 11:28:08	U	SMPL
CCV58 - 1	CCV58	21096	5.2046	-	7470A	PPB	25 May 2022 11:30:24	U	SMPL
CCB58 - 1	CCB58	101	0.0069	-	7470A	PPB	25 May 2022 11:32:39	U	SMPL
N3021-01 - 1	220511029-03	321	0.0613	-	7470A	PPB	25 May 2022 11:34:56	U	SMPL
N2981-21LX5 - 1		77	0.0009	-	7470A	PPB	25 May 2022 11:37:11	U	SMPL
N2981-21A - 1		15402	3.7950	-	7470A	PPB	25 May 2022 11:39:27	U	SMPL
CCV59 - 1	CCV59	19415	4.7885	-	7470A	PPB	25 May 2022 11:44:50	U	SMPL
CCB59 - 1	CCB59	42	-0.0077	-	7470A	PPB	25 May 2022 11:47:05	U	SMPL