

LB120363


7470A

INSTRUMENT ID: CV2

Linear

 μ Abs.:

41933

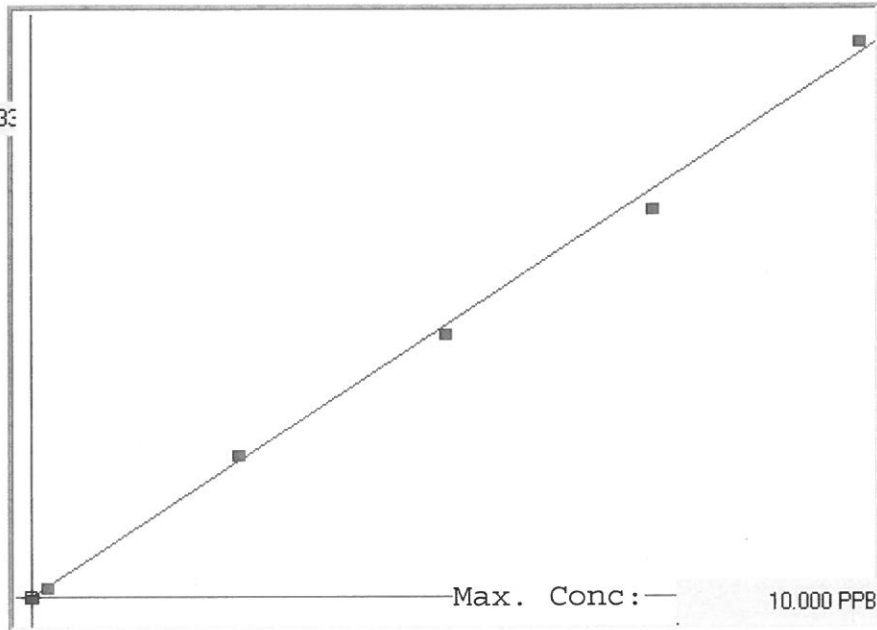

A= 0.0000e+000

B= 2.4404e-004

C= 1.0146e-002

Rho= 0.9987173

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.019	0.019	37	0.000	37					-
0.2	0.200	0.220	0.020	861	0.0 %	861					10
2.5	2.500	2.666	0.166	10882	0.0 %	10882					7
5.0	5.000	4.879	-0.121	19951	0.0 %	19951					-2
7.5	7.500	7.172	-0.328	29349	0.0 %	29349					-4
10.0	10.000	10.243	0.243	41933	0.0 %	41933					2

LB120363 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 May 2022 10:09:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	37	-	0.0000	7470A	PPB	26 May 2022 10:14:33	S	Std
0.2 - 1	50.2	861	-	0.2000	7470A	PPB	26 May 2022 10:19:24	S	Std
2.5 - 1	52.5	10882	-	2.5000	7470A	PPB	26 May 2022 10:21:41	S	Std
5.0 - 1	55	19951	-	5.0000	7470A	PPB	26 May 2022 10:23:58	S	Std
7.5 - 1	57.5	29349	-	7.5000	7470A	PPB	26 May 2022 10:26:14	S	Std
10.0 - 1	57.5	41933	-	10.0000	7470A	PPB	26 May 2022 10:28:30	S	Std
ICV46 - 1	ICV46	16718	4.0900	-	7470A	PPB	26 May 2022 10:31:33	U	SMPL
ICB46 - 1	ICB46	10	0.0126	-	7470A	PPB	26 May 2022 10:36:20	U	SMPL
CCV64 - 1	CCV64	19819	4.8467	-	7470A	PPB	26 May 2022 10:38:34	U	SMPL
CCB64 - 1	CCB64	-12	0.0072	-	7470A	PPB	26 May 2022 10:43:19	U	SMPL
CRA - 1	CRA	830	0.2127	-	7470A	PPB	26 May 2022 10:45:33	U	SMPL
HighStd - 1	HighStd	40946	10.0025	-	7470A	PPB	26 May 2022 10:47:48	U	SMPL
ChkStd - 1	ChkStd	28049	6.8552	-	7470A	PPB	26 May 2022 10:50:03	U	SMPL
PB145111BL - 1	PBW	-11	0.0075	-	7470A	PPB	26 May 2022 10:56:01	U	SMPL
PB145111BS - 1	LCSW	17210	4.2100	-	7470A	PPB	26 May 2022 10:58:16	U	SMPL
N3024-11 - 1	31532-34AQ	157621	38.4757	-	7470A	PPB	26 May 2022 11:00:33	U	SMPL
N3026-01 - 1	N48967	1484	0.3723	-	7470A	PPB	26 May 2022 11:09:28	U	SMPL
N3026-01DUP - 1	N48967DUP	1450	0.3640	-	7470A	PPB	26 May 2022 11:11:45	U	SMPL
N3026-01MS - 1	N48967MS	17710	4.3321	-	7470A	PPB	26 May 2022 11:14:02	U	SMPL
N3026-01MSD - 1	N48967MSD	15522	3.7981	-	7470A	PPB	26 May 2022 11:16:17	U	SMPL
CCV65 - 1	CCV65	20215	4.9434	-	7470A	PPB	26 May 2022 11:18:32	U	SMPL
CCB65 - 1	CCB65	-71	-0.0072	-	7470A	PPB	26 May 2022 11:25:42	U	SMPL
N3038-01 - 1	TT-045-IPWGW-20220524	367	0.0997	-	7470A	PPB	26 May 2022 11:27:57	U	SMPL
N3053-07 - 1	52322-WATER	986	0.2508	-	7470A	PPB	26 May 2022 11:30:12	U	SMPL
N3059-01 - 1	4922A	109	0.0367	-	7470A	PPB	26 May 2022 11:32:27	U	SMPL
N3026-01LX5 - 1		299	0.0831	-	7470A	PPB	26 May 2022 11:34:43	U	SMPL
N3026-01A - 1		17924	4.3843	-	7470A	PPB	26 May 2022 11:36:59	U	SMPL
N3024-11DLX5 - 1		18045	4.4138	-	7470A	PPB	26 May 2022 11:39:16	U	SMPL
CCV66 - 1	CCV66	20215	4.9434	-	7470A	PPB	26 May 2022 11:41:33	U	SMPL
CCB66 - 1	CCB66	-84	-0.0104	-	7470A	PPB	26 May 2022 11:43:50	U	SMPL