

LB12 0.371

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : Sy Instrument ID : Konelab

5/26/2022 12:10

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.332	0.0	0.075	
ICB1	0.267	0.0	0.001	
CCV1	239.521	0.0	0.190	
CCB1	0.229	0.0	0.001	
N3028-02	0.084	0.0	0.001	
N3028-02DUP	0.086	0.0	0.001	
N3041-02	0.199	0.0	0.001	
N3042-07	0.052	0.0	0.001	
PB145126BL	0.092	0.0	0.001	
N3026-01	-0.077	0.0	0.001	
N3026-01DUP	-0.001	0.0	0.001	
PB145125BL	0.026	0.0	0.001	
CCV2	254.008	0.0	0.201	
CCB2	0.118	0.0	0.001	

N 14
Mean 41.995
SD 90.2606
CV% 214.93

Aquakem v. 7.2AQ1

Results from time period:

Wed May 25 16:30:11 2022

Thu May 26 12:07:41 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.0PPBCN	A	Total CN	P	-0.3045	µg/l	5/26/2022 10:19:35
5.0PPBCN	A	Total CN	P	4.7074	µg/l	5/26/2022 10:19:36
10PPBCN	A	Total CN	P	9.9902	µg/l	5/26/2022 10:19:37
50PPBCN	A	Total CN	P	50.8874	µg/l	5/26/2022 10:19:38
100PPBCN	A	Total CN	P	99.3407	µg/l	5/26/2022 10:19:39
250PPBCN	A	Total CN	P	250.6649	µg/l	5/26/2022 10:19:40
500PPBCN	A	Total CN	P	499.7137	µg/l	5/26/2022 10:19:41
ICV1	S	Total CN	P	93.3317	µg/l	5/26/2022 11:39:24
ICB1	S	Total CN	P	0.2671	µg/l	5/26/2022 11:39:25
CCV1	S	Total CN	P	239.5205	µg/l	5/26/2022 11:39:26
CCB1	S	Total CN	P	0.2291	µg/l	5/26/2022 11:39:27
N3028-02	S	Total CN	P	0.084	µg/l	5/26/2022 11:39:29
N3028-02DUP	S	Total CN	P	0.086	µg/l	5/26/2022 11:39:30
N3041-02	S	Total CN	P	0.1985	µg/l	5/26/2022 11:39:31
N3042-07	S	Total CN	P	0.0517	µg/l	5/26/2022 11:39:32
PB145126BL	S	Total CN	P	0.0918	µg/l	5/26/2022 11:39:33
N3026-01	S	Total CN	P	-0.0772	µg/l	5/26/2022 11:39:34
N3026-01DUP	S	Total CN	P	-0.0013	µg/l	5/26/2022 11:45:40
PB145125BL	S	Total CN	P	0.0256	µg/l	5/26/2022 12:07:39
CCV2	S	Total CN	P	254.0077	µg/l	5/26/2022 12:07:40
CCB2	S	Total CN	P	0.1175	µg/l	5/26/2022 12:07:41

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

5/26/2022 10:28

Reviewed by : *SL*

Instrument ID : Konelab


Test Total CN

Accepted 5/26/2022 10:28

Factor 1267
Bias 0.001

Coeff. of det. 0.999991

Errors

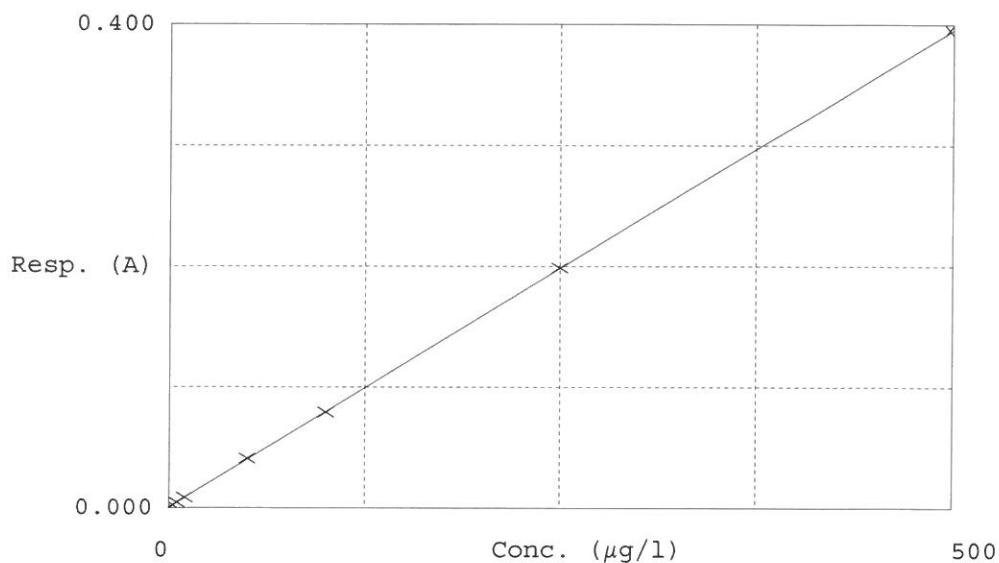

					<i>R</i>
	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.3045	0.0000	-5.9
2	5.0PPBCN	0.005	4.7074	5.0000	-0.1
3	10PPBCN	0.009	9.9902	10.0000	1.8
4	50PPBCN	0.041	50.8874	50.0000	-0.7
5	100PPBCN	0.079	99.3407	100.0000	0.3
6	250PPBCN	0.199	250.6649	250.0000	-0.1
7	500PPBCN	0.395	499.7137	500.0000	

SL 5/26/22