

LB120437

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : 12 Instrument ID : Konelab

6/1/2022 16:35

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.456	0.0	0.076	
ICB1	-0.536	0.0	0.001	
CCV1	256.289	0.0	0.197	
CCB1	-0.338	0.0	0.001	
N2990-05	-0.875	0.0	0.001	
N2990-06	-0.754	0.0	0.001	
N2990-06DUP	-0.906	0.0	0.001	
N2990-07	-0.932	0.0	0.001	
N2990-08	-0.524	0.0	0.001	
N2990-09	-0.938	0.0	0.001	
N3051-02	-0.733	0.0	0.001	
N2990-21MS	38.525	0.0	0.031	
N2990-22MSD	38.733	0.0	0.031	
CCV2	263.988	0.0	0.203	
CCB2	-0.348	0.0	0.001	

N	15
Mean	45.874
SD	91.1416
CV%	198.68

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 01 15:47:49 2022

Wed Jun 01 16:34:44 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.0PPBCN	A	Total CN	P	-0.7299	µg/l	6/1/2022 10:19:37
5.0PPBCN	A	Total CN	P	3.9739	µg/l	6/1/2022 10:19:38
10PPBCN	A	Total CN	P	9.4775	µg/l	6/1/2022 10:19:39
50PPBCN	A	Total CN	P	49.6787	µg/l	6/1/2022 10:19:40
100PPBCN	A	Total CN	P	101.0518	µg/l	6/1/2022 10:19:41
250PPBCN	A	Total CN	P	253.4111	µg/l	6/1/2022 10:19:42
500PPBCN	A	Total CN	P	498.1369	µg/l	6/1/2022 10:19:43
ICV1	S	Total CN	P	97.4559	µg/l	6/1/2022 15:47:49
ICB1	S	Total CN	P	-0.5362	µg/l	6/1/2022 15:47:52
CCV1	S	Total CN	P	256.2886	µg/l	6/1/2022 15:47:53
CCB1	S	Total CN	P	-0.3383	µg/l	6/1/2022 15:47:55
N2990-05	S	Total CN	P	-0.875	µg/l	6/1/2022 15:47:57
N2990-06	S	Total CN	P	-0.7537	µg/l	6/1/2022 15:47:58
N2990-06DUP	S	Total CN	P	-0.9063	µg/l	6/1/2022 15:47:59
N2990-07	S	Total CN	P	-0.9325	µg/l	6/1/2022 15:54:02
N2990-08	S	Total CN	P	-0.5242	µg/l	6/1/2022 15:54:03
N2990-09	S	Total CN	P	-0.9385	µg/l	6/1/2022 15:54:04
N3051-02	S	Total CN	P	-0.7328	µg/l	6/1/2022 15:54:05
N2990-21MS	S	Total CN	P	38.5252	µg/l	6/1/2022 16:15:15
N2990-22MSD	S	Total CN	P	38.733	µg/l	6/1/2022 16:15:17
CCV2	S	Total CN	P	263.9883	µg/l	6/1/2022 16:15:18
CCB2	S	Total CN	P	-0.3481	µg/l	6/1/2022 16:34:44

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RE

Instrument ID : Konelab

6/1/2022 10:21


Test Total CN

Accepted 6/1/2022 10:21

Factor 1311
Bias 0.002

Coeff. of det. 0.999912

Errors

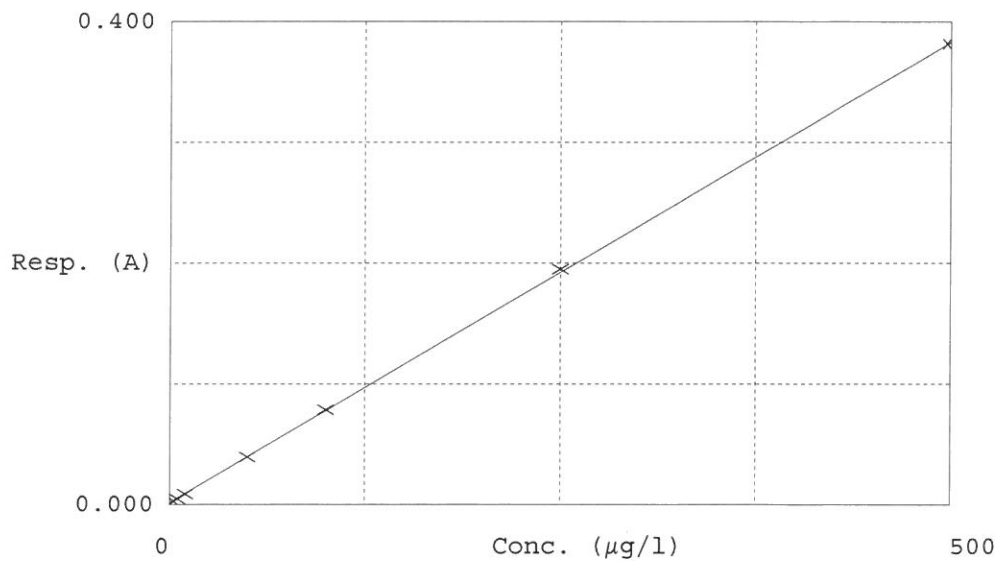

					<i>Re</i>
Calibrator	Response	Calc. con.	Conc.	Errors	
1	0.0PPBCN	0.001	-0.7299	0.0000	
2	5.0PPBCN	0.005	3.9739	5.0000	-20.5
3	10PPBCN	0.009	9.4775	10.0000	5.2
4	50PPBCN	0.040	49.6787	50.0000	-0.6
5	100PPBCN	0.079	101.0518	100.0000	1.1
6	250PPBCN	0.195	253.4111	250.0000	1.4
7	500PPBCN	0.382	498.1369	500.0000	-0.6

12

6/1/22