

LB120452

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

6/1/2022 15:12

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.005	0.0	0.106	
ICB1	-0.000	0.0	0.006	
CCV1	0.971	0.0	0.102	
CCB1	-0.000	0.0	0.006	
PB145249BL	0.000	0.0	0.006	
PB145249BS	1.012	0.0	0.106	
N3068-01	0.997	0.0	0.105	
N3068-01DUP	1.110	0.0	0.116	
N3068-01MS	2.138	0.0	0.218	Test limit high
N3068-01MSD	2.143	0.0	0.218	Test limit high
CCV2	0.959	0.0	0.101	
CCB2	-0.001	0.0	0.006	

N	12
Mean	0.861
SD	0.7621
CV%	88.50

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 01 14:35:14 2022

Wed Jun 01 15:09:03 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0007	mg/l	6/1/2022 14:35:14	
0.05PPM	A	Phenolics-	P	0.0503	mg/l	6/1/2022 14:35:15	
0.1PPM	A	Phenolics-	P	0.0998	mg/l	6/1/2022 14:35:16	
0.25PPM	A	Phenolics-	P	0.2502	mg/l	6/1/2022 14:35:17	
0.50PPM	A	Phenolics-	P	0.5087	mg/l	6/1/2022 14:35:18	
1.0PPM	A	Phenolics-	P	0.988	mg/l	6/1/2022 14:35:19	
2.0PPM	A	Phenolics-	P	2.0038	mg/l	6/1/2022 14:35:20	
ICV1	S	Phenolics-	P	1.005	mg/l	6/1/2022 15:03:09	
ICB1	S	Phenolics-	P	-0.0002	mg/l	6/1/2022 15:03:10	
CCV1	S	Phenolics-	P	0.9712	mg/l	6/1/2022 15:03:12	
CCB1	S	Phenolics-	P	-0.0004	mg/l	6/1/2022 15:03:14	
PB145249BL	S	Phenolics-	P	0.0004	mg/l	6/1/2022 15:03:17	
PB145249BS	S	Phenolics-	P	1.0116	mg/l	6/1/2022 15:03:18	
N3068-01	S	Phenolics-	P	0.9969	mg/l	6/1/2022 15:08:58	
N3068-01DUP	S	Phenolics-	P	1.1097	mg/l	6/1/2022 15:08:59	
N3068-01MS	S	Phenolics-	P	2.1382	mg/l	6/1/2022 15:09:00	
N3068-01MSD	S	Phenolics-	P	2.1432	mg/l	6/1/2022 15:09:01	
CCV2	S	Phenolics-	P	0.9586	mg/l	6/1/2022 15:09:02	
CCB2	S	Phenolics-	P	-0.0011	mg/l	6/1/2022 15:09:03	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

6/1/2022 14:41

Reviewed by : 12

Instrument ID : Konelab

Test Phenolics-


Accepted 6/1/2022 14:35

Factor 10.09

Bias 0.006

Coeff. of det. 0.999926

Errors

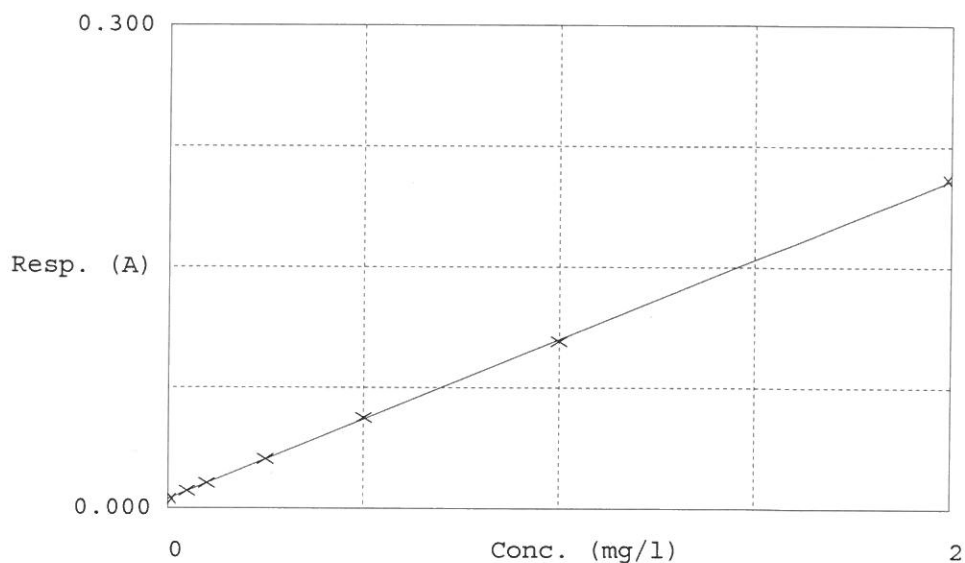

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	-0.0007	0.0000	-
2	Phenol-2	0.011	0.0503	0.0500	0.6
3	Phenol-2	0.016	0.0998	0.1000	-0.2
4	Phenol-2	0.031	0.2502	0.2500	0.1
5	Phenol-2	0.056	0.5087	0.5000	1.7
6	Phenol-2	0.104	0.9880	1.0000	-1.2
7	Phenol-2	0.204	2.0038	2.0000	0.2

12
6/1/22