


LB 120499

7470A

INSTRUMENT ID: CV2

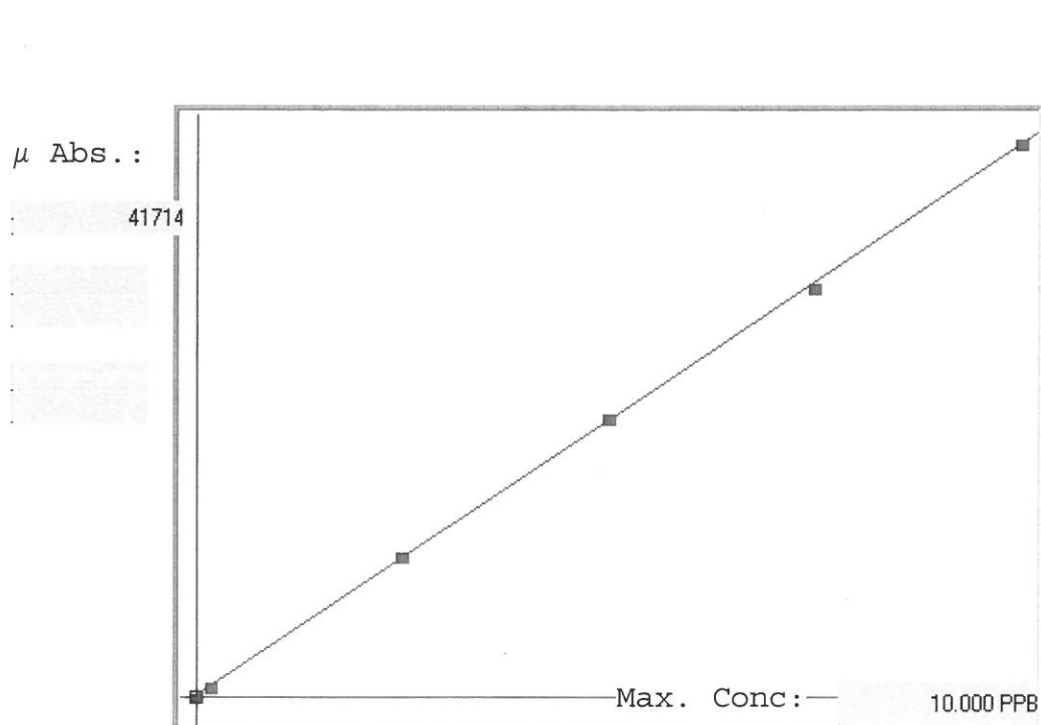

Linear

A= 0.0000e+000

B= 2.4078e-004

C= -1.4615e-002

Rho= 0.9999278

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.015	-0.015	-3	0.000	-3					-
0.2	0.200	0.185	-0.015	828	0.0 %	828					8
2.5	2.500	2.540	0.040	10611	0.0 %	10611					2
5.0	5.000	5.044	0.044	21009	0.0 %	21009					1
7.5	7.500	7.417	-0.083	30864	0.0 %	30864					-1
10.0	10.000	10.029	0.029	41714	0.0 %	41714					0

LB120499 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Jun 2022 07:12:44

Sample ID	Extended ID	μ Abs	Conc	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	5 ⁸	-3	-	0.00007470A	PPB		04 Jun 2022 07:26:42	S	Std
0.2 - 1	5 ⁶	828	-	0.20007470A	PPB		04 Jun 2022 07:28:59	S	Std
2.5 - 1	5 ^{2.5}	10611	-	2.50007470A	PPB		04 Jun 2022 07:31:16	S	Std
5.0 - 1	5 ⁵	21009	-	5.00007470A	PPB		04 Jun 2022 07:33:33	S	Std
7.5 - 1	5 ^{7.5}	30864	-	7.50007470A	PPB		04 Jun 2022 07:35:49	S	Std
10.0 - 1	5 ¹⁰	41714	-	10.00007470A	PPB		04 Jun 2022 07:38:05	S	Std
ICV59 - 1	ICV59	16250	3.8981	-7470A	PPB		04 Jun 2022 07:40:45	U	SMPL
ICB59 - 1	ICB59	-33	-0.0226	-7470A	PPB		04 Jun 2022 07:42:59	U	SMPL
CCV25 - 1	CCV25	20063	4.8162	-7470A	PPB		04 Jun 2022 07:45:15	U	SMPL
CCB25 - 1	CCB25	-46	-0.0257	-7470A	PPB		04 Jun 2022 07:47:30	U	SMPL
CRA - 1	CRA	807	0.1797	-7470A	PPB		04 Jun 2022 07:49:45	U	SMPL
HighStd - 1	HighStd	41338	9.9388	-7470A	PPB		04 Jun 2022 07:52:00	U	SMPL
ChkStd - 1	ChkStd	28111	6.7540	-7470A	PPB		04 Jun 2022 07:54:15	U	SMPL
PB145288BL - 1	PBW	-8	-0.0165	-7470A	PPB		04 Jun 2022 07:59:09	U	SMPL
PB145288BS - 1	LCSW	15097	3.6205	-7470A	PPB		04 Jun 2022 08:04:04	U	SMPL
N3143-05 - 1	20220425-SPLP-AMENDED-COMP-E	681	0.1494	-7470A	PPB		04 Jun 2022 08:06:19	U	SMPL
N3143-05DUP - 1	20220425-SPLP-AMENDED-COMP-EDUP	698	0.1535	-7470A	PPB		04 Jun 2022 08:08:35	U	SMPL
N3143-05MS - 1	20220425-SPLP-AMENDED-COMP-EMS	15289	3.6667	-7470A	PPB		04 Jun 2022 08:10:52	U	SMPL
N3143-05MSD - 1	20220425-SPLP-AMENDED-COMP-EMSD	15571	3.7346	-7470A	PPB		04 Jun 2022 08:13:09	U	SMPL
N3143-06 - 1	20220427-SPLP-AMENDED-SB-8-(DISCRETE-COMP-G)	-17	-0.0187	-7470A	PPB		04 Jun 2022 08:15:24	U	SMPL
CCV26 - 1	CCV26	21065	5.0575	-7470A	PPB		04 Jun 2022 08:17:40	U	SMPL
CCB26 - 1	CCB26	-32	-0.0223	-7470A	PPB		04 Jun 2022 08:19:55	U	SMPL
PB145309BL - 1	PBW	23	-0.0091	-7470A	PPB		04 Jun 2022 08:22:11	U	SMPL
PB145309BS - 1	LCSW	15752	3.7782	-7470A	PPB		04 Jun 2022 08:26:56	U	SMPL
N3143-07 - 1	20220408-FIELD-BLANK-1	-141	-0.0486	-7470A	PPB		04 Jun 2022 08:29:11	U	SMPL
N3154-02 - 1	COMP	623	0.1354	-7470A	PPB		04 Jun 2022 08:38:19	U	SMPL
N3154-02DUP - 1	COMP DUP	580	0.1250	-7470A	PPB		04 Jun 2022 08:40:35	U	SMPL
N3154-02MS - 1	COMPMS	16265	3.9017	-7470A	PPB		04 Jun 2022 08:45:42	U	SMPL
N3154-02MSD - 1	COMPMSD	16147	3.8733	-7470A	PPB		04 Jun 2022 08:47:59	U	SMPL
N3166-17 - 1	RB07-20220601	-135	-0.0471	-7470A	PPB		04 Jun 2022 08:50:17	U	SMPL
N3170-07 - 1	20220409-FIELD-BLANK-2	-62	-0.0295	-7470A	PPB		04 Jun 2022 08:52:34	U	SMPL
PB145311BL - 1	PBW	-27	-0.0211	-7470A	PPB		04 Jun 2022 08:54:49	U	SMPL
CCV27 - 1	CCV27	21637	5.1952	-7470A	PPB		04 Jun 2022 08:57:05	U	SMPL
CCB27 - 1	CCB27	-43	-0.0250	-7470A	PPB		04 Jun 2022 08:59:20	U	SMPL
PB145311BS - 1	LCSW	13872	3.3255	-7470A	PPB		04 Jun 2022 09:01:37	U	SMPL
N3170-05 - 1	20220422-SPLP-AMENDED-COMPOSITE-B	794	0.1766	-7470A	PPB		04 Jun 2022 09:03:53	U	SMPL
N3170-05DUP - 1	20220422-SPLP-AMENDED-COMPOSITE-BDUP	854	0.1910	-7470A	PPB		04 Jun 2022 09:06:08	U	SMPL
N3170-05MS - 1	20220422-SPLP-AMENDED-COMPOSITE-BMS	16707	4.0081	-7470A	PPB		04 Jun 2022 09:08:24	U	SMPL
N3170-05MSD - 1	20220422-SPLP-AMENDED-COMPOSITE-BMSD	17274	4.1447	-7470A	PPB		04 Jun 2022 09:10:41	U	SMPL
N3170-06 - 1	20220424-SPLP-AMENDED-COMPOSITE-D	2370	0.5560	-7470A	PPB		04 Jun 2022 09:12:57	U	SMPL
PB145330BL - 1	PBW	-36	-0.0233	-7470A	PPB		04 Jun 2022 09:15:14	U	SMPL
PB145330BS - 1	LCSW	16391	3.9320	-7470A	PPB		04 Jun 2022 09:17:30	U	SMPL
N3024-13 - 1	31532-34-SOL	-53	-0.0274	-7470A	PPB		04 Jun 2022 09:19:48	U	SMPL
N3169-01 - 1	149TH-ST-DRUM-2-PPE	-23	-0.0202	-7470A	PPB		04 Jun 2022 09:22:04	U	SMPL
CCV28 - 1	CCV28	21886	5.2551	-7470A	PPB		04 Jun 2022 09:24:19	U	SMPL
CCB28 - 1	CCB28	-114	-0.0421	-7470A	PPB		04 Jun 2022 09:26:35	U	SMPL
N3169-02 - 1	149TH-ST-DRUM-3-POLY	-18	-0.0189	-7470A	PPB		04 Jun 2022 09:28:51	U	SMPL
N3178-01 - 1	2329	-31	-0.0221	-7470A	PPB		04 Jun 2022 09:31:06	U	SMPL
N3178-01DUP - 1	2329DUP	-21	-0.0197	-7470A	PPB		04 Jun 2022 09:33:22	U	SMPL
N3178-01MS - 1	2329MS	17577	4.2176	-7470A	PPB		04 Jun 2022 09:35:37	U	SMPL
N3178-01MSD - 1	2329MSD	18089	4.3409	-7470A	PPB		04 Jun 2022 09:37:53	U	SMPL
PB145331BL - 1	PBW	-108	-0.0406	-7470A	PPB		04 Jun 2022 09:40:09	U	SMPL
PB145331BS - 1	LCSW	15401	3.6937	-7470A	PPB		04 Jun 2022 09:42:26	U	SMPL
N3119-03 - 1	40016	-98	-0.0382	-7470A	PPB		04 Jun 2022 09:44:43	U	SMPL
N3119-03DUP - 1	40016DUP	-25	-0.0206	-7470A	PPB		04 Jun 2022 09:47:00	U	SMPL
N3119-03MS - 1	40016MS	16594	3.9809	-7470A	PPB		04 Jun 2022 09:49:16	U	SMPL
CCV29 - 1	CCV29	20434	4.9055	-7470A	PPB		04 Jun 2022 09:51:32	U	SMPL
CCB29 - 1	CCB29	-108	-0.0406	-7470A	PPB		04 Jun 2022 09:53:48	U	SMPL
N3119-03MSD - 1	40016MSD	16669	3.9990	-7470A	PPB		04 Jun 2022 09:56:04	U	SMPL
N3167-02 - 1	BLUE-DRUM	-88	-0.0358	-7470A	PPB		04 Jun 2022 09:58:20	U	SMPL
N3178-02 - 1	2330-2332	0	-0.0146	-7470A	PPB		04 Jun 2022 10:00:35	U	SMPL
N3178-03 - 1	2342	11	-0.0120	-7470A	PPB		04 Jun 2022 10:02:51	U	SMPL
PB145288TB - 1	PB145253TB	-47	-0.0259	-7470A	PPB		04 Jun 2022 10:05:06	U	SMPL
PB145311TB - 1	PB145280TB	-40	-0.0242	-7470A	PPB		04 Jun 2022 10:07:22	U	SMPL
PB145290TB - 1	PB145290TB	-4	-0.0156	-7470A	PPB		04 Jun 2022 10:09:39	U	SMPL
PB145292TB - 1	PB145292TB	-19	-0.0192	-7470A	PPB		04 Jun 2022 10:11:56	U	SMPL
CCV30 - 1	CCV30	21282	5.1097	-7470A	PPB		04 Jun 2022 10:14:13	U	SMPL
CCB30 - 1	CCB30	-101	-0.0389	-7470A	PPB		04 Jun 2022 10:16:29	U	SMPL
N3143-05LX5 - 1		76	0.0037	-7470A	PPB		04 Jun 2022 10:40:54	U	SMPL
N3143-05A - 1		17968	4.3118	-7470A	PPB		04 Jun 2022 10:43:10	U	SMPL
N3154-02LX5 - 1		-28	-0.0214	-7470A	PPB		04 Jun 2022 10:45:26	U	SMPL
N3154-02A - 1		18348	4.4033	-7470A	PPB		04 Jun 2022 10:47:42	U	SMPL
N3170-05LX5 - 1		54	-0.0016	-7470A	PPB		04 Jun 2022 10:49:59	U	SMPL
N3170-05A - 1		17477	4.1935	-7470A	PPB		04 Jun 2022 10:52:15	U	SMPL
N3178-01LX5 - 1		130	0.0167	-7470A	PPB		04 Jun 2022 10:54:31	U	SMPL
N3178-01A - 1		17676	4.2415	-7470A	PPB		04 Jun 2022 10:56:48	U	SMPL
N3119-03LX5 - 1		-144	-0.0493	-7470A	PPB		04 Jun 2022 10:59:04	U	SMPL
N3119-03A - 1		17259	4.1410	-7470A	PPB		04 Jun 2022 11:01:21	U	SMPL
CCV31 - 1	CCV31	20609	4.9477	-7470A	PPB		04 Jun 2022 11:03:38	U	SMPL
CCB31 - 1	CCB31	-52	-0.0271	-7470A	PPB		04 Jun 2022 11:05:55	U	SMPL