


LB120500

7471B

INSTRUMENT ID: CV1

Linear

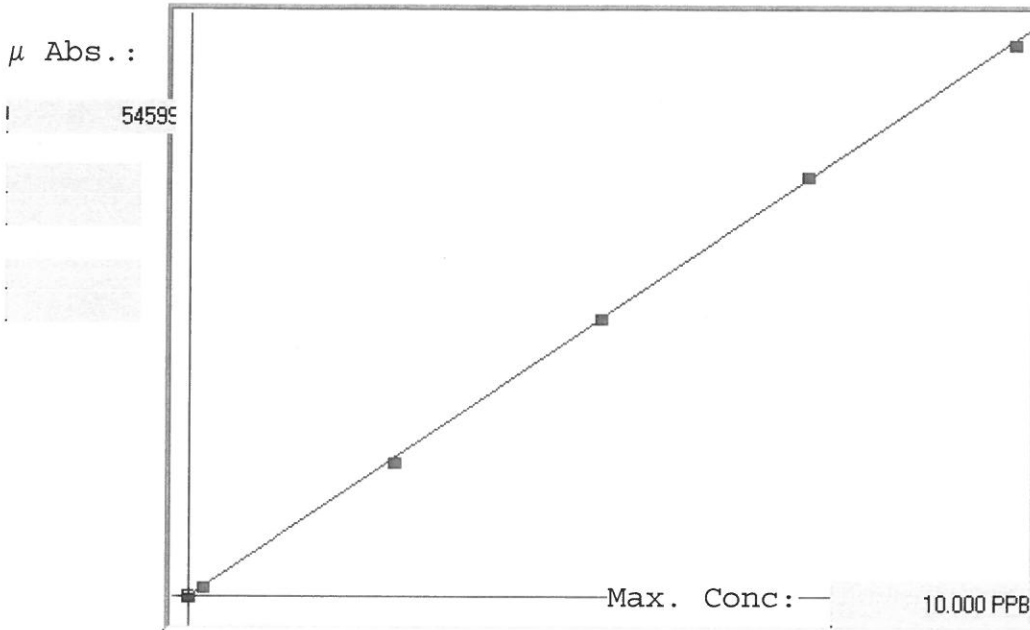

A= 0.0000e+000

B= 1.8186e-004

C= 2.0749e-002

Rho= 0.9999375

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	C/D
0.0	0.000	0.002	0.002	-102	0.000	-102					
0.2	0.200	0.209	0.009	1037	0.0 %	1037					4
2.5	2.500	2.447	-0.053	13342	0.0 %	13342					-2
5.0	5.000	5.026	0.026	27523	0.0 %	27523					1
7.5	7.500	7.565	0.065	41481	0.0 %	41481					1
10.0	10.000	9.950	-0.050	54599	0.0 %	54599					-1

LB120500 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 04 Jun 2022 11:51:52

Sample ID	Extended ID	μ Abs	Conc	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-102	-	0.00007471B	PPB	04 Jun 2022 12:16:24	S	Std
0.2 - 1	50.5	1037	-	0.20007471B	PPB	04 Jun 2022 12:18:42	S	Std
2.5 - 1	52.5	13342	-	2.50007471B	PPB	04 Jun 2022 12:20:59	S	Std
5.0 - 1	55	27523	-	5.00007471B	PPB	04 Jun 2022 12:23:16	S	Std
7.5 - 1	57.5	41481	-	7.50007471B	PPB	04 Jun 2022 12:25:33	S	Std
10.0 - 1	59	54599	-	10.00007471B	PPB	04 Jun 2022 12:27:51	S	Std
ICV60 - 1	ICV60	21786	3.9829	-7471B	PPB	04 Jun 2022 12:30:39	U	SMPL
ICB60 - 1	ICB60	-118	-0.0007	-7471B	PPB	04 Jun 2022 12:35:28	U	SMPL
CCV32 - 1	CCV32	28539	5.2110	-7471B	PPB	04 Jun 2022 12:37:42	U	SMPL
CCB32 - 1	CCB32	-204	-0.0164	-7471B	PPB	04 Jun 2022 12:39:57	U	SMPL
CRA - 1	CRA	1009	0.2043	-7471B	PPB	04 Jun 2022 12:42:14	U	SMPL
HighStd - 1	HighStd	54700	9.9687	-7471B	PPB	04 Jun 2022 12:44:28	U	SMPL
ChkStd - 1	ChkStd	39789	7.2570	-7471B	PPB	04 Jun 2022 12:46:44	U	SMPL
PB145334BL - 1	PBS	-108	0.0011	-7471B	PPB	04 Jun 2022 12:49:02	U	SMPL
PB145334BS - 1	LCSS	20221	3.6982	-7471B	PPB	04 Jun 2022 12:51:20	U	SMPL
N3143-01 - 1	20220392-SB-8-(DISCRETE-COMP-G)	7514	1.3873	-7471B	PPB	04 Jun 2022 12:53:37	U	SMPL
N3143-01DUP - 1	20220392-SB-8-(DISCRETE-COMP-G)DUP	8009	1.4773	-7471B	PPB	04 Jun 2022 12:55:53	U	SMPL
N3143-01MS - 1	20220392-SB-8-(DISCRETE-COMP-G)MS	29083	5.3099	-7471B	PPB	04 Jun 2022 12:58:11	U	SMPL
N3143-01MSD - 1	20220392-SB-8-(DISCRETE-COMP-G)MSD	29005	5.2957	-7471B	PPB	04 Jun 2022 13:00:27	U	SMPL
N3143-02 - 1	20220416-COMPOSITE-E	29630	5.4094	-7471B	PPB	04 Jun 2022 13:02:44	U	SMPL
CCV33 - 1	CCV33	28421	5.1895	-7471B	PPB	04 Jun 2022 13:05:02	U	SMPL
CCB33 - 1	CCB33	-94	0.0037	-7471B	PPB	04 Jun 2022 13:07:18	U	SMPL
N3143-03 - 1	20220425-AMENDED-COMP-E	31339	5.7202	-7471B	PPB	04 Jun 2022 13:09:35	U	SMPL
N3143-04 - 1	20220427-AMENDED-SB-8-(DISCRETE-COMP-G)	8120	1.4975	-7471B	PPB	04 Jun 2022 13:11:50	U	SMPL
N3158-01 - 1	OR-2-060122	5370	0.9974	-7471B	PPB	04 Jun 2022 13:14:08	U	SMPL
N3159-01 - 1	PT-1-060122	1308	0.2586	-7471B	PPB	04 Jun 2022 13:16:23	U	SMPL
N3168-01 - 1	HELENS-0602	3231	0.6084	-7471B	PPB	04 Jun 2022 13:18:39	U	SMPL
N3170-01 - 1	20220413-COMPOSITE-B	37003	6.7503	-7471B	PPB	04 Jun 2022 13:20:57	U	SMPL
N3170-02 - 1	20220415-COMPOSITE-D	27732	5.0642	-7471B	PPB	04 Jun 2022 13:23:13	U	SMPL
N3170-03 - 1	20220422-AMENDED-COMPOSITE-B	28266	5.1613	-7471B	PPB	04 Jun 2022 13:25:32	U	SMPL
N3170-04 - 1	20220424-AMENDED-COMPOSITE-D	24652	4.5041	-7471B	PPB	04 Jun 2022 13:27:51	U	SMPL
N3175-16 - 1	AUD-1714-17	21912	4.0058	-7471B	PPB	04 Jun 2022 13:30:08	U	SMPL
CCV34 - 1	CCV34	28891	5.2750	-7471B	PPB	04 Jun 2022 13:32:26	U	SMPL
CCB34 - 1	CCB34	-81	0.0060	-7471B	PPB	04 Jun 2022 13:34:42	U	SMPL
N3175-17 - 1	AUD-1718-21	1770	0.3426	-7471B	PPB	04 Jun 2022 13:36:59	U	SMPL
N3175-18 - 1	AUD-1722-25	378	0.0895	-7471B	PPB	04 Jun 2022 13:39:15	U	SMPL
N3175-19 - 1	AUD-1726-27	53423	9.7365	-7471B	PPB	04 Jun 2022 13:41:30	U	SMPL
N3179-01 - 1	TR-4-060222	1745	0.3381	-7471B	PPB	04 Jun 2022 13:43:45	U	SMPL
PB145337BL - 1	PBS	-10	0.0189	-7471B	PPB	04 Jun 2022 13:46:04	U	SMPL
PB145337BS - 1	LCSS	22168	4.0523	-7471B	PPB	04 Jun 2022 13:48:20	U	SMPL
N3176-01 - 1	NEWARK-SP	2808	0.5314	-7471B	PPB	04 Jun 2022 13:50:37	U	SMPL
N3186-01 - 1	2513-2514	4522	0.8431	-7471B	PPB	04 Jun 2022 13:52:54	U	SMPL
N3186-03 - 1	VNJ-218	6631	1.2267	-7471B	PPB	04 Jun 2022 13:55:11	U	SMPL
N3189-01 - 1	20220414-COMPOSITE-C	34665	6.3251	-7471B	PPB	04 Jun 2022 13:57:27	U	SMPL
CCV35 - 1	CCV35	28269	5.1619	-7471B	PPB	04 Jun 2022 14:00:00	U	SMPL
CCB35 - 1	CCB35	-216	-0.0185	-7471B	PPB	04 Jun 2022 14:02:17	U	SMPL
N3189-02 - 1	20220419-COMPOSITE-H	38928	7.1004	-7471B	PPB	04 Jun 2022 14:04:34	U	SMPL
N3189-03 - 1	20220423-AMENDED-COMPOSITE-C	25701	4.6949	-7471B	PPB	04 Jun 2022 14:06:50	U	SMPL
N3189-04 - 1	20220428-AMENDED-COMPOSITE-H	26356	4.8140	-7471B	PPB	04 Jun 2022 14:08:50	U	SMPL
N3197-01 - 1	SU-3-060322	2150	0.4118	-7471B	PPB	04 Jun 2022 14:11:08	U	SMPL
N3197-03 - 1	SU-4-060322	1764	0.3416	-7471B	PPB	04 Jun 2022 14:13:16	U	SMPL
N3197-03DUP - 1	SU-4-060322DUP	1684	0.3270	-7471B	PPB	04 Jun 2022 14:20:32	U	SMPL
N3197-03MS - 1	SU-4-060322MS	22909	4.1871	-7471B	PPB	04 Jun 2022 14:22:48	U	SMPL
N3197-03MSD - 1	SU-4-060322MSD	21644	3.9570	-7471B	PPB	04 Jun 2022 14:25:05	U	SMPL
N3201-01 - 1	11939	1344	0.2652	-7471B	PPB	04 Jun 2022 14:27:23	U	SMPL
N3201-03 - 1	21500	2380	0.4536	-7471B	PPB	04 Jun 2022 14:29:40	U	SMPL
CCV36 - 1	CCV36	28346	5.1759	-7471B	PPB	04 Jun 2022 14:31:56	U	SMPL
CCB36 - 1	CCB36	-179	-0.0118	-7471B	PPB	04 Jun 2022 14:34:11	U	SMPL
N3205-01 - 1	HR-02-060322	2488	0.4732	-7471B	PPB	04 Jun 2022 14:36:29	U	SMPL
N3206-01 - 1	CL-01-060322	3691	0.6920	-7471B	PPB	04 Jun 2022 14:38:46	U	SMPL
N3143-01LX5 - 1		1469	0.2879	-7471B	PPB	04 Jun 2022 14:41:01	U	SMPL
N3143-01A - 1		29264	5.3428	-7471B	PPB	04 Jun 2022 14:43:18	U	SMPL
N3197-03LX5 - 1		183	0.0540	-7471B	PPB	04 Jun 2022 14:45:33	U	SMPL
N3197-03A - 1		23692	4.3295	-7471B	PPB	04 Jun 2022 14:47:51	U	SMPL
CCV37 - 1	CCV37	28293	5.1662	-7471B	PPB	04 Jun 2022 14:50:07	U	SMPL
CCB37 - 1	CCB37	-187	-0.0133	-7471B	PPB	04 Jun 2022 14:52:25	U	SMPL