

L15120539

Result archive

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by :

12

Instrument ID : Konelab

6/7/2022 10:48

Sample id	Test id	Result	Status	Date	Errors
ICV1	Total CN	95.082	man acc	6/6/2022	
ICB1	Total CN	-0.037	man acc	6/6/2022	
CCV1	Total CN	243.980	man acc	6/6/2022	
CCB1	Total CN	-0.193	man acc	6/6/2022	
PB145364BL	Total CN	-0.450	man acc	6/6/2022	
N3028-04	Total CN	-0.642	man acc	6/6/2022	
N3028-04DUP	Total CN	-0.477	man acc	6/6/2022	
N3178-01	Total CN	-0.632	man acc	6/6/2022	
N3194-02	Total CN	-0.467	man acc	6/6/2022	
N3194-05	Total CN	-0.515	man acc	6/6/2022	
N3209-02	Total CN	-0.605	man acc	6/6/2022	
N3209-07	Total CN	-0.579	man acc	6/6/2022	
N3209-12	Total CN	-0.459	man acc	6/6/2022	
N3203-02	Total CN	-0.391	man acc	6/6/2022	
CCV2	Total CN	244.563	man acc	6/6/2022	
CCB2	Total CN	-0.105	man acc	6/6/2022	
PB145365BL	Total CN	-0.579	man acc	6/6/2022	
N3167-02	Total CN	-0.356	man acc	6/6/2022	
N3167-02DUP	Total CN	-0.446	man acc	6/6/2022	
N3178-02	Total CN	-0.463	man acc	6/6/2022	
N3178-03	Total CN	-0.270	man acc	6/6/2022	
N3215-01	Total CN	-0.458	man acc	6/6/2022	
CCV3	Total CN	247.645	man acc	6/6/2022	
CCB3	Total CN	-0.394	man acc	6/6/2022	

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 06 15:51:14 2022

Mon Jun 06 16:05:33 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.9047	µg/l	6/6/2022 14:19:07	
5.OPPBCN	A	Total CN	P	4.0979	µg/l	6/6/2022 14:19:08	
10PPBCN	A	Total CN	P	9.508	µg/l	6/6/2022 14:19:09	
50PPBCN	A	Total CN	P	50.1575	µg/l	6/6/2022 14:19:10	
100PPBCN	A	Total CN	P	99.9046	µg/l	6/6/2022 14:19:11	
250PPBCN	A	Total CN	P	254.429	µg/l	6/6/2022 14:19:12	
500PPBCN	A	Total CN	P	497.8076	µg/l	6/6/2022 14:19:13	
ICV1	S	Total CN	P	95.0819	µg/l	6/6/2022 15:51:14	
ICB1	S	Total CN	P	-0.0372	µg/l	6/6/2022 15:51:17	
CCV1	S	Total CN	P	243.9801	µg/l	6/6/2022 15:51:19	
CCB1	S	Total CN	P	-0.1934	µg/l	6/6/2022 15:51:20	
PB145364BL	S	Total CN	P	-0.4502	µg/l	6/6/2022 15:51:23	
N3028-04	S	Total CN	P	-0.6423	µg/l	6/6/2022 15:51:24	
N3028-04DUP	S	Total CN	P	-0.477	µg/l	6/6/2022 15:58:46	
N3178-01	S	Total CN	P	-0.6319	µg/l	6/6/2022 15:58:47	
N3194-02	S	Total CN	P	-0.4672	µg/l	6/6/2022 15:58:48	
N3194-05	S	Total CN	P	-0.5148	µg/l	6/6/2022 15:58:49	
N3209-02	S	Total CN	P	-0.6049	µg/l	6/6/2022 15:58:51	
N3209-07	S	Total CN	P	-0.5794	µg/l	6/6/2022 15:58:52	
N3209-12	S	Total CN	P	-0.4586	µg/l	6/6/2022 15:58:53	
N3203-02	S	Total CN	P	-0.3906	µg/l	6/6/2022 15:58:54	
CCV2	S	Total CN	P	244.5631	µg/l	6/6/2022 15:58:55	
CCB2	S	Total CN	P	-0.1048	µg/l	6/6/2022 15:58:56	
PB145365BL	S	Total CN	P	-0.5791	µg/l	6/6/2022 16:05:25	
N3167-02	S	Total CN	P	-0.3564	µg/l	6/6/2022 16:05:26	
N3167-02DUP	S	Total CN	P	-0.4457	µg/l	6/6/2022 16:05:27	
N3178-02	S	Total CN	P	-0.4629	µg/l	6/6/2022 16:05:28	
N3178-03	S	Total CN	P	-0.2704	µg/l	6/6/2022 16:05:29	
N3215-01	S	Total CN	P	-0.4576	µg/l	6/6/2022 16:05:30	
CCV3	S	Total CN	P	247.6446	µg/l	6/6/2022 16:05:32	
CCB3	S	Total CN	P	-0.3937	µg/l	6/6/2022 16:05:33	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *SM* Instrument ID : Konelab

6/6/2022 14:19


Test Total CN

Accepted 6/6/2022 14:19

Factor 1250
Bias 0.002

Coeff. of det. 0.999872

Errors

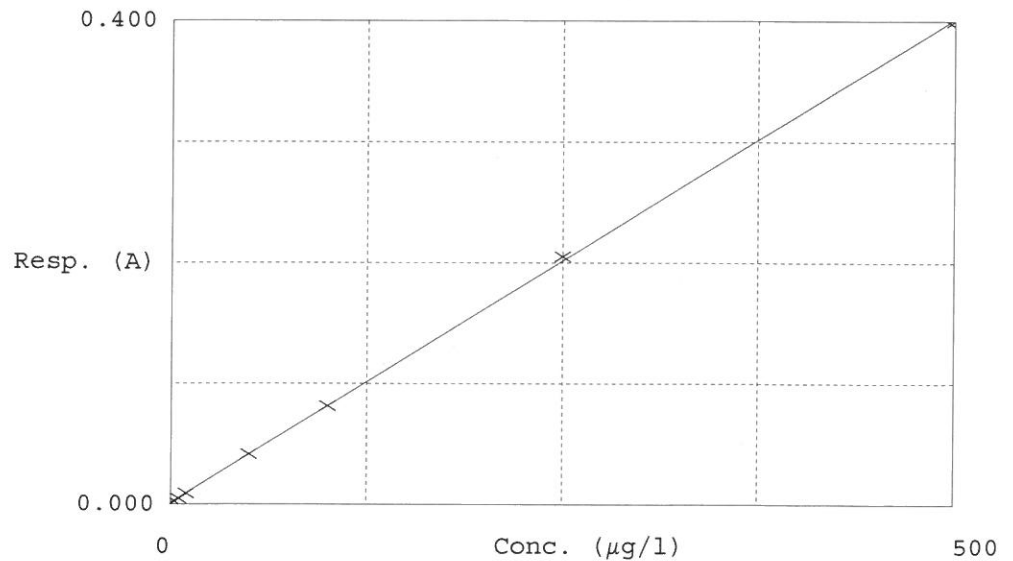

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.9047	0.0000	
2	5.0PPBCN	0.005	4.0979	5.0000	-18.0
3	10PPBCN	0.009	9.5080	10.0000	-4.9
4	50PPBCN	0.042	50.1575	50.0000	0.3
5	100PPBCN	0.082	99.9046	100.0000	-0.1
6	250PPBCN	0.205	254.4290	250.0000	1.8
7	500PPBCN	0.400	497.8076	500.0000	-0.4

Re
SM
6/6/22