

LB120542

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092Reviewed by : *SM*

Instrument ID : Konelab

6/7/2022 11:51

Test: Total CN

Sample Id	<i>M/L</i> Result	Dil. 1 +	Response	Errors
ICV1	94.393	0.0	0.078	
ICB1	0.301	0.0	0.002	
CCV1	243.482	0.0	0.198	
CCB1	0.071	0.0	0.002	
PB145351BL	-0.473	0.0	0.001	
PB145351BS	94.631	0.0	0.078	
MIDPB145351	241.140	0.0	0.196	
N3198-07	7.193	0.0	0.008	
N3198-07DUP	6.519	0.0	0.007	
N3198-07MS	45.549	0.0	0.038	
N3198-07MSD	45.484	0.0	0.038	
CCV2	245.719	0.0	0.199	
CCB2	-0.207	0.0	0.002	

96% (R0 - 118)

SM 6/7/22

N	13
Mean	78.754
SD	99.7015
CV%	126.60

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *SM* Instrument ID : Konelab

6/7/2022 10:26


Test Total CN

Accepted 6/7/2022 10:26

Factor 1243
Bias 0.002

Coeff. of det. 0.999898

Errors

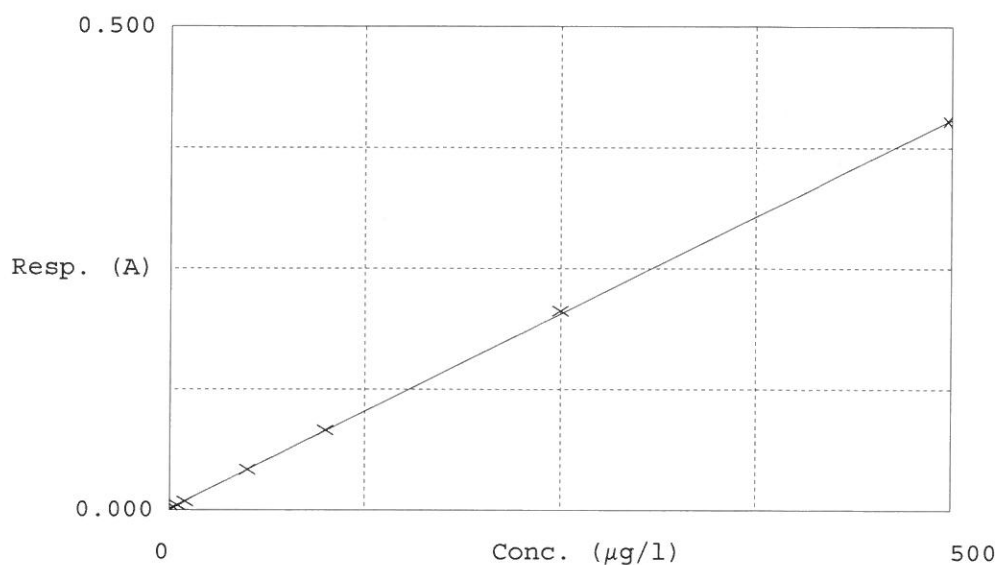

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.7020	0.0000	
2	5.0PPBCN	0.005	4.0573	5.0000	-23.3
3	10PPBCN	0.009	9.0612	10.0000	-9.9
4	50PPBCN	0.042	50.2263	50.0000	0.2
5	100PPBCN	0.083	100.5678	100.0000	1.6
6	250PPBCN	0.206	253.7948	250.0000	1.3
7	500PPBCN	0.402	497.9947	500.0000	-0.7

SM
6/7/22

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 07 09:51:50 2022

Tue Jun 07 11:46:49 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.702	µg/l	6/7/2022 10:15:31	
5.0PPBCN	A	Total CN	P	4.0573	µg/l	6/7/2022 10:15:32	
10PPBCN	A	Total CN	P	9.0612	µg/l	6/7/2022 10:15:33	
50PPBCN	A	Total CN	P	50.2263	µg/l	6/7/2022 10:15:34	
100PPBCN	A	Total CN	P	100.5678	µg/l	6/7/2022 10:15:35	
250PPBCN	A	Total CN	P	253.7948	µg/l	6/7/2022 10:15:36	
500PPBCN	A	Total CN	P	497.9947	µg/l	6/7/2022 10:15:37	
ICV1	S	Total CN	P	94.393	µg/l	6/7/2022 11:39:04	
ICB1	S	Total CN	P	0.3011	µg/l	6/7/2022 11:39:07	
CCV1	S	Total CN	P	243.4823	µg/l	6/7/2022 11:39:09	
CCB1	S	Total CN	P	0.0707	µg/l	6/7/2022 11:39:11	
PB145351BL	S	Total CN	P	-0.4725	µg/l	6/7/2022 11:39:12	
PB145351BS	S	Total CN	P	94.6314	µg/l	6/7/2022 11:46:39	
MIDPB145351	S	Total CN	P	241.1403	µg/l	6/7/2022 11:46:40	
N3198-07	S	Total CN	P	7.1929	µg/l	6/7/2022 11:46:42	
N3198-07DUP	S	Total CN	P	6.5195	µg/l	6/7/2022 11:46:43	
N3198-07MS	S	Total CN	P	45.5486	µg/l	6/7/2022 11:46:44	
N3198-07MSD	S	Total CN	P	45.484	µg/l	6/7/2022 11:46:45	
CCV2	S	Total CN	P	245.7191	µg/l	6/7/2022 11:46:48	
CCB2	S	Total CN	P	-0.2066	µg/l	6/7/2022 11:46:49	