

LB120546

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *YM*

Instrument ID : Konelab

6/7/2022 12:41

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.299	0.0	0.078	
ICB1	-0.396	0.0	0.001	
CCV1	243.212	0.0	0.197	
CCB1	-0.535	0.0	0.001	
PB145363BL	-0.702	0.0	0.001	
PB145363BS	95.025	0.0	0.078	
N3189-01	-1.036	0.0	0.001	
N3189-01DUP	-0.919	0.0	0.001	
N3189-01MS	37.096	0.0	0.032	
N3189-01MSD	38.177	0.0	0.032	
N3189-02	-0.698	0.0	0.001	
N3189-03	-0.565	0.0	0.001	
N3189-04	0.764	0.0	0.002	
CCV2	241.898	0.0	0.196	
CCB2	-0.707	0.0	0.001	

N	15
Mean	49.661
SD	85.1192
CV%	171.40

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *SM* Instrument ID : Konelab

6/7/2022 10:26


Test Total CN

Accepted 6/7/2022 10:26

Factor 1243
Bias 0.002

Coeff. of det. 0.999898

Errors

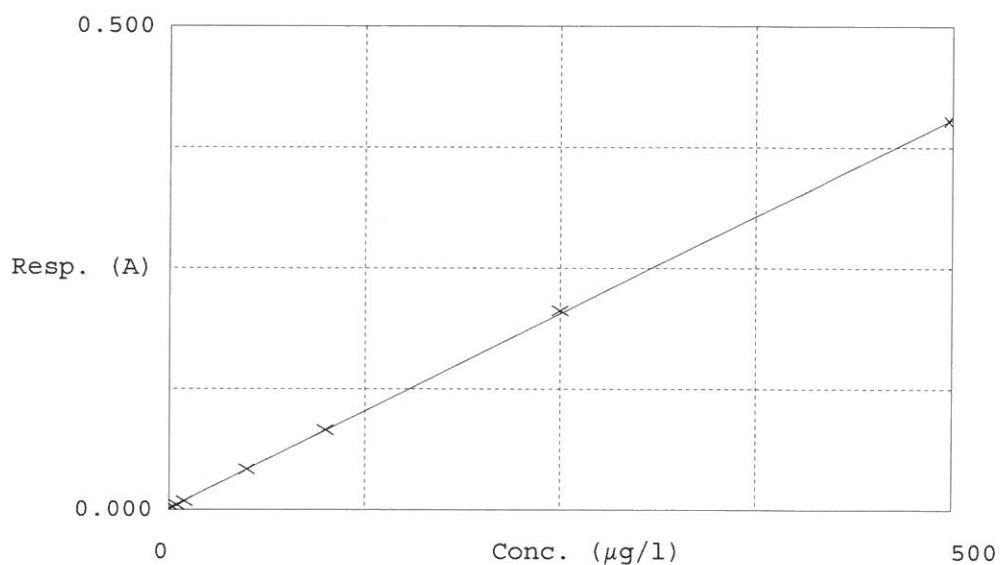

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.7020	0.0000	-23.3
2	5.0PPBCN	0.005	4.0573	5.0000	-9.9
3	10PPBCN	0.009	9.0612	10.0000	0.2
4	50PPBCN	0.042	50.2263	50.0000	1.6
5	100PPBCN	0.083	100.5678	100.0000	1.3
6	250PPBCN	0.206	253.7948	250.0000	-0.7
7	500PPBCN	0.402	497.9947	500.0000	

SM
6/7/22

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 07 12:21:18 2022

Tue Jun 07 12:31:41 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
ICV1	S	Total CN	P	94.2986	µg/l	6/7/2022 12:21:18	
ICB1	S	Total CN	P	-0.3955	µg/l	6/7/2022 12:21:21	
CCV1	S	Total CN	P	243.2115	µg/l	6/7/2022 12:21:23	
CCB1	S	Total CN	P	-0.5347	µg/l	6/7/2022 12:21:25	
PB145363BL	S	Total CN	P	-0.7024	µg/l	6/7/2022 12:21:26	
PB145363BS	S	Total CN	P	95.0252	µg/l	6/7/2022 12:28:53	
N3189-01	S	Total CN	P	-1.0356	µg/l	6/7/2022 12:28:54	
N3189-01DUP	S	Total CN	P	-0.9185	µg/l	6/7/2022 12:28:55	
N3189-01MS	S	Total CN	P	37.0957	µg/l	6/7/2022 12:28:58	
N3189-01MSD	S	Total CN	P	38.1774	µg/l	6/7/2022 12:28:59	
N3189-02	S	Total CN	P	-0.6983	µg/l	6/7/2022 12:29:00	
N3189-03	S	Total CN	P	-0.5646	µg/l	6/7/2022 12:29:01	
N3189-04	S	Total CN	P	0.7642	µg/l	6/7/2022 12:29:02	
CCV2	S	Total CN	P	241.8982	µg/l	6/7/2022 12:29:03	
CCB2	S	Total CN	P	-0.7068	µg/l	6/7/2022 12:31:41	