


LB 120722 Instrument ID : CV1

7470A

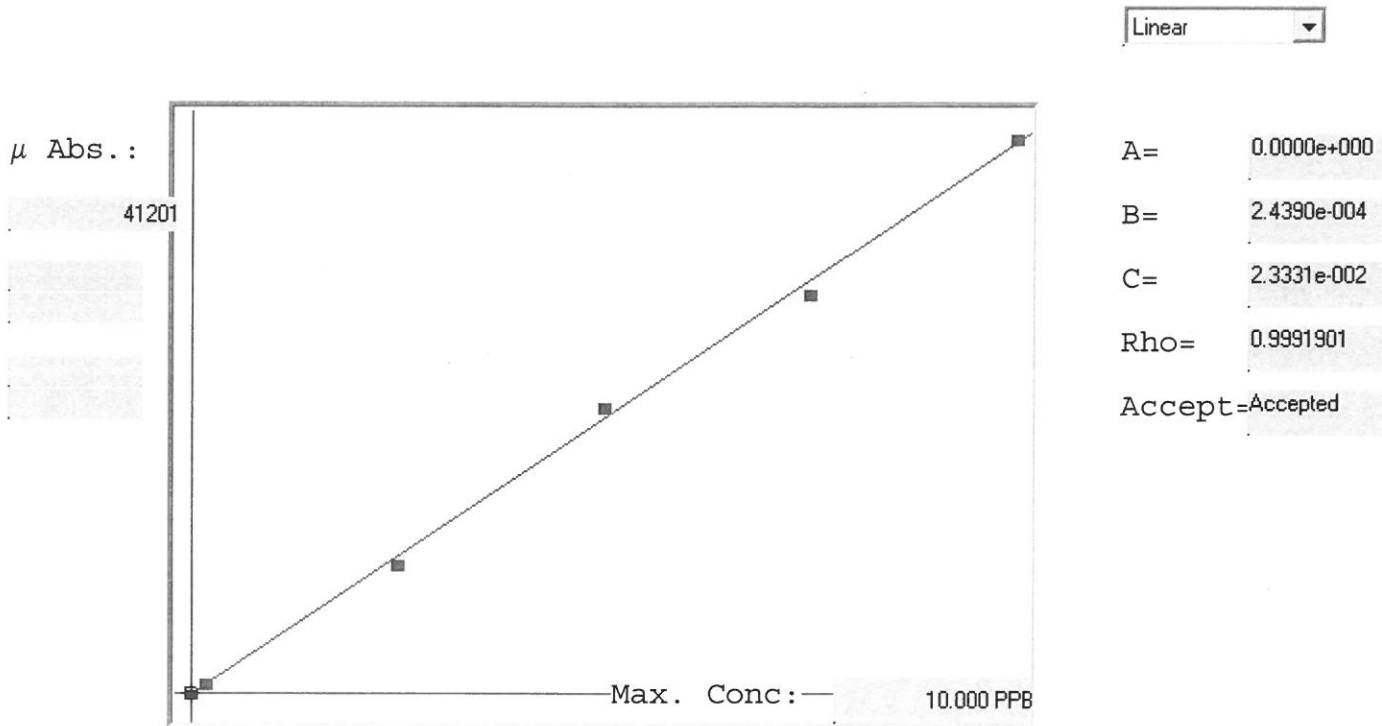

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.048	0.048	100	0.000	100				
0.2	0.200	0.210	0.010	766	0.0 %	766				
2.5	2.500	2.359	-0.141	9577	0.0 %	9577				
5.0	5.000	5.234	0.234	21364	0.0 %	21364				
7.5	7.500	7.276	-0.224	29737	0.0 %	29737				
10.0	10.000	10.072	0.072	41201	0.0 %	41201				

LB120722 Instrument ID: CV1

Method: 7470A		Operator: Admin		Date of Analysis: 14 Jun 2022 16:34:08					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD.0	100	-	0.0000	7470A	PPB	16 Jun 2022 16:46:16	S	Std
0.2 - 1	SD.2	766	-	0.2000	7470A	PPB	16 Jun 2022 16:48:33	S	Std
2.5 - 1	SD.5	9577	-	2.5000	7470A	PPB	16 Jun 2022 16:50:50	S	Std
5.0 - 1	SD.0	21364	-	5.0000	7470A	PPB	16 Jun 2022 16:53:07	S	Std
7.5 - 1	SD.5	29737	-	7.5000	7470A	PPB	16 Jun 2022 16:55:24	S	Std
10.0 - 1	SD.0	41201	-	10.0000	7470A	PPB	16 Jun 2022 16:57:43	S	Std
ICV78 - 1	ICV78	16617	4.0763	-	7470A	PPB	16 Jun 2022 17:17:01	U	SMPL
ICB78 - 1	ICB78	331	0.1041	-	7470A	PPB	16 Jun 2022 17:19:16	U	SMPL
CCV120 - 1	CCV120	21306	5.2200	-	7470A	PPB	16 Jun 2022 17:21:32	U	SMPL
CRA - 1	CRA	777	0.2128	-	7470A	PPB	16 Jun 2022 17:26:03	U	SMPL
CCB120 - 1	CCB120	364	0.1121	-	7470A	PPB	16 Jun 2022 17:23:47	U	SMPL
HighStd - 1	HighStd	40978	10.0181	-	7470A	PPB	16 Jun 2022 17:28:20	U	SMPL
ChkStd - 1	ChkStd	28236	6.9102	-	7470A	PPB	16 Jun 2022 17:30:41	U	SMPL
PB145597BL - 1	PBW	293	0.0948	-	7470A	PPB	16 Jun 2022 17:32:59	U	SMPL
PB145597BS - 1	LCSW	16348	4.0107	-	7470A	PPB	16 Jun 2022 17:35:17	U	SMPL
N3363-01 - 1	NWB-1801	287	0.0933	-	7470A	PPB	16 Jun 2022 17:37:34	U	SMPL
N3363-01DUP - 1	NWB-1801DUP	382	0.1165	-	7470A	PPB	16 Jun 2022 17:39:52	U	SMPL
N3363-01MS - 1	NWB-1801MS	15589	3.8256	-	7470A	PPB	16 Jun 2022 17:42:09	U	SMPL
N3363-01MSD - 1	NWB-1801MSD	15128	3.7131	-	7470A	PPB	16 Jun 2022 17:44:26	U	SMPL
N3363-03 - 1	NWB-1802	247	0.0836	-	7470A	PPB	16 Jun 2022 17:46:41	U	SMPL
CCV121 - 1	CCV121	21202	5.1946	-	7470A	PPB	16 Jun 2022 17:48:58	U	SMPL
CCB121 - 1	CCB121	-14	0.0199	-	7470A	PPB	16 Jun 2022 17:51:14	U	SMPL
PB145598BL - 1	PBW	85	0.0441	-	7470A	PPB	16 Jun 2022 17:53:30	U	SMPL
PB145598BS - 1	LCSW	16304	4.0000	-	7470A	PPB	16 Jun 2022 17:55:46	U	SMPL
N3314-01 - 1	ER-HEATER-COMP	240	0.0819	-	7470A	PPB	16 Jun 2022 17:58:01	U	SMPL
N3314-01DUP - 1	ER-HEATER-COMPDUP	310	0.0989	-	7470A	PPB	16 Jun 2022 18:00:17	U	SMPL
N3314-01MS - 1	ER-HEATER-COMPMS	15782	3.8726	-	7470A	PPB	16 Jun 2022 18:02:33	U	SMPL
N3314-01MSD - 1	ER-HEATER-COMPMSD	15928	3.9082	-	7470A	PPB	16 Jun 2022 18:04:50	U	SMPL
N3363-01LX5 - 1		51	0.0358	-	7470A	PPB	16 Jun 2022 18:07:07	U	SMPL
N3363-01A - 1		15152	3.7190	-	7470A	PPB	16 Jun 2022 18:09:24	U	SMPL
N3314-01A - 1		15721	3.8578	-	7470A	PPB	16 Jun 2022 18:13:59	U	SMPL
CCV122 - 1	CCV122	18803	4.6095	-	7470A	PPB	16 Jun 2022 18:16:15	U	SMPL
CCB122 - 1	CCB122	249	0.0841	-	7470A	PPB	16 Jun 2022 18:18:30	U	SMPL
PB145565TB - 1		236	0.0809	-	7470A	PPB	16 Jun 2022 18:20:46	U	SMPL
PB145577TB - 1		263	0.0875	-	7470A	PPB	16 Jun 2022 18:23:01	U	SMPL
N3314-01LX5 - 1		190	0.0697	-	7470A	PPB	16 Jun 2022 18:28:01	U	SMPL
CCV123 - 1	CCV123	20954	5.1341	-	7470A	PPB	16 Jun 2022 18:30:16	U	SMPL
CCB123 - 1	CCB123	215	0.0758	-	7470A	PPB	16 Jun 2022 18:32:32	U	SMPL