


LB120820

7470A

INSTRUMENT ID: CV2

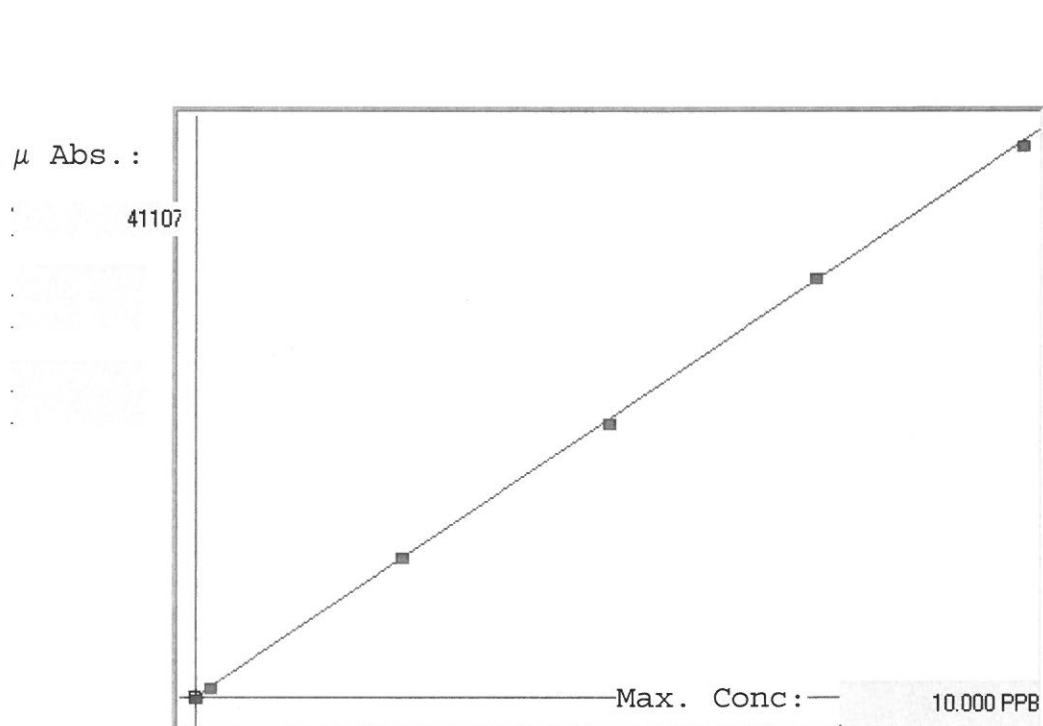

Linear

A= 0.0000e+000

B= 2.4206e-004

C= 5.5895e-003

Rho= 0.9999261

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.001	-0.001	-29	0.000	-29					-1)
0.2	0.200	0.179	-0.021	716	0.0 %	716					-1)
2.5	2.500	2.537	0.037	10459	0.0 %	10459					-1)
5.0	5.000	4.952	-0.048	20435	0.0 %	20435					-1)
7.5	7.500	7.577	0.077	31281	0.0 %	31281					-1)
10.0	10.000	9.956	-0.044	41107	0.0 %	41107					0

LB120820 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 Jun 2022 13:10:44

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-29	-	0.0000	7470A	PPB	24 Jun 2022 13:14:28	S	Std
0.2 - 1	50.2	716	-	0.2000	7470A	PPB	24 Jun 2022 13:16:45	S	Std
2.5 - 1	52.5	10459	-	2.5000	7470A	PPB	24 Jun 2022 13:19:02	S	Std
5.0 - 1	55	20435	-	5.0000	7470A	PPB	24 Jun 2022 13:21:19	S	Std
7.5 - 1	57.5	31281	-	7.5000	7470A	PPB	24 Jun 2022 13:23:36	S	Std
10.0 - 1	510	41107	-	10.0000	7470A	PPB	24 Jun 2022 13:25:52	S	Std
ICV10 - 1	ICV10	16075	3.8967	-	7470A	PPB	24 Jun 2022 13:28:48	U	SMPL
ICB10 - 1	ICB10	-88	-0.0157	-	7470A	PPB	24 Jun 2022 13:31:03	U	SMPL
CCV35 - 1	CCV35	20487	4.9646	-	7470A	PPB	24 Jun 2022 13:33:19	U	SMPL
CCB35 - 1	CCB35	-92	-0.0167	-	7470A	PPB	24 Jun 2022 13:35:34	U	SMPL
CRA - 1	CRA	653	0.1637	-	7470A	PPB	24 Jun 2022 13:37:50	U	SMPL
HighStd - 1	HighStd	40618	9.8375	-	7470A	PPB	24 Jun 2022 13:40:05	U	SMPL
ChkStd - 1	ChkStd	28776	6.9710	-	7470A	PPB	24 Jun 2022 13:42:20	U	SMPL
PB145756BL - 1	PBW	-130	-0.0259	-	7470A	PPB	24 Jun 2022 13:44:38	U	SMPL
PB145756BS - 1	LCSW	15539	3.7669	-	7470A	PPB	24 Jun 2022 13:46:55	U	SMPL
N3340-06 - 1	CS-1	6466	1.5707	-	7470A	PPB	24 Jun 2022 13:49:11	U	SMPL
N3340-06DUP - 1	CS-1DUP	6295	1.5293	-	7470A	PPB	24 Jun 2022 13:51:27	U	SMPL
N3340-06MS - 1	CS-1MS	21742	5.2684	-	7470A	PPB	24 Jun 2022 13:53:45	U	SMPL
N3340-06MSD - 1	CS-1MSD	21594	5.2326	-	7470A	PPB	24 Jun 2022 13:56:01	U	SMPL
PB145814BL - 1	PBW	-84	-0.0147	-	7470A	PPB	24 Jun 2022 13:58:18	U	SMPL
CCV36 - 1	CCV36	20387	4.9404	-	7470A	PPB	24 Jun 2022 14:00:33	U	SMPL
CCB36 - 1	CCB36	-65	-0.0101	-	7470A	PPB	24 Jun 2022 14:02:50	U	SMPL
PB145814BS - 1	LCSW	14702	3.5643	-	7470A	PPB	24 Jun 2022 14:05:05	U	SMPL
N3429-01 - 1	DRUM-1	278	0.0729	-	7470A	PPB	24 Jun 2022 14:07:20	U	SMPL
N3429-01DUP - 1	DRUM-1DUP	334	0.0864	-	7470A	PPB	24 Jun 2022 14:09:36	U	SMPL
N3429-01MS - 1	DRUM-1MS	15645	3.7926	-	7470A	PPB	24 Jun 2022 14:11:52	U	SMPL
N3429-01MSD - 1	DRUM-1MSD	15493	3.7558	-	7470A	PPB	24 Jun 2022 14:14:08	U	SMPL
N3436-01 - 1	31677	-87	-0.0155	-	7470A	PPB	24 Jun 2022 14:16:24	U	SMPL
N3447-02 - 1	D2342	-11	0.0029	-	7470A	PPB	24 Jun 2022 14:18:41	U	SMPL
N3447-03 - 1	D2345	39	0.0150	-	7470A	PPB	24 Jun 2022 14:20:57	U	SMPL
PB145815BL - 1	PBW	-23	0.0000	-	7470A	PPB	24 Jun 2022 14:23:14	U	SMPL
PB145815BS - 1	LCSW	15180	3.6800	-	7470A	PPB	24 Jun 2022 14:25:30	U	SMPL
CCV37 - 1	CCV37	20592	4.9900	-	7470A	PPB	24 Jun 2022 14:27:46	U	SMPL
CCB37 - 1	CCB37	-91	-0.0164	-	7470A	PPB	24 Jun 2022 14:30:01	U	SMPL
N3431-02 - 1	WC-14B-2-2	-9	0.0034	-	7470A	PPB	24 Jun 2022 14:32:17	U	SMPL
N3431-02DUP - 1	WC-14B-2-2DUP	7	0.0073	-	7470A	PPB	24 Jun 2022 14:34:32	U	SMPL
N3431-02MS - 1	WC-14B-2-2MS	14165	3.4343	-	7470A	PPB	24 Jun 2022 14:36:47	U	SMPL
N3431-02MSD - 1	WC-14B-2-2MSD	14473	3.5089	-	7470A	PPB	24 Jun 2022 14:39:03	U	SMPL
N3431-08 - 1	WC-14B-2-3	-38	-0.0036	-	7470A	PPB	24 Jun 2022 14:41:18	U	SMPL
N3431-14 - 1	WC-14B-2-4	8	0.0075	-	7470A	PPB	24 Jun 2022 14:43:35	U	SMPL
N3431-20 - 1	WC-14B-2-5	60	0.0201	-	7470A	PPB	24 Jun 2022 14:45:51	U	SMPL
N3447-01 - 1	D2356	-37	-0.0034	-	7470A	PPB	24 Jun 2022 14:48:08	U	SMPL
PB145816BL - 1	PBW	-35	-0.0029	-	7470A	PPB	24 Jun 2022 14:50:25	U	SMPL
PB145816BS - 1	LCSW	15164	3.6761	-	7470A	PPB	24 Jun 2022 14:52:41	U	SMPL
CCV38 - 1	CCV38	20989	5.0861	-	7470A	PPB	24 Jun 2022 14:54:56	U	SMPL
CCB38 - 1	CCB38	-94	-0.0172	-	7470A	PPB	24 Jun 2022 14:57:11	U	SMPL
N3438-01 - 1	FRAC-TANK-N47935	184	0.0501	-	7470A	PPB	24 Jun 2022 14:59:27	U	SMPL
N3471-15 - 1	COMP1-WATER	1832	0.4490	-	7470A	PPB	24 Jun 2022 15:01:42	U	SMPL
N3471-15DUP - 1	COMP1-WATERDUP	1638	0.4021	-	7470A	PPB	24 Jun 2022 15:03:58	U	SMPL
N3471-15MS - 1	COMP1-WATERMS	13524	3.2792	-	7470A	PPB	24 Jun 2022 15:06:13	U	SMPL
N3471-15MSD - 1	COMP1-WATERMSD	13451	3.2615	-	7470A	PPB	24 Jun 2022 15:08:29	U	SMPL
N3471-16 - 1	COMP2-WATER	2740	0.6688	-	7470A	PPB	24 Jun 2022 15:10:47	U	SMPL
N3471-17 - 1	COMP3-WATER	12180	2.9538	-	7470A	PPB	24 Jun 2022 15:13:04	U	SMPL
N3476-02 - 1	52422	-96	-0.0176	-	7470A	PPB	24 Jun 2022 15:15:21	U	SMPL
N3476-04 - 1	31535-WATER	4804	1.1684	-	7470A	PPB	24 Jun 2022 15:17:38	U	SMPL
PB145756TB - 1	P3145736TB	-59	-0.0087	-	7470A	PPB	24 Jun 2022 15:19:53	U	SMPL
CCV39 - 1	CCV39	19786	4.7949	-	7470A	PPB	24 Jun 2022 15:22:09	U	SMPL
CCB39 - 1	CCB39	-69	-0.0111	-	7470A	PPB	24 Jun 2022 15:24:25	U	SMPL
PB145765TB - 1	PB145765TB	-39	-0.0039	-	7470A	PPB	24 Jun 2022 15:26:41	U	SMPL
N3340-06LX5 - 1		1308	0.3222	-	7470A	PPB	24 Jun 2022 15:28:57	U	SMPL
N3340-06A - 1		22571	5.4691	-	7470A	PPB	24 Jun 2022 15:31:12	U	SMPL
N3429-01LX5 - 1		-70	-0.0114	-	7470A	PPB	24 Jun 2022 15:33:28	U	SMPL
N3429-01A - 1		16372	3.9686	-	7470A	PPB	24 Jun 2022 15:35:44	U	SMPL
N3431-02LX5 - 1		-121	-0.0237	-	7470A	PPB	24 Jun 2022 15:38:00	U	SMPL
N3431-02A - 1		16662	4.0387	-	7470A	PPB	24 Jun 2022 15:40:16	U	SMPL
N3471-15LX5 - 1		260	0.0685	-	7470A	PPB	24 Jun 2022 15:42:33	U	SMPL
N3471-15A - 1		17507	4.2433	-	7470A	PPB	24 Jun 2022 15:44:50	U	SMPL
CCV40 - 1	CCV40	20602	4.9925	-	7470A	PPB	24 Jun 2022 15:47:07	U	SMPL
CCB40 - 1	CCB40	-37	-0.0034	-	7470A	PPB	24 Jun 2022 15:49:22	U	SMPL