


LB120866

7471B

INSTRUMENT ID: CV1

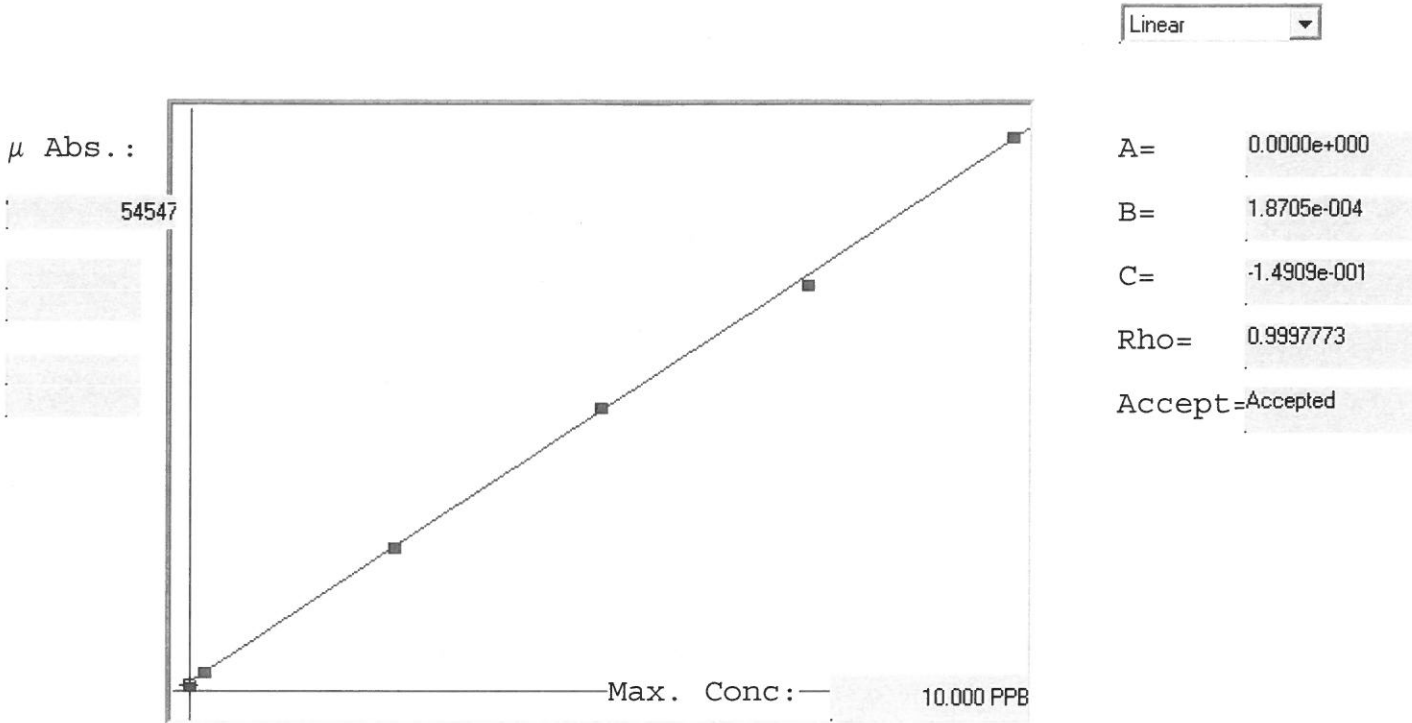

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	-0.030	-0.030	637	0.000	637					5
0.2	0.200	0.210	0.010	1919	0.0 %	1919					1
2.5	2.500	2.515	0.015	14240	0.0 %	14240					2
5.0	5.000	5.100	0.100	28065	0.0 %	28065					2
7.5	7.500	7.351	-0.149	40097	0.0 %	40097					-2
10.0	10.000	10.054	0.054	54547	0.0 %	54547					1

LB120866 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 28 Jun 2022 14:18:17				
Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	637	-	0.00007471B	PPB	28 Jun 2022 14:19:13	S	Std
0.2 - 1	50.2	1919	-	0.20007471B	PPB	28 Jun 2022 14:21:30	S	Std
2.5 - 1	52.5	14240	-	2.50007471B	PPB	28 Jun 2022 14:23:47	S	Std
5.0 - 1	55	28065	-	5.00007471B	PPB	28 Jun 2022 14:26:04	S	Std
7.5 - 1	57.5	40097	-	7.50007471B	PPB	28 Jun 2022 14:28:21	S	Std
10.0 - 1	510	54547	-	10.00007471B	PPB	28 Jun 2022 14:30:39	S	Std
ICV14 - 1	ICV14	22668	4.0910	-7471B	PPB	28 Jun 2022 14:33:20	U	SMPL
ICB14 - 1	ICB14	647	-0.0281	-7471B	PPB	28 Jun 2022 14:35:35	U	SMPL
CCV52 - 1	CCV52	28090	5.1052	-7471B	PPB	28 Jun 2022 14:37:52	U	SMPL
CCB52 - 1	CCB52	721	-0.0142	-7471B	PPB	28 Jun 2022 14:40:08	U	SMPL
CRA - 1	CRA	1940	0.2138	-7471B	PPB	28 Jun 2022 14:42:25	U	SMPL
HighStd - 1	HighStd	55450	10.2229	-7471B	PPB	28 Jun 2022 14:44:40	U	SMPL
ChkStd - 1	ChkStd	38112	6.9798	-7471B	PPB	28 Jun 2022 14:46:56	U	SMPL
PB145904BL - 1	PBS	932	0.0252	-7471B	PPB	28 Jun 2022 14:49:14	U	SMPL
PB145904BS - 1	LCSS	23705	4.2850	-7471B	PPB	28 Jun 2022 14:51:32	U	SMPL
N3462-01 - 1	SB-8-0-2-20220622	1747	0.1777	-7471B	PPB	28 Jun 2022 14:53:49	U	SMPL
N3462-02 - 1	SB-8-7-9-20220622	1239	0.0827	-7471B	PPB	28 Jun 2022 14:56:07	U	SMPL
N3462-04 - 1	SB-6-0-2-20220622	1106	0.0578	-7471B	PPB	28 Jun 2022 14:58:24	U	SMPL
N3462-05 - 1	SB-6-4-6-20220622	9800	1.6840	-7471B	PPB	28 Jun 2022 15:00:41	U	SMPL
N3462-07 - 1	SB-2-0-2-20220622	25226	4.5695	-7471B	PPB	28 Jun 2022 15:02:57	U	SMPL
CCV53 - 1	CCV53	28131	5.1128	-7471B	PPB	28 Jun 2022 15:05:12	U	SMPL
CCB53 - 1	CCB53	697	-0.0187	-7471B	PPB	28 Jun 2022 15:07:28	U	SMPL
N3462-08 - 1	SB-2-3-5-20220622	524	-0.0511	-7471B	PPB	28 Jun 2022 15:09:45	U	SMPL
N3476-01 - 1	31535-SLUDGE	26228	4.7569	-7471B	PPB	28 Jun 2022 15:12:00	U	SMPL
N3478-02 - 1	RO-364	1490	0.1296	-7471B	PPB	28 Jun 2022 15:14:16	U	SMPL
N3478-02DUP - 1	RO-364DUP	1737	0.1758	-7471B	PPB	28 Jun 2022 15:16:34	U	SMPL
N3478-02MS - 1	RO-364MS	26513	4.8102	-7471B	PPB	28 Jun 2022 15:18:50	U	SMPL
N3478-02MSD - 1	RO-364MSD	25563	4.6325	-7471B	PPB	28 Jun 2022 15:24:41	U	SMPL
N3488-01 - 1	SB-9-0-2-20220623	7494	1.2527	-7471B	PPB	28 Jun 2022 15:26:57	U	SMPL
N3488-02 - 1	SB-9-8.5-10.5-20220623	11023	1.9128	-7471B	PPB	28 Jun 2022 15:29:14	U	SMPL
N3488-04 - 1	SB-10-0-2-20220623	19293	3.4597	-7471B	PPB	28 Jun 2022 15:31:31	U	SMPL
N3488-06 - 1	SB-11-0-2-20220623	10833	1.8772	-7471B	PPB	28 Jun 2022 15:33:46	U	SMPL
CCV54 - 1	CCV54	28409	5.1648	-7471B	PPB	28 Jun 2022 15:36:02	U	SMPL
CCB54 - 1	CCB54	719	-0.0146	-7471B	PPB	28 Jun 2022 15:38:17	U	SMPL
N3488-08 - 1	SB-12-0-2-20220623	11994	2.0944	-7471B	PPB	28 Jun 2022 15:40:34	U	SMPL
N3488-09 - 1	SB-12-3-5-20220623	9225	1.5765	-7471B	PPB	28 Jun 2022 15:42:50	U	SMPL
N3488-11 - 1	SB-7-0-2-20220623	22753	4.1069	-7471B	PPB	28 Jun 2022 15:45:05	U	SMPL
N3488-13 - 1	SB-13-0-2-20220623	3506	0.5067	-7471B	PPB	28 Jun 2022 15:47:20	U	SMPL
N3488-15 - 1	SB-14-0-2-20220623	12144	2.1225	-7471B	PPB	28 Jun 2022 15:49:37	U	SMPL
N3478-02LX5 - 1		231	-0.1059	-7471B	PPB	28 Jun 2022 15:51:54	U	SMPL
N3478-02A - 1		23732	4.2900	-7471B	PPB	28 Jun 2022 15:54:10	U	SMPL
CCV55 - 1	CCV55	28457	5.1738	-7471B	PPB	28 Jun 2022 15:56:27	U	SMPL
CCB55 - 1	CCB55	765	-0.0060	-7471B	PPB	28 Jun 2022 15:58:46	U	SMPL