

LB120874

Test results Aquakem 7.2AQ1 Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

6/28/2022 16:15 Reviewed by : *GM* Instrument ID : Konelab

Test: Total CN

Sample Id	<i>my/k</i> Result	Dil. 1 +	Response	Errors
ICV1	95.233	0.0	0.083	
ICB1	0.368	0.0	0.001	
CCV1	249.611	0.0	0.217	
CCB1	0.270	0.0	0.001	
PB145909BL	0.199	0.0	0.001	
N3472-06	0.186	0.0	0.001	
N3472-06DUP	0.366	0.0	0.001	
CCV2	253.284	0.0	0.220	
CCB2	0.334	0.0	0.001	

N 9
Mean 66.650
SD 109.2865
CV% 163.97

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 28 16:13:07 2022

Tue Jun 28 16:13:15 2022


Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.2136	µg/l	6/28/2022 10:30:31	
5.OPPBCN	A	Total CN	P	4.6121	µg/l	6/28/2022 10:30:32	
10PPBCN	A	Total CN	P	9.5108	µg/l	6/28/2022 10:30:33	
50PPBCN	A	Total CN	P	49.8419	µg/l	6/28/2022 10:30:34	
100PPBCN	A	Total CN	P	100.7889	µg/l	6/28/2022 10:30:35	
250PPBCN	A	Total CN	P	250.3221	µg/l	6/28/2022 10:30:36	
500PPBCN	A	Total CN	P	499.7107	µg/l	6/28/2022 10:30:37	
ICV1	S	Total CN	P	95.2334	µg/l	6/28/2022 16:13:07	
ICB1	S	Total CN	P	0.3676	µg/l	6/28/2022 16:13:08	
CCV1	S	Total CN	P	249.6107	µg/l	6/28/2022 16:13:09	
CCB1	S	Total CN	P	0.2699	µg/l	6/28/2022 16:13:10	
PB145909BL	S	Total CN	P	0.1991	µg/l	6/28/2022 16:13:11	
N3472-06	S	Total CN	P	0.1862	µg/l	6/28/2022 16:13:12	
N3472-06DUP	S	Total CN	P	0.3655	µg/l	6/28/2022 16:13:13	
CCV2	S	Total CN	P	253.2843	µg/l	6/28/2022 16:13:14	
CCB2	S	Total CN	P	0.3337	µg/l	6/28/2022 16:13:15	

Reviewed by : SM Instrument ID : Konelab

Test	Total	CN
------	-------	----

Factor	1154
Bias	0.001

Errors

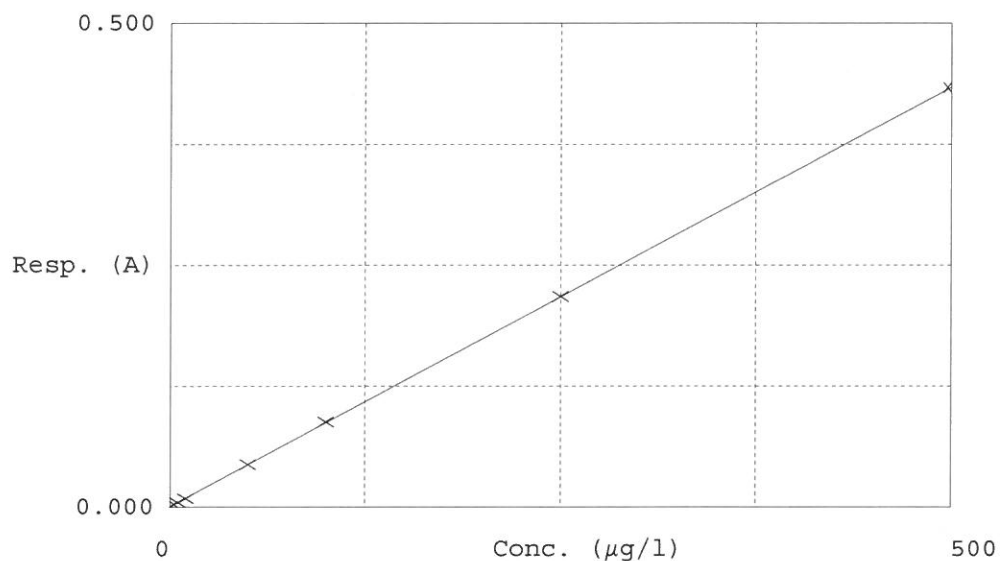

	Calibrator	Response	Calc. con.	Conc.	^{pc} Errors
1	0.0PPBCN	0.001	0.2136	0.0000	—
2	5.0PPBCN	0.005	4.6121	5.0000	-23.3
3	10PPBCN	0.009	9.5108	10.0000	-9.5
4	50PPBCN	0.044	49.8419	50.0000	0.2
5	100PPBCN	0.088	100.7889	100.0000	1.6
6	250PPBCN	0.218	250.3221	250.0000	1.3
7	500PPBCN	0.434	499.7107	500.0000	0.4

8 a1
6/28/22