

63120821


7470A

INSTRUMENT ID: CV2

Linear

μ Abs.:

41729

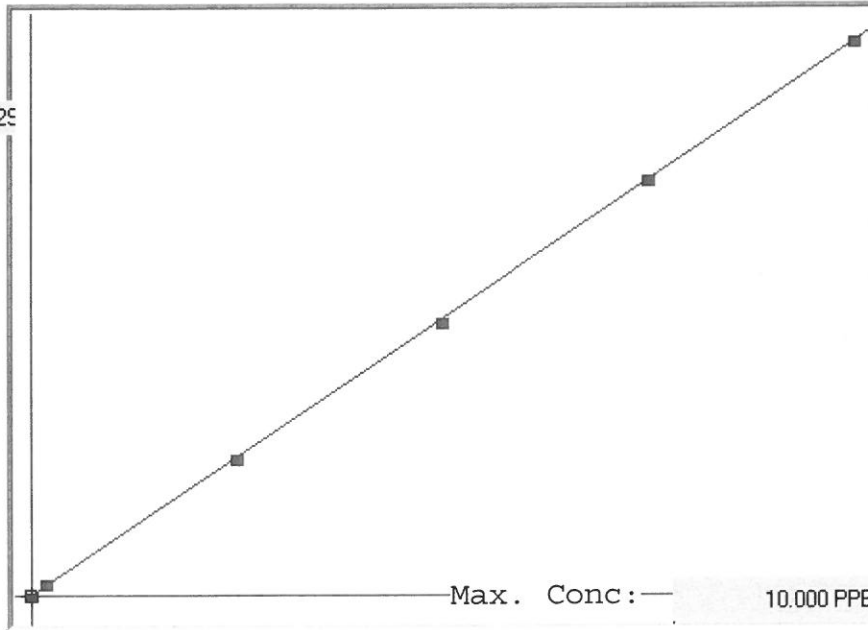

A= 0.0000e+000

B= 2.3991e-004

C= 8.5600e-003

Rho= 0.9999541

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.000	-0.000	-37	0.000	-37					
0.2	0.200	0.248	0.048	998	0.0 %	998					
2.5	2.500	2.472	-0.028	10267	0.0 %	10267					
5.0	5.000	4.940	-0.060	20556	0.0 %	20556					
7.5	7.500	7.521	0.021	31312	0.0 %	31312					
10.0	10.000	10.020	0.020	41729	0.0 %	41729					

0.00
24
11
00

LB120881 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Jun 2022 13:47:44					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-37	-	0.0000	7470A	PPB	29 Jun 2022 14:00:12	S	Std
0.2 - 1	50.2	998	-	0.2000	7470A	PPB	29 Jun 2022 14:02:29	S	Std
2.5 - 1	52.5	10267	-	2.5000	7470A	PPB	29 Jun 2022 14:04:46	S	Std
5.0 - 1	55	20556	-	5.0000	7470A	PPB	29 Jun 2022 14:07:03	S	Std
7.5 - 1	57.5	31312	-	7.5000	7470A	PPB	29 Jun 2022 14:09:19	S	Std
10.0 - 1	58	41729	-	10.0000	7470A	PPB	29 Jun 2022 14:11:35	S	Std
ICV18 - 1	ICV18	15854	3.8121	-	7470A	PPB	29 Jun 2022 14:15:15	U	SMPL
ICB18 - 1	ICB18	-69	-0.0080	-	7470A	PPB	29 Jun 2022 14:17:30	U	SMPL
CCV61 - 1	CCV61	20293	4.8771	-	7470A	PPB	29 Jun 2022 14:19:45	U	SMPL
CCB61 - 1	CCB61	-80	-0.0106	-	7470A	PPB	29 Jun 2022 14:22:00	U	SMPL
CRA - 1	CRA	998	0.2480	-	7470A	PPB	29 Jun 2022 14:24:15	U	SMPL
HighStd - 1	HighStd	41422	9.9461	-	7470A	PPB	29 Jun 2022 14:26:30	U	SMPL
ChkStd - 1	ChkStd	29131	6.9974	-	7470A	PPB	29 Jun 2022 14:31:19	U	SMPL
PB145880BL - 1	PBW	233	0.0645	-	7470A	PPB	29 Jun 2022 14:33:34	U	SMPL
PB145880BS - 1	LCSW	16003	3.8479	-	7470A	PPB	29 Jun 2022 14:38:24	U	SMPL
N3491-01 - 1	AUD-1728	107	0.0342	-	7470A	PPB	29 Jun 2022 14:40:40	U	SMPL
N3504-07 - 1	TRE-1613-15	826	0.2067	-	7470A	PPB	29 Jun 2022 14:42:56	U	SMPL
N3504-07DUP - 1	TRE-1613-15DUP	908	0.2264	-	7470A	PPB	29 Jun 2022 14:45:12	U	SMPL
N3504-07MS - 1	TRE-1613-15MS	17205	4.1362	-	7470A	PPB	29 Jun 2022 14:51:42	U	SMPL
N3504-07MSD - 1	TRE-1613-15MSD	18401	4.4232	-	7470A	PPB	29 Jun 2022 14:53:56	U	SMPL
CCV62 - 1	CCV62	20567	4.9428	-	7470A	PPB	29 Jun 2022 14:56:13	U	SMPL
CCB62 - 1	CCB62	-148	-0.0269	-	7470A	PPB	29 Jun 2022 14:58:29	U	SMPL
N3504-08 - 1	TRE-1616-1618	6022	1.4533	-	7470A	PPB	29 Jun 2022 15:00:45	U	SMPL
N3515-01 - 1	END-OF-TRENCH	1853	0.4531	-	7470A	PPB	29 Jun 2022 15:03:00	U	SMPL
N3515-02 - 1	SPOT-3	13485	3.2438	-	7470A	PPB	29 Jun 2022 15:05:15	U	SMPL
N3524-06 - 1	31466	82967	19.9132	-	7470A	PPB	29 Jun 2022 15:07:30	U	SMPL
PB145944BL - 1	PBW	-35	0.0002	-	7470A	PPB	29 Jun 2022 15:09:47	U	SMPL
PB145944BS - 1	LCSW	18494	4.4455	-	7470A	PPB	29 Jun 2022 15:12:06	U	SMPL
N3472-06 - 1	D2559	147	0.0438	-	7470A	PPB	29 Jun 2022 15:14:22	U	SMPL
N3472-06DUP - 1	D2559DUP	319	0.0851	-	7470A	PPB	29 Jun 2022 15:16:39	U	SMPL
N3472-06MS - 1	D2559MS	18503	4.4476	-	7470A	PPB	29 Jun 2022 15:18:56	U	SMPL
CCV63 - 1	CCV63	20804	4.9997	-	7470A	PPB	29 Jun 2022 15:23:28	U	SMPL
CCB63 - 1	CCB63	-118	-0.0197	-	7470A	PPB	29 Jun 2022 15:25:43	U	SMPL
N3504-07LX5 - 1		166	0.0484	-	7470A	PPB	29 Jun 2022 15:27:58	U	SMPL
N3504-07A - 1		17589	4.2283	-	7470A	PPB	29 Jun 2022 15:30:14	U	SMPL
N3472-06LX5 - 1		-86	-0.0121	-	7470A	PPB	29 Jun 2022 15:32:29	U	SMPL
N3472-06A - 1		19373	4.6564	-	7470A	PPB	29 Jun 2022 15:34:46	U	SMPL
PB145911TB - 1	PB145911TB	21	0.0136	-	7470A	PPB	29 Jun 2022 15:37:02	U	SMPL
N3472-06MSD - 1	D2559MSD	18869	4.5354	-	7470A	PPB	29 Jun 2022 15:39:19	U	SMPL
N3524-06DLX5 - 1		19690	4.7324	-	7470A	PPB	29 Jun 2022 15:54:03	U	SMPL
CCV64 - 1	CCV64	20287	4.8756	-	7470A	PPB	29 Jun 2022 15:56:19	U	SMPL
CCB64 - 1	PB145911TB CCB64	-120	-0.0202	-	7470A	PPB	29 Jun 2022 15:58:37	U	SMPL

ms
6/29/22