

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

6/27/2022 16:09

Test: TEST CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	90.338	0.0	0.020	
ICB001 ICB001	0.974	0.0	0.001	
CCV001 CCV001	242.327	0.0	0.053	
CCB001 CCB001	0.988	0.0	0.001	
12 6/27/22 P B145866BL PBW866	1.109	0.0	0.001	
N3356-01 MEY0C3	0.593	0.0	0.001	
N3356-02 MEY0C7	2.267	0.0	0.001	
N3356-03 MEY0C5	0.833	0.0	0.001	
N3356-04 MEY0C6	0.663	0.0	0.001	
N3356-05 MEY0C9	0.534	0.0	0.001	
N3356-06 MEY0C9D	1.058	0.0	0.001	
N3356-07 MEY0C9S	93.287	0.0	0.021	
N3356-08 MEY0D0	1.323	0.0	0.001	
N3356-10 MEY0C8	0.797	0.0	0.001	
N3356-11 MEY0D3	1.456	0.0	0.001	
CCV002 CCV002	241.877	0.0	0.053	
CCB002 CCB002	1.226	0.0	0.001	

N	17
Mean	40.097
SD	81.6911
CV%	203.73

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 27 15:56:35 2022

Mon Jun 27 16:09:28 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	TEST CN	P	1.3034	µg/l	6/27/2022 15:56:49
S5.0	A	TEST CN	P	4.9577	µg/l	6/27/2022 15:56:50
S10.0	A	TEST CN	P	10.0417	µg/l	6/27/2022 15:56:51
S100.0	A	TEST CN	P	97.134	µg/l	6/27/2022 15:56:52
S250.0	A	TEST CN	P	251.9806	µg/l	6/27/2022 15:56:53
S500.0	A	TEST CN	P	499.5825	µg/l	6/27/2022 15:56:54
ICV001 ICV001	S	TEST CN	P	90.3378	µg/l	6/27/2022 16:01:04
ICB001 ICB001	S	TEST CN	P	0.9737	µg/l	6/27/2022 16:01:05
CCV001 CCV001	S	TEST CN	P	242.3265	µg/l	6/27/2022 16:01:06
CCB001 CCB001	S	TEST CN	P	0.9878	µg/l	6/27/2022 16:01:07
PB145866BL PBW866	S	TEST CN	P	1.1087	µg/l	6/27/2022 16:01:08
N3356-01 MEY0C3	S	TEST CN	P	0.593	µg/l	6/27/2022 16:01:09
N3356-02 MEY0C7	S	TEST CN	P	2.2672	µg/l	6/27/2022 16:09:22
N3356-03 MEY0C5	S	TEST CN	P	0.8333	µg/l	6/27/2022 16:09:23
N3356-04 MEY0C6	S	TEST CN	P	0.6632	µg/l	6/27/2022 16:09:24
N3356-05 MEY0C9	S	TEST CN	P	0.5341	µg/l	6/27/2022 16:09:25
N3356-06 MEY0C9D	S	TEST CN	P	1.0584	µg/l	6/27/2022 16:09:26
N3356-07 MEY0C9S	S	TEST CN	P	93.287	µg/l	6/27/2022 16:09:27
N3356-08 MEY0D0	S	TEST CN	P	1.3229	µg/l	6/27/2022 16:09:28
N3356-10 MEY0C8	S	TEST CN	P	0.7969	µg/l	6/27/2022 16:09:29
N3356-11 MEY0D3	S	TEST CN	P	1.4563	µg/l	6/27/2022 16:09:30
CCV002 CCV002	S	TEST CN	P	241.8768	µg/l	6/27/2022 16:09:31
CCB002 CCB002	S	TEST CN	P	1.2257	µg/l	6/27/2022 16:09:32

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

6/27/2022 15:57


Test TEST CN

Accepted 6/27/2022 15:57

~~Factor Slope~~ ~~4656~~ 0.000215
Bias % Intercept 0.001 07/01/22

Coeff. of det. 0.999929

Errors

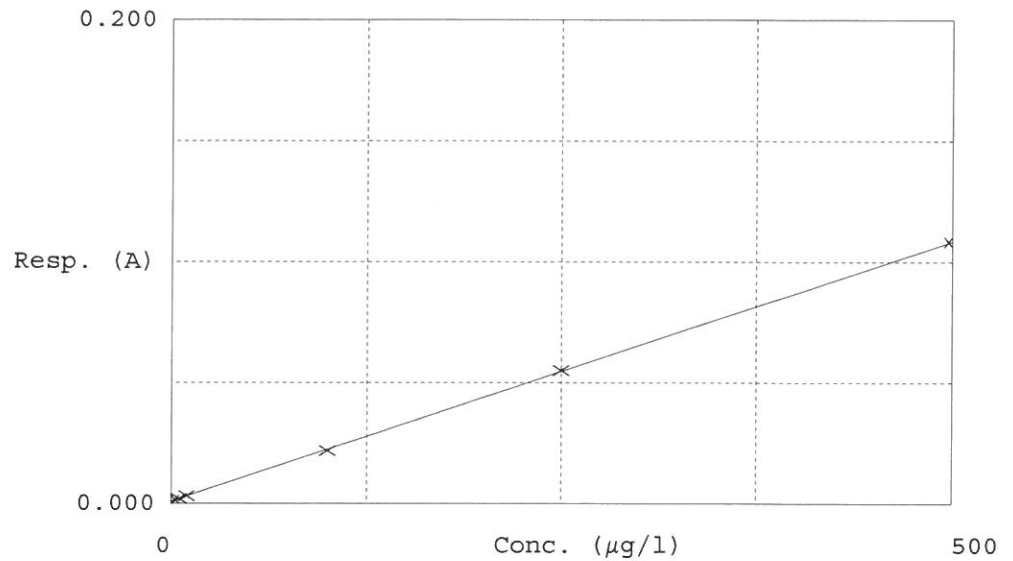

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN 5.00	0.001	1.3034	0.0000	-
2	5.0PPBCN 5.5.0	0.002	4.9577	5.0000	-0.8
3	10PPBCN 5.10.0	0.003	10.0417	10.0000	0.4
4	100PPBCN 5.100.0	0.022	97.1340	100.0000	-2.9
5	250PPBCN 5.250.0	0.055	251.9806	250.0000	0.8
6	500PPBCN 5.500.0	0.108	499.5825	500.0000	-0.1

12
6/28/22