

LB120925


245.1

INSTRUMENT ID: CV1

Linear

μ Abs.:

39017

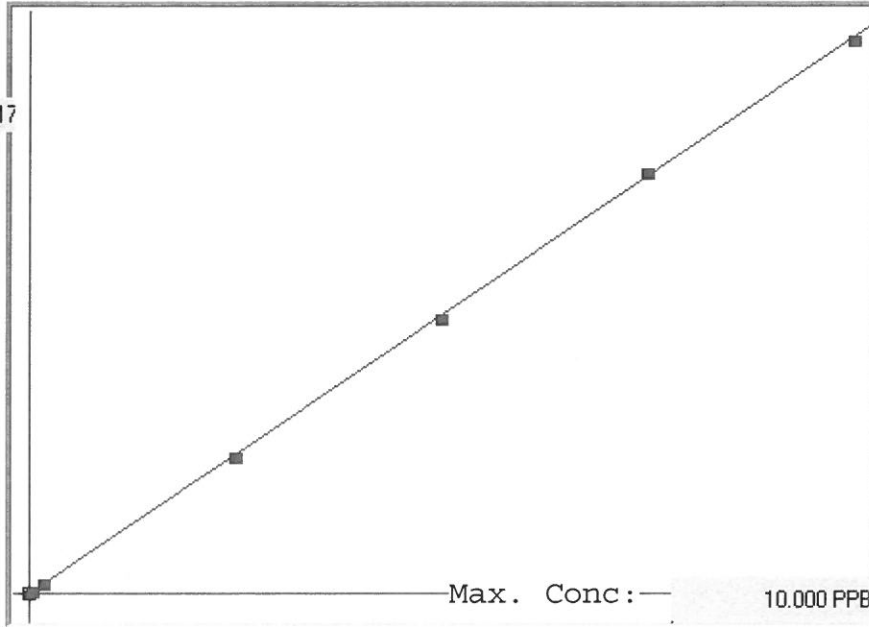

A= 0.0000e+000

B= 2.5502e-004

C= 1.4952e-002

Rho= 0.9999596

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.011	0.011	-17	0.000	-17				
0.05	0.050	0.058	0.008	168	0.0 %	168	0			
0.2	0.200	0.194	-0.006	702	0.0 %	702				
2.5	2.500	2.479	-0.021	9664	0.0 %	9664				
5.0	5.000	4.972	-0.028	19437	0.0 %	19437				
7.5	7.500	7.572	0.072	29632	0.0 %	29632				
10.0	10.000	9.965	-0.035	39017	0.0 %	39017				

900
-14 16
-3
-1
1
0
m3
215k22

LB120925 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 05 Jul 2022 10:11:35

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-17	-	0.0000	245.1	PPB	05 Jul 2022 10:33:24	S	Std
0.05 - 1	50.05	168	-	0.0500	245.1	PPB	05 Jul 2022 10:35:41	S	Std
0.2 - 1	50.2	702	-	0.2000	245.1	PPB	05 Jul 2022 10:37:58	S	Std
2.5 - 1	52.5	9664	-	2.5000	245.1	PPB	05 Jul 2022 10:40:16	S	Std
5.0 - 1	55	19437	-	5.0000	245.1	PPB	05 Jul 2022 10:42:32	S	Std
7.5 - 1	57.5	29632	-	7.5000	245.1	PPB	05 Jul 2022 10:44:48	S	Std
10.0 - 1	516	39017	-	10.0000	245.1	PPB	05 Jul 2022 11:07:39	S	Std
ICV24 - 1	ICV24	15479	3.9623	-245.1		PPB	05 Jul 2022 11:12:55	U	SMPL
ICB24 - 1	ICB24	-60	-0.0003	-245.1		PPB	05 Jul 2022 11:15:10	U	SMPL
CCV82 - 1	CCV82	19750	5.0515	-245.1		PPB	05 Jul 2022 11:17:26	U	SMPL
CCB82 - 1	CCB82	-62	-0.0009	-245.1		PPB	05 Jul 2022 11:19:41	U	SMPL
CRA - 1	CRA	196	0.0649	-245.1		PPB	05 Jul 2022 11:21:56	U	SMPL
HighStd - 1	HighStd	38094	9.7295	-245.1		PPB	05 Jul 2022 11:24:11	U	SMPL
ChkStd - 1	ChkStd	27577	7.0475	-245.1		PPB	05 Jul 2022 11:26:27	U	SMPL
PB146017BL - 1	PBW	-66	-0.0019	-245.1		PPB	05 Jul 2022 11:31:18	U	SMPL
PB146017BS - 1	LCSW	13519	3.4625	-245.1		PPB	05 Jul 2022 11:36:08	U	SMPL
N3518-01 - 1	TI-604-EB	275	0.0851	-245.1		PPB	05 Jul 2022 11:38:24	U	SMPL
N3518-03 - 1	TI-604	406	0.1185	-245.1		PPB	05 Jul 2022 11:40:41	U	SMPL
N3518-03DUP - 1	TI-604DUP	409	0.1193	-245.1		PPB	05 Jul 2022 11:42:58	U	SMPL
N3518-03MS - 1	TI-604MS	16084	4.1166	-245.1		PPB	05 Jul 2022 11:47:47	U	SMPL
N3518-03MSD - 1	TI-604MSD	16342	4.1824	-245.1		PPB	05 Jul 2022 11:53:11	U	SMPL
CCV83 - 1	CCV83	19621	5.0186	-245.1		PPB	05 Jul 2022 11:55:26	U	SMPL
CCB83 - 1	CCB83	-68	-0.0024	-245.1		PPB	05 Jul 2022 11:57:41	U	SMPL
N3518-05 - 1	TI-604-X	435	0.1259	-245.1		PPB	05 Jul 2022 11:59:57	U	SMPL
N3525-01 - 1	MH-725	399	0.1167	-245.1		PPB	05 Jul 2022 12:02:12	U	SMPL
N3525-02 - 1	MH-725	365	0.1080	-245.1		PPB	05 Jul 2022 12:04:27	U	SMPL
N3518-03LX5 - 1		31	0.0229	-245.1		PPB	05 Jul 2022 12:06:43	U	SMPL
N3518-03A - 1		16502	4.2232	-245.1		PPB	05 Jul 2022 12:08:59	U	SMPL
CCV84 - 1	CCV84	19157	4.9003	-245.1		PPB	05 Jul 2022 12:11:15	U	SMPL
CCB84 - 1	CCB84	-56	0.0007	-245.1		PPB	05 Jul 2022 12:13:32	U	SMPL