

LB120955

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : SM

Instrument ID : Konelab

7/6/2022 15:57

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.147	0.0	0.076	
ICB1	1.019	0.0	0.002	
CCV1	242.195	0.0	0.197	
CCB1	1.097	0.0	0.002	
PB146058BL	0.874	0.0	0.001	
N3575-01	0.844	0.0	0.001	
N3575-01DUP	0.802	0.0	0.001	
N3583-02	1.110	0.0	0.002	
N3583-03	0.690	0.0	0.001	
N3604-04	1.074	0.0	0.002	
N3604-05	0.786	0.0	0.001	
CCV2	247.667	0.0	0.202	
CCB2	1.076	0.0	0.002	

N	13
Mean	45.568
SD	92.0549
CV%	202.02

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 06 15:48:31 2022

Wed Jul 06 15:54:49 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Total CN	P	0.6768	µg/l	7/6/2022 13:41:06
5.OPPBCN	A	Total CN	P	4.8583	µg/l	7/6/2022 13:41:07
10PPBCN	A	Total CN	P	10.2363	µg/l	7/6/2022 13:41:08
50PPBCN	A	Total CN	P	48.8203	µg/l	7/6/2022 13:41:09
100PPBCN	A	Total CN	P	98.5996	µg/l	7/6/2022 13:41:10
250PPBCN	A	Total CN	P	252.8282	µg/l	7/6/2022 13:41:11
500PPBCN	A	Total CN	P	498.9807	µg/l	7/6/2022 13:41:12
ICV1	S	Total CN	P	93.1472	µg/l	7/6/2022 15:48:31
ICB1	S	Total CN	P	1.0186	µg/l	7/6/2022 15:48:33
CCV1	S	Total CN	P	242.1945	µg/l	7/6/2022 15:48:36
CCB1	S	Total CN	P	1.0971	µg/l	7/6/2022 15:48:38
PB146058BL	S	Total CN	P	0.8744	µg/l	7/6/2022 15:48:40
N3575-01	S	Total CN	P	0.8436	µg/l	7/6/2022 15:48:41
N3575-01DUP	S	Total CN	P	0.802	µg/l	7/6/2022 15:54:42
N3583-02	S	Total CN	P	1.11	µg/l	7/6/2022 15:54:43
N3583-03	S	Total CN	P	0.6897	µg/l	7/6/2022 15:54:44
N3604-04	S	Total CN	P	1.0739	µg/l	7/6/2022 15:54:45
N3604-05	S	Total CN	P	0.7859	µg/l	7/6/2022 15:54:46
CCV2	S	Total CN	P	247.667	µg/l	7/6/2022 15:54:48
CCB2	S	Total CN	P	1.0757	µg/l	7/6/2022 15:54:49

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : SM Instrument ID : Konelab

7/6/2022 13:43


Test Total CN

Accepted 7/6/2022 13:43

Factor 1233
Bias 0.001

Coeff. of det. 0.999937

Errors

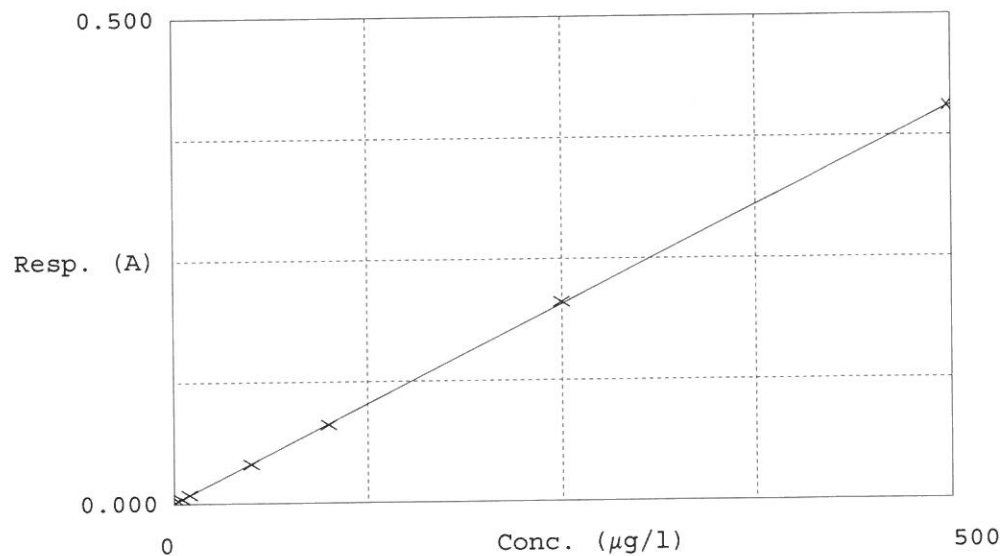

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.6768	0.0000	
2	5.0PPBCN	0.005	4.8583	5.0000	-2.8
3	10PPBCN	0.009	10.2363	10.0000	2.4
4	50PPBCN	0.040	48.8203	50.0000	-2.4
5	100PPBCN	0.081	98.5996	100.0000	-1.7
6	250PPBCN	0.206	252.8282	250.0000	1.1
7	500PPBCN	0.405	498.9807	500.0000	-0.2

RE
SM
7/6/22