


LB120976

7470A

INSTRUMENT ID: CV1

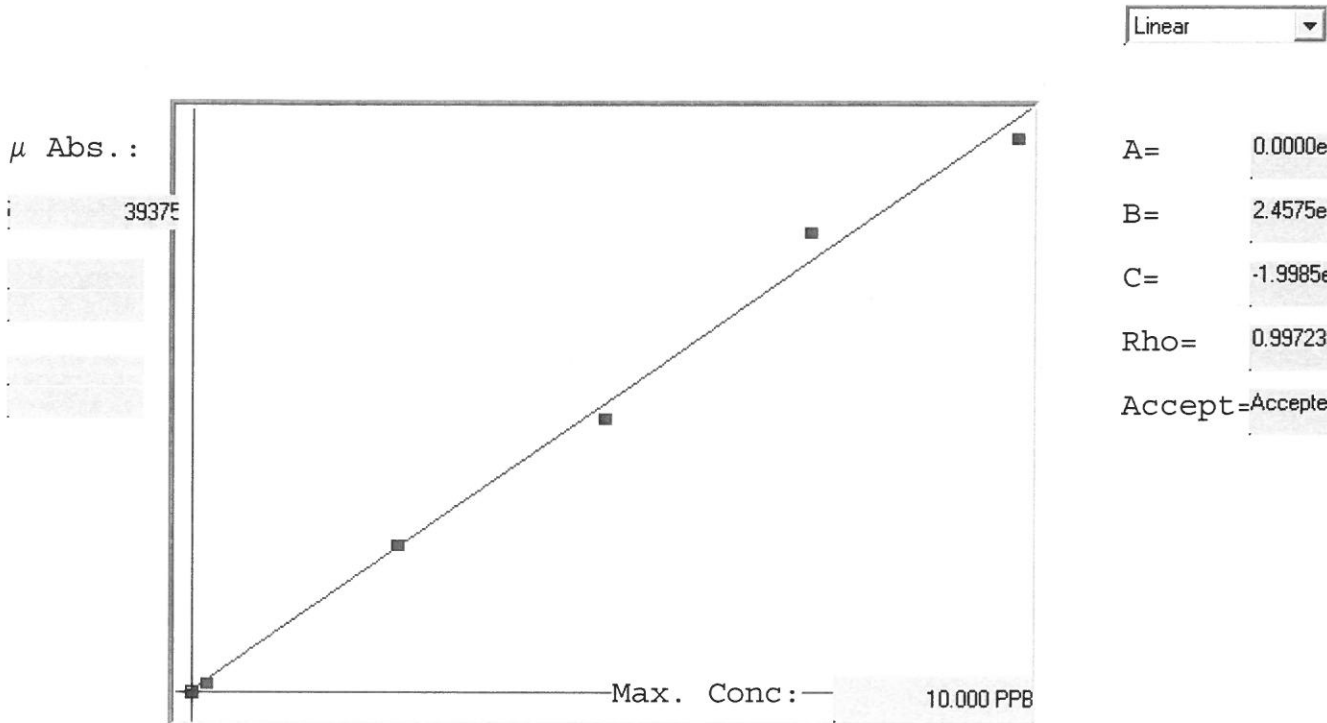

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.020	-0.020	1	0.000	1					1
0.2	0.200	0.180	-0.020	814	0.0 %	814					-10
2.5	2.500	2.591	0.091	10626	0.0 %	10626					4
5.0	5.000	4.771	-0.229	19497	0.0 %	19497					-5
7.5	7.500	8.021	0.521	32719	0.0 %	32719					7
10.0	10.000	9.656	-0.344	39375	0.0 %	39375					-3

LB120976 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Jul 2022 08:21:09

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	1	-	0.0000	7470A	PPB	08 Jul 2022 08:37:15	S	Std
0.2 - 1	50.2	814	-	0.2000	7470A	PPB	08 Jul 2022 08:39:32	S	Std
2.5 - 1	52.5	10626	-	2.5000	7470A	PPB	08 Jul 2022 08:41:50	S	Std
5.0 - 1	55	19497	-	5.0000	7470A	PPB	08 Jul 2022 08:49:14	S	Std
7.5 - 1	57.5	32719	-	7.5000	7470A	PPB	08 Jul 2022 08:51:31	S	Std
10.0 - 1	510	39375	-	10.0000	7470A	PPB	08 Jul 2022 08:56:24	S	Std
ICV30 - 1	ICV30	14957	3.6557	-	7470A	PPB	08 Jul 2022 08:59:16	U	SMPL
ICB30 - 1	ICB30	-59	-0.0345	-	7470A	PPB	08 Jul 2022 09:01:31	U	SMPL
CCV01 - 1	CCV01	19726	4.8276	-	7470A	PPB	08 Jul 2022 09:03:46	U	SMPL
CCB01 - 1	CCB01	-59	-0.0345	-	7470A	PPB	08 Jul 2022 09:06:01	U	SMPL
CRA - 1	CRA	811	0.1793	-	7470A	PPB	08 Jul 2022 09:10:47	U	SMPL
HighStd - 1	HighStd	39344	9.6487	-	7470A	PPB	08 Jul 2022 09:13:02	U	SMPL
ChkStd - 1	ChkStd	29231	7.1635	-	7470A	PPB	08 Jul 2022 09:15:17	U	SMPL
PB146081BL - 1	PBW	-74	-0.0382	-	7470A	PPB	08 Jul 2022 09:17:34	U	SMPL
PB146081BS - 1	LCSW	15212	3.7183	-	7470A	PPB	08 Jul 2022 09:19:50	U	SMPL
N3578-02 - 1	MF-OIL-D-0705	-27	-0.0266	-	7470A	PPB	08 Jul 2022 09:22:07	U	SMPL
N3578-05 - 1	MF-SOLID-D-0705	4	-0.0190	-	7470A	PPB	08 Jul 2022 09:24:23	U	SMPL
N3578-08 - 1	MF-OIL-T-0705	25	-0.0138	-	7470A	PPB	08 Jul 2022 09:26:40	U	SMPL
N3590-02 - 1	162	15	-0.0163	-	7470A	PPB	08 Jul 2022 09:31:13	U	SMPL
CCV02 - 1	CCV02	20860	5.1063	-	7470A	PPB	08 Jul 2022 09:33:29	U	SMPL
CCB02 - 1	CCB02	-61	-0.0350	-	7470A	PPB	08 Jul 2022 09:35:44	U	SMPL
N3590-05 - 1	160	814	0.1801	-	7470A	PPB	08 Jul 2022 09:37:59	U	SMPL
N3604-01 - 1	1975	-127	-0.0512	-	7470A	PPB	08 Jul 2022 09:40:14	U	SMPL
N3604-02 - 1	1973-1974	57	-0.0060	-	7470A	PPB	08 Jul 2022 09:42:30	U	SMPL
N3604-03 - 1	1965-1976	-13	-0.0232	-	7470A	PPB	08 Jul 2022 09:44:46	U	SMPL
N3604-03DUP - 1	1965-1976DUP	-13	-0.0232	-	7470A	PPB	08 Jul 2022 09:47:02	U	SMPL
N3604-03MS - 1	1965-1976MS	14582	3.5635	-	7470A	PPB	08 Jul 2022 09:49:18	U	SMPL
N3604-03MSD - 1	1965-1976MSD	14036	3.4293	-	7470A	PPB	08 Jul 2022 09:51:34	U	SMPL
PB146082BL - 1	PBW	-50	-0.0323	-	7470A	PPB	08 Jul 2022 09:53:51	U	SMPL
PB146082BS - 1	LCSW	15216	3.7193	-	7470A	PPB	08 Jul 2022 09:59:30	U	SMPL
N3583-02 - 1	307	-5	-0.0212	-	7470A	PPB	08 Jul 2022 10:01:45	U	SMPL
CCV03 - 1	CCV03	21081	5.1606	-	7470A	PPB	08 Jul 2022 10:04:00	U	SMPL
CCB03 - 1	CCB03	-45	-0.0310	-	7470A	PPB	08 Jul 2022 10:06:16	U	SMPL
N3583-03 - 1	311	21	-0.0148	-	7470A	PPB	08 Jul 2022 10:08:31	U	SMPL
N3590-06 - 1	161	37	-0.0109	-	7470A	PPB	08 Jul 2022 10:10:47	U	SMPL
N3604-04 - 1	1969	-4	-0.0210	-	7470A	PPB	08 Jul 2022 10:13:02	U	SMPL
N3604-04DUP - 1	1969DUP	1	-0.0197	-	7470A	PPB	08 Jul 2022 10:15:18	U	SMPL
N3604-04MS - 1	1969MS	14460	3.5335	-	7470A	PPB	08 Jul 2022 10:17:34	U	SMPL
N3604-04MSD - 1	1969MSD	14260	3.4844	-	7470A	PPB	08 Jul 2022 10:19:50	U	SMPL
N3604-05 - 1	1970	-19	-0.0247	-	7470A	PPB	08 Jul 2022 10:22:07	U	SMPL
PB146086BL - 1	PBW	-17	-0.0242	-	7470A	PPB	08 Jul 2022 10:24:24	U	SMPL
PB146086BS - 1	LCSW	15577	3.8080	-	7470A	PPB	08 Jul 2022 10:26:41	U	SMPL
N3594-02 - 1	COMP	421	0.0835	-	7470A	PPB	08 Jul 2022 10:28:56	U	SMPL
CCV04 - 1	CCV04	20235	4.9527	-	7470A	PPB	08 Jul 2022 10:31:12	U	SMPL
CCB04 - 1	CCB04	-71	-0.0374	-	7470A	PPB	08 Jul 2022 10:33:27	U	SMPL
N3594-02DUP - 1	COMP DUP	469	0.0953	-	7470A	PPB	08 Jul 2022 10:38:17	U	SMPL
N3594-02MS - 1	COMPMS	10850	2.6464	-	7470A	PPB	08 Jul 2022 10:40:32	U	SMPL
N3594-02MSD - 1	COMPMSD	11283	2.7528	-	7470A	PPB	08 Jul 2022 10:42:48	U	SMPL
N3595-16 - 1	20220493-FIELD-BLANK	-106	-0.0460	-	7470A	PPB	08 Jul 2022 10:45:05	U	SMPL
N3596-01 - 1	20220482-FIELD-BLANK	-37	-0.0291	-	7470A	PPB	08 Jul 2022 10:47:22	U	SMPL
N3621-02 - 1	TT-047-IDWGW-20220706	84	0.0007	-	7470A	PPB	08 Jul 2022 10:49:38	U	SMPL
PB146040TB - 1	PB146040TB	3	-0.0192	-	7470A	PPB	08 Jul 2022 10:51:55	U	SMPL
PB146041TB - 1	PB146041TB	0	-0.0200	-	7470A	PPB	08 Jul 2022 10:54:11	U	SMPL
CCV05 - 1	CCV05	20006	4.8964	-	7470A	PPB	08 Jul 2022 10:56:28	U	SMPL
CCB05 - 1	CCB05	-59	-0.0345	-	7470A	PPB	08 Jul 2022 10:58:44	U	SMPL
N3604-03LX5 - 1		-58	-0.0342	-	7470A	PPB	08 Jul 2022 11:00:59	U	SMPL
N3604-03A - 1		16955	4.1467	-	7470A	PPB	08 Jul 2022 11:03:15	U	SMPL
N3604-04LX5 - 1		-98	-0.0441	-	7470A	PPB	08 Jul 2022 11:05:31	U	SMPL
N3604-04A - 1		15993	3.9103	-	7470A	PPB	08 Jul 2022 11:07:47	U	SMPL
N3594-02LX5 - 1		-30	-0.0274	-	7470A	PPB	08 Jul 2022 11:10:02	U	SMPL
N3594-02A - 1		16598	4.0589	-	7470A	PPB	08 Jul 2022 11:12:18	U	SMPL
CCV06 - 1	CCV06	19388	4.7446	-	7470A	PPB	08 Jul 2022 11:14:34	U	SMPL
CCB06 - 1	CCB06	-73	-0.0379	-	7470A	PPB	08 Jul 2022 11:16:50	U	SMPL