

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : SM Instrument ID : Kone

7/13/2022 13:10

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.239	0.0	0.071	
ICB1	0.806	0.0	0.001	
CCV1	252.903	0.0	0.191	
CCB1	0.859	0.0	0.001	
PB146197BL	1.002	0.0	0.001	
N3648-02	0.955	0.0	0.001	
N3648-02DUP	0.776	0.0	0.001	
N3648-05	0.853	0.0	0.001	
N3663-02	0.852	0.0	0.001	
N3682-01	0.968	0.0	0.001	
N3682-03	0.994	0.0	0.001	
N3682-04	1.102	0.0	0.002	
N3687-05	1.072	0.0	0.002	
N3682-02	1.140	0.0	0.002	
CCV2	250.136	0.0	0.189	
CCB2	1.162	0.0	0.002	
N3687-06	0.586	0.0	0.001	
PB146198BL	0.753	0.0	0.001	
N3682-05	0.722	0.0	0.001	
N3682-05DUP	0.871	0.0	0.001	
N3682-06	0.885	0.0	0.001	
CCV3	251.505	0.0	0.190	
CCB3	1.130	0.0	0.002	

N	23
Mean	37.620
SD	86.8492
CV%	230.86

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 13 12:43:59 2022

Wed Jul 13 12:57:52 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Total CN	P	0.6676	µg/l	7/13/2022 11:29:25
5.OPPBCN	A	Total CN	P	4.9827	µg/l	7/13/2022 11:29:26
10PPBCN	A	Total CN	P	9.9137	µg/l	7/13/2022 11:29:27
50PPBCN	A	Total CN	P	48.3084	µg/l	7/13/2022 11:29:28
100PPBCN	A	Total CN	P	98.6347	µg/l	7/13/2022 11:29:29
250PPBCN	A	Total CN	P	254.0977	µg/l	7/13/2022 11:29:30
500PPBCN	A	Total CN	P	498.3952	µg/l	7/13/2022 11:29:31
ICV1	S	Total CN	P	93.2389	µg/l	7/13/2022 12:43:59
ICB1	S	Total CN	P	0.8059	µg/l	7/13/2022 12:44:01
CCV1	S	Total CN	P	252.9034	µg/l	7/13/2022 12:44:04
CCB1	S	Total CN	P	0.8587	µg/l	7/13/2022 12:44:06
PB146197BL	S	Total CN	P	1.0018	µg/l	7/13/2022 12:44:08
N3648-02	S	Total CN	P	0.9551	µg/l	7/13/2022 12:44:09
N3648-02DUP	S	Total CN	P	0.7764	µg/l	7/13/2022 12:51:34
N3648-05	S	Total CN	P	0.8529	µg/l	7/13/2022 12:51:35
N3663-02	S	Total CN	P	0.8522	µg/l	7/13/2022 12:51:36
N3682-01	S	Total CN	P	0.9684	µg/l	7/13/2022 12:51:37
N3682-03	S	Total CN	P	0.994	µg/l	7/13/2022 12:51:39
N3682-04	S	Total CN	P	1.1016	µg/l	7/13/2022 12:51:40
N3687-05	S	Total CN	P	1.0722	µg/l	7/13/2022 12:51:41
N3682-02	S	Total CN	P	1.1405	µg/l	7/13/2022 12:51:42
CCV2	S	Total CN	P	250.1364	µg/l	7/13/2022 12:51:43
CCB2	S	Total CN	P	1.1615	µg/l	7/13/2022 12:51:44
N3687-06	S	Total CN	P	0.5859	µg/l	7/13/2022 12:57:45
PB146198BL	S	Total CN	P	0.7526	µg/l	7/13/2022 12:57:46
N3682-05	S	Total CN	P	0.7221	µg/l	7/13/2022 12:57:47
N3682-05DUP	S	Total CN	P	0.8712	µg/l	7/13/2022 12:57:48
N3682-06	S	Total CN	P	0.8851	µg/l	7/13/2022 12:57:49
CCV3	S	Total CN	P	251.5048	µg/l	7/13/2022 12:57:51
CCB3	S	Total CN	P	1.1295	µg/l	7/13/2022 12:57:52

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : SM

Instrument ID : Konelab

7/13/2022 11:30


Test Total CN

Accepted 7/13/2022 11:30

Factor 1327
Bias 0.001

Coeff. of det. 0.999881

Errors

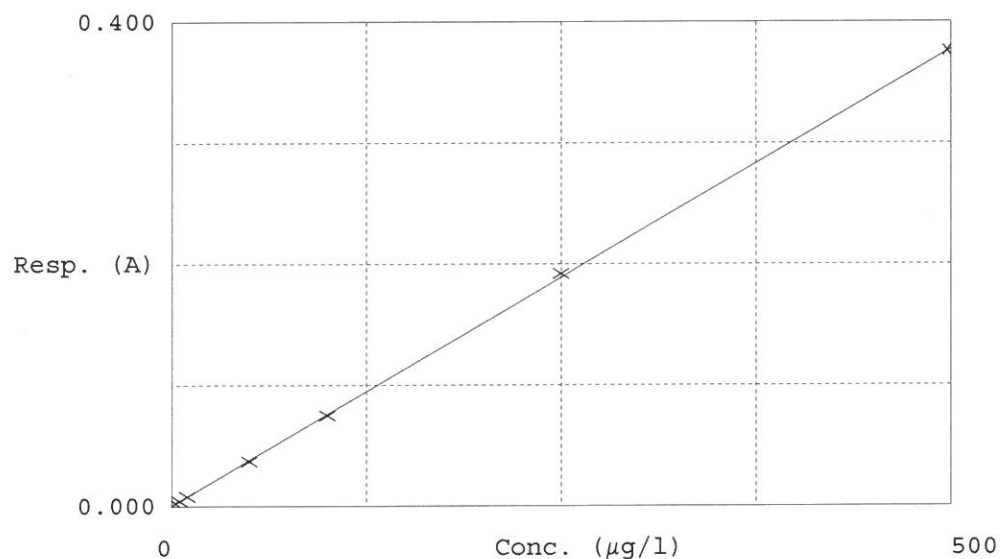

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.6676	0.0000	
2	5.0PPBCN	0.004	4.9827	5.0000	-0.3
3	10PPBCN	0.008	9.9137	10.0000	-0.9
4	50PPBCN	0.037	48.3084	50.0000	-3.4
5	100PPBCN	0.075	98.6347	100.0000	-1.7
6	250PPBCN	0.192	254.0977	250.0000	1.6
7	500PPBCN	0.376	498.3952	500.0000	-0.3

RM

7/13/22