

LB121053

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

7/13/2022 15:45

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.059	0.0	0.108	
ICB1	0.005	0.0	0.008	
CCV1	1.063	0.0	0.109	
CCB1	0.004	0.0	0.008	
PB146176BL	0.005	0.0	0.008	
PB146176BS	1.062	0.0	0.108	
N3214-10	0.028	0.0	0.010	
N3214-11	0.056	0.0	0.013	
N3633-02	0.081	0.0	0.015	
N3633-02DUP	0.083	0.0	0.015	
N3633-02MS	1.346	0.0	0.136	
N3633-02MSD	1.356	0.0	0.136	
N3633-04	0.004	0.0	0.008	
N3633-06	0.008	0.0	0.008	
CCV2	1.070	0.0	0.109	
CCB2	0.003	0.0	0.008	

N	16
Mean	0.452
SD	0.5728
CV%	126.71

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 13 13:45:13 2022

Wed Jul 13 15:41:29 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0062	mg/l	7/13/2022 13:45:13	
0.05PPM	A	Phenolics-	P	0.0583	mg/l	7/13/2022 13:45:14	
0.1PPM	A	Phenolics-	P	0.1052	mg/l	7/13/2022 13:45:15	
0.25PPM	A	Phenolics-	P	0.2466	mg/l	7/13/2022 13:45:16	
0.50PPM	A	Phenolics-	P	0.5005	mg/l	7/13/2022 13:45:17	
1.0PPM	A	Phenolics-	P	0.9666	mg/l	7/13/2022 13:45:18	
2.0PPM	A	Phenolics-	P	2.0165	mg/l	7/13/2022 13:45:19	
ICV1	S	Phenolics-	P	1.0592	mg/l	7/13/2022 15:36:32	
ICB1	S	Phenolics-	P	0.0055	mg/l	7/13/2022 15:36:33	
CCV1	S	Phenolics-	P	1.0631	mg/l	7/13/2022 15:36:34	
CCB1	S	Phenolics-	P	0.0038	mg/l	7/13/2022 15:36:35	
PB146176BL	S	Phenolics-	P	0.0052	mg/l	7/13/2022 15:36:36	
PB146176BS	S	Phenolics-	P	1.0621	mg/l	7/13/2022 15:36:37	
N3214-10	S	Phenolics-	P	0.0276	mg/l	7/13/2022 15:36:38	
N3214-11	S	Phenolics-	P	0.0563	mg/l	7/13/2022 15:36:39	
N3633-02	S	Phenolics-	P	0.0811	mg/l	7/13/2022 15:36:40	
N3633-02DUP	S	Phenolics-	P	0.0832	mg/l	7/13/2022 15:36:41	
N3633-02MS	S	Phenolics-	P	1.3457	mg/l	7/13/2022 15:36:42	
N3633-02MSD	S	Phenolics-	P	1.3557	mg/l	7/13/2022 15:36:43	
N3633-04	S	Phenolics-	P	0.0037	mg/l	7/13/2022 15:41:26	
N3633-06	S	Phenolics-	P	0.008	mg/l	7/13/2022 15:41:27	
CCV2	S	Phenolics-	P	1.0697	mg/l	7/13/2022 15:41:28	
CCB2	S	Phenolics-	P	0.0031	mg/l	7/13/2022 15:41:29	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

7/13/2022 13:56


Test Phenolics-

Accepted 7/13/2022 13:45

Factor 10.49
Bias 0.007

Coeff. of det. 0.999514

Errors

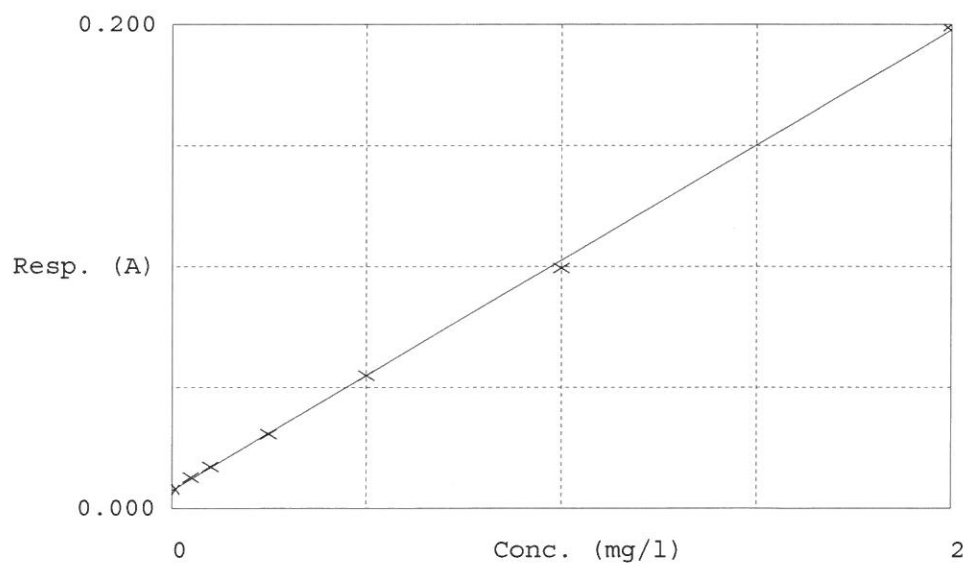

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.008	0.0062	0.0000	-
2	Phenol-2	0.013	0.0583	0.0500	16.6
3	Phenol-2	0.017	0.1052	0.1000	5.2
4	Phenol-2	0.031	0.2466	0.2500	-1.4
5	Phenol-2	0.055	0.5005	0.5000	0.1
6	Phenol-2	0.099	0.9666	1.0000	-3.3
7	Phenol-2	0.199	2.0165	2.0000	0.6

12 7/13/22