

LB121085

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : *AY* Instrument ID : Konelab

7/15/2022 9:05

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.987	0.0	0.109	
ICB1	-0.015	0.0	0.006	
CCV1	0.990	0.0	0.109	
CCB1	-0.014	0.0	0.006	
PB146221BL	-0.015	0.0	0.006	
PB146221BS	0.990	0.0	0.109	
N3214-03	0.026	0.0	0.010	
PB146223BL	-0.015	0.0	0.006	
PB146223BS	0.993	0.0	0.109	
N3214-09	0.027	0.0	0.010	
CCV2	0.987	0.0	0.109	
CCB2	-0.015	0.0	0.006	

N	12
Mean	0.410
SD	0.5111
CV%	124.57

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 14 16:41:32 2022

Thu Jul 14 16:51:45 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.00PPM	A	Phenolics-	P	-0.0005	mg/l	7/14/2022 14:45:19
0.05PPM	A	Phenolics-	P	0.046	mg/l	7/14/2022 14:45:20
0.1PPM	A	Phenolics-	P	0.104	mg/l	7/14/2022 14:45:21
0.25PPM	A	Phenolics-	P	0.2575	mg/l	7/14/2022 14:45:22
0.50PPM	A	Phenolics-	P	0.5075	mg/l	7/14/2022 14:45:23
1.0PPM	A	Phenolics-	P	0.9767	mg/l	7/14/2022 14:45:24
2.0PPM	A	Phenolics-	P	2.0087	mg/l	7/14/2022 14:45:25
ICV1	S	Phenolics-	P	0.9866	mg/l	7/14/2022 16:41:32
ICB1	S	Phenolics-	P	-0.0152	mg/l	7/14/2022 16:41:35
CCV1	S	Phenolics-	P	0.99	mg/l	7/14/2022 16:41:37
CCB1	S	Phenolics-	P	-0.0143	mg/l	7/14/2022 16:41:38
PB146221BL	S	Phenolics-	P	-0.0151	mg/l	7/14/2022 16:41:40
PB146221BS	S	Phenolics-	P	0.9896	mg/l	7/14/2022 16:41:42
N3214-03	S	Phenolics-	P	0.0259	mg/l	7/14/2022 16:51:35
PB146223BL	S	Phenolics-	P	-0.0153	mg/l	7/14/2022 16:51:37
PB146223BS	S	Phenolics-	P	0.9926	mg/l	7/14/2022 16:51:39
N3214-09	S	Phenolics-	P	0.0275	mg/l	7/14/2022 16:51:41
CCV2	S	Phenolics-	P	0.9865	mg/l	7/14/2022 16:51:43
CCB2	S	Phenolics-	P	-0.0152	mg/l	7/14/2022 16:51:44

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : SM

Instrument ID : Konelab

7/14/2022 14:47

Test Phenolics-


Accepted 7/14/2022 14:47

Factor 9.725

Bias 0.007

Coeff. of det. 0.999757

Errors

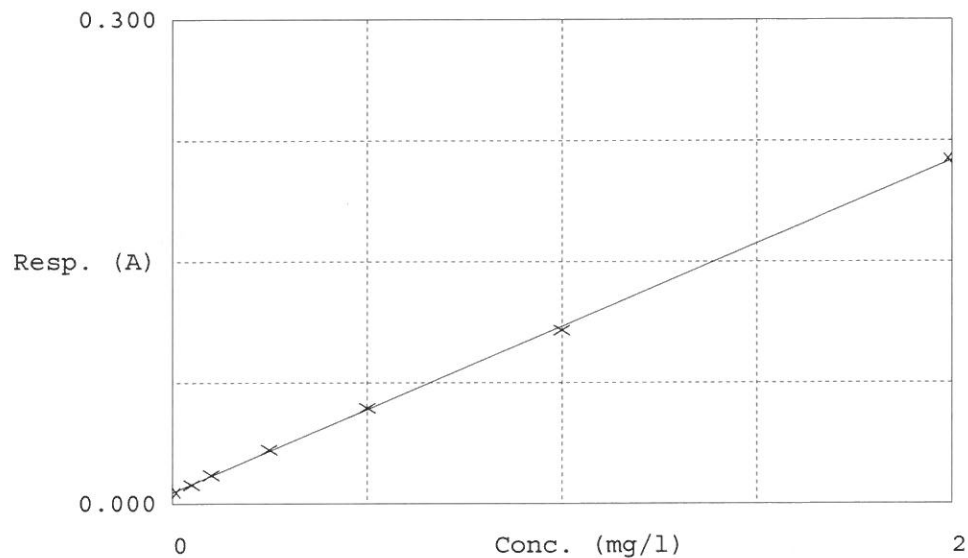

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.007	-0.0005	0.0000	
2	Phenol-2	0.012	0.0460	0.0500	-8.0
3	Phenol-2	0.018	0.1040	0.1000	4.0
4	Phenol-2	0.034	0.2575	0.2500	3.0
5	Phenol-2	0.059	0.5075	0.5000	1.5
6	Phenol-2	0.108	0.9767	1.0000	-2.3
7	Phenol-2	0.214	2.0087	2.0000	0.4

SM
7/14/2022