


63121142

7470A

INSTRUMENT ID: CV1

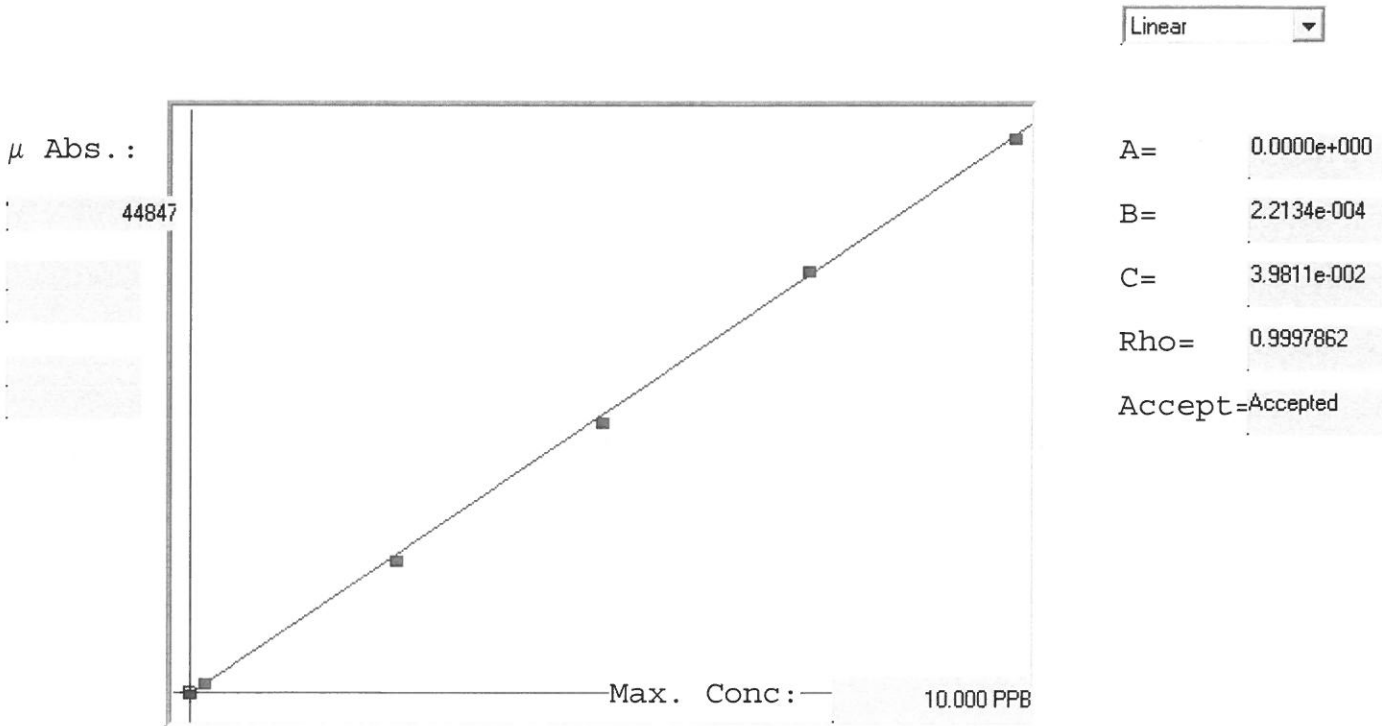

| Std ID | Conc.  | Calc. | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | % D |
|--------|--------|-------|--------|-------|------------|-------|-------|-------|-------|-------|-----|
| 0.0    | 0.000  | 0.043 | 0.043  | 14    | 0.000      | 14    |       |       |       |       | 17  |
| 0.2    | 0.200  | 0.233 | 0.033  | 874   | 0.0 %      | 874   |       |       |       |       | -3  |
| 2.5    | 2.500  | 2.424 | -0.076 | 10772 | 0.0 %      | 10772 |       |       |       |       | -2  |
| 5.0    | 5.000  | 4.906 | -0.094 | 21986 | 0.0 %      | 21986 |       |       |       |       | 2   |
| 7.5    | 7.500  | 7.627 | 0.127  | 34281 | 0.0 %      | 34281 |       |       |       |       | 0   |
| 10.0   | 10.000 | 9.966 | -0.034 | 44847 | 0.0 %      | 44847 |       |       |       |       |     |

## LB121142 INSTRUMENT ID ; CV1

| Method: 7470A   |                 | Operator: Admin |        | Date of Analysis: 20 Jul 2022 12:39:50 |        |       |                      |      |      |
|-----------------|-----------------|-----------------|--------|----------------------------------------|--------|-------|----------------------|------|------|
| Sample ID       | Extended ID     | μ Abs.          | Conc.  | Std Conc                               | Method | Units | Date                 | Type | Type |
| 0.0 - 1         | SP              | 14              | -      | 0.0000                                 | 7470A  | PPB   | 20 Jul 2022 13:35:10 | S    | Std  |
| 0.2 - 1         | SP.2            | 874             | -      | 0.2000                                 | 7470A  | PPB   | 20 Jul 2022 13:37:27 | S    | Std  |
| 2.5 - 1         | SP.5            | 10772           | -      | 2.5000                                 | 7470A  | PPB   | 20 Jul 2022 13:39:44 | S    | Std  |
| 5.0 - 1         | SP.5            | 21986           | -      | 5.0000                                 | 7470A  | PPB   | 20 Jul 2022 13:42:01 | S    | Std  |
| 7.5 - 1         | SP.5            | 34281           | -      | 7.5000                                 | 7470A  | PPB   | 20 Jul 2022 13:44:17 | S    | Std  |
| 10.0 - 1        | SP.5            | 44847           | -      | 10.0000                                | 7470A  | PPB   | 20 Jul 2022 13:46:33 | S    | Std  |
| ICV46 - 1       | ICV46           | 17790           | 3.9774 | -                                      | 7470A  | PPB   | 20 Jul 2022 13:49:19 | U    | SMPL |
| ICB46 - 1       | ICB46           | -78             | 0.0225 | -                                      | 7470A  | PPB   | 20 Jul 2022 13:51:33 | U    | SMPL |
| CCV55 - 1       | CCV55           | 20579           | 4.5947 | -                                      | 7470A  | PPB   | 20 Jul 2022 13:53:48 | U    | SMPL |
| CCB55 - 1       | CCB55           | -78             | 0.0225 | -                                      | 7470A  | PPB   | 20 Jul 2022 13:56:03 | U    | SMPL |
| CRA - 1         | CRA             | 829             | 0.2233 | -                                      | 7470A  | PPB   | 20 Jul 2022 13:58:19 | U    | SMPL |
| HighStd - 1     | HighStd         | 44022           | 9.7835 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:00:34 | U    | SMPL |
| ChkStd - 1      | ChkStd          | 30228           | 6.7304 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:02:49 | U    | SMPL |
| PB146332BL - 1  | PBW             | -95             | 0.0188 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:05:06 | U    | SMPL |
| PB146332BS - 1  | LCSW            | 17561           | 3.9267 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:07:22 | U    | SMPL |
| N3756-03 - 1    | TP-1            | -23             | 0.0347 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:09:38 | U    | SMPL |
| N3756-03DUP - 1 | TP-1DUP         | 170             | 0.0774 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:11:55 | U    | SMPL |
| N3756-03MS - 1  | TP-1MS          | 17602           | 3.9358 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:16:45 | U    | SMPL |
| N3756-03MSD - 1 | TP-1MSD         | 17386           | 3.8880 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:19:01 | U    | SMPL |
| PB146333BL - 1  | PBW             | -66             | 0.0252 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:21:16 | U    | SMPL |
| CCV56 - 1       | CCV56           | 20716           | 4.6250 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:23:32 | U    | SMPL |
| CCB56 - 1       | CCB56           | -70             | 0.0243 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:25:47 | U    | SMPL |
| PB146333BS - 1  | LCSW            | 16881           | 3.7762 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:30:48 | U    | SMPL |
| N3760-03 - 1    | AUD-1821-1822   | 24              | 0.0451 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:33:03 | U    | SMPL |
| N3760-04 - 1    | AUD-1640        | 2445            | 0.5810 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:35:19 | U    | SMPL |
| N3760-05 - 1    | AUD-1645        | 5899            | 1.3455 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:37:35 | U    | SMPL |
| N3760-07 - 1    | AUD-1651        | 837             | 0.2251 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:39:51 | U    | SMPL |
| N3763-02 - 1    | TRE-1279-WATER  | 39157           | 8.7067 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:42:08 | U    | SMPL |
| N3775-01 - 1    | M-R-1           | -80             | 0.0221 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:44:24 | U    | SMPL |
| N3775-03 - 1    | M-R-2           | 37              | 0.0480 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:46:43 | U    | SMPL |
| N3779-01 - 1    | FRAC-TANK-40811 | -29             | 0.0334 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:49:00 | U    | SMPL |
| N3781-01 - 1    | ORA-0037        | 137             | 0.0701 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:51:16 | U    | SMPL |
| CCV57 - 1       | CCV57           | 20698           | 4.6211 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:53:31 | U    | SMPL |
| CCB57 - 1       | CCB57           | -85             | 0.0210 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:55:47 | U    | SMPL |
| N3781-02 - 1    | ORA-0019        | 120             | 0.0664 | -                                      | 7470A  | PPB   | 20 Jul 2022 14:58:02 | U    | SMPL |
| N3781-03 - 1    | ORA-0020        | 300             | 0.1062 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:00:18 | U    | SMPL |
| N3781-04 - 1    | ORA-62322       | 50              | 0.0509 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:02:33 | U    | SMPL |
| N3781-04DUP - 1 | ORA-62322DUP    | 259             | 0.0971 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:04:48 | U    | SMPL |
| N3781-04MS - 1  | ORA-62322MS     | 18172           | 4.0620 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:09:17 | U    | SMPL |
| N3781-04MSD - 1 | ORA-62322MSD    | 16480           | 3.6875 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:11:33 | U    | SMPL |
| PB146336BL - 1  | PBW             | -53             | 0.0281 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:13:48 | U    | SMPL |
| PB146336BS - 1  | LCSW            | 15539           | 3.4792 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:19:02 | U    | SMPL |
| N3767-02 - 1    | TANK-M          | 33              | 0.0471 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:21:18 | U    | SMPL |
| N3767-02DUP - 1 | TANK-MDUP       | 88              | 0.0593 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:23:35 | U    | SMPL |
| CCV58 - 1       | CCV58           | 21009           | 4.6899 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:25:50 | U    | SMPL |
| CCB58 - 1       | CCB58           | -71             | 0.0241 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:28:05 | U    | SMPL |
| N3767-02MS - 1  | TANK-MMS        | 12279           | 2.7576 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:30:21 | U    | SMPL |
| N3767-02MSD - 1 | TANK-MMSD       | 12437           | 2.7926 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:32:36 | U    | SMPL |
| N3767-04 - 1    | TANK-N          | -13             | 0.0369 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:34:52 | U    | SMPL |
| N3767-06 - 1    | TANK-O          | 13              | 0.0427 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:37:09 | U    | SMPL |
| N3767-08 - 1    | TANK-P          | -23             | 0.0347 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:39:25 | U    | SMPL |
| PB146315TB - 1  | PB146315TB      | 1               | 0.0400 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:41:40 | U    | SMPL |
| PB146331TB - 1  | PB146331TB      | 4               | 0.0407 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:43:57 | U    | SMPL |
| CCV59 - 1       | CCV59           | 21383           | 4.7727 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:46:14 | U    | SMPL |
| CCB59 - 1       | CCB59           | -89             | 0.0201 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:48:30 | U    | SMPL |
| N3756-03LX5 - 1 |                 | -28             | 0.0336 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:50:46 | U    | SMPL |
| N3756-03A - 1   |                 | 16415           | 3.6731 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:53:01 | U    | SMPL |
| N3781-04LX5 - 1 |                 | -13             | 0.0369 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:55:16 | U    | SMPL |
| N3781-04A - 1   |                 | 18833           | 4.2083 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:57:32 | U    | SMPL |
| N3767-02LX5 - 1 |                 | -80             | 0.0221 | -                                      | 7470A  | PPB   | 20 Jul 2022 15:59:47 | U    | SMPL |
| N3767-02A - 1   |                 | 17085           | 3.8214 | -                                      | 7470A  | PPB   | 20 Jul 2022 16:02:03 | U    | SMPL |
| CCV60 - 1       | CCV60           | 21334           | 4.7618 | -                                      | 7470A  | PPB   | 20 Jul 2022 16:04:18 | U    | SMPL |
| CCB60 - 1       | CCB60           | -61             | 0.0263 | -                                      | 7470A  | PPB   | 20 Jul 2022 16:06:34 | U    | SMPL |