

LB121176

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

7/21/2022 14:25

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	94.707	0.0	0.097	
ICB001 ICB001	1.223	0.0	0.009	
CCV001 CCV001	239.030	0.0	0.235	
CCB001 CCB001	1.060	0.0	0.009	
PB146280BL PBS280	0.983	0.0	0.008	
N3723-22 X3B73	143.207	0.0	0.144	
N3723-23 X3B73D	143.523	0.0	0.144	
N3723-24 X3B73S	236.179	0.0	0.232	
PB146281BL PBW281	0.842	0.0	0.008	
N3723-10 X3B69	115.699	0.0	0.117	
N3723-11 X3B69D	116.928	0.0	0.119	
N3723-12 X3B69S	215.685	0.0	0.212	
CCV002 CCV002	254.034	0.0	0.249	
CCB002 CCB002	2.063	0.0	0.009	

N 14
Mean 111.797
SD 98.5010
CV% 88.11

12
7/21/22

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 21 13:17:56 2022

Thu Jul 21 14:21:41 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		0.556	µg/l	7/21/2022 11:20:17
S5.0	A	CNEPA-NE\ P		5.3449	µg/l	7/21/2022 11:20:18
S10.0	A	CNEPA-NE\ P		10.3042	µg/l	7/21/2022 11:20:19
S100.0	A	CNEPA-NE\ P		98.8821	µg/l	7/21/2022 11:20:20
S250.0	A	CNEPA-NE\ P		249.3975	µg/l	7/21/2022 11:20:21
S500.0	A	CNEPA-NE\ P		500.5153	µg/l	7/21/2022 11:20:22
ICV001 ICV001	S	CNEPA-NE\ P		94.7073	µg/l	7/21/2022 14:08:47
ICB001 ICB001	S	CNEPA-NE\ P		1.2226	µg/l	7/21/2022 14:08:48
CCV001 CCV001	S	CNEPA-NE\ P		239.0303	µg/l	7/21/2022 14:08:51
CCB001 CCB001	S	CNEPA-NE\ P		1.0601	µg/l	7/21/2022 14:08:53
PB146280BL PBS280	S	CNEPA-NE\ P		0.9825	µg/l	7/21/2022 14:08:54
N3723-22 X3B73	S	CNEPA-NE\ P		143.2071	µg/l	7/21/2022 14:16:21
N3723-23 X3B73D	S	CNEPA-NE\ P		143.5229	µg/l	7/21/2022 14:16:22
N3723-24 X3B73S	S	CNEPA-NE\ P		236.1786	µg/l	7/21/2022 14:16:24
PB146281BL PBW281	S	CNEPA-NE\ P		0.8421	µg/l	7/21/2022 14:16:30
N3723-10 X3B69	S	CNEPA-NE\ P		115.6993	µg/l	7/21/2022 14:21:36
N3723-11 X3B69D	S	CNEPA-NE\ P		116.9278	µg/l	7/21/2022 14:21:38
N3723-12 X3B69S	S	CNEPA-NE\ P		215.6853	µg/l	7/21/2022 14:21:39
CCV002 CCV002	S	CNEPA-NE\ P		254.0337	µg/l	7/21/2022 14:21:40
CCB002 CCB002	S	CNEPA-NE\ P		2.0625	µg/l	7/21/2022 14:21:41

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

7/21/2022 11:20

Test CNEPA-NEW


Accepted 7/21/2022 11:20

Factor *Slope* 1053 0.000950
Bias *Y-intercept* 0.008

12/7/22/22

Coeff. of det. 0.999988

Errors

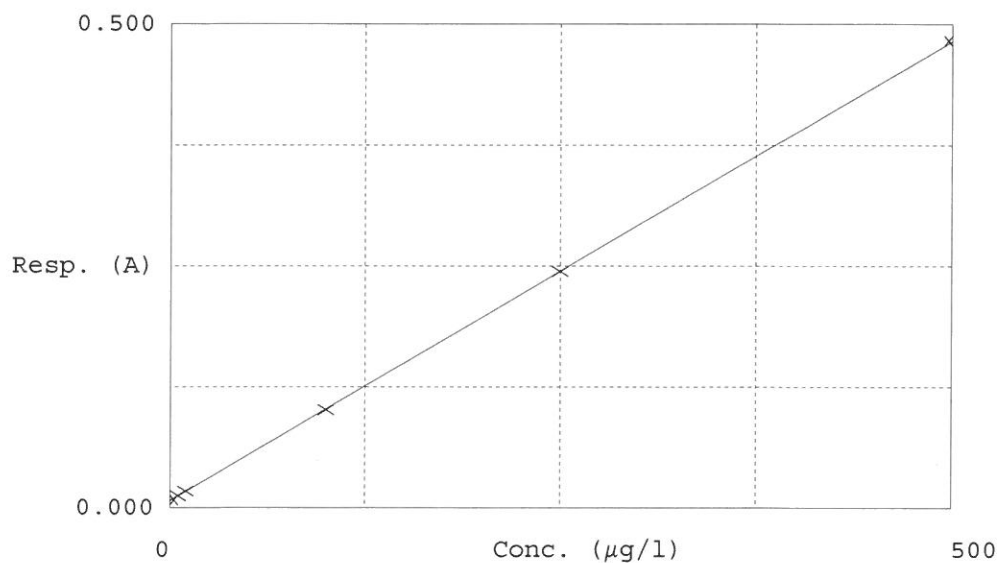

	Calibrator	Response	Calc. con.	Conc.	<i>Re</i> Errors
1	0.0PPBCN	0.008	0.5560	0.0000	-
2	5.0PPBCN	0.013	5.3449	5.0000	6.9
3	10PPBCN	0.017	10.3042	10.0000	3.0
4	100PPBCN	0.101	98.8821	100.0000	-1.1
5	250PPBCN	0.244	249.3975	250.0000	-0.2
6	500PPBCN	0.483	500.5153	500.0000	0.1

12
7/21/22