

LB121188


7470A

INSTRUMENT ID: CVT

Linear

 μ Abs.:

39458

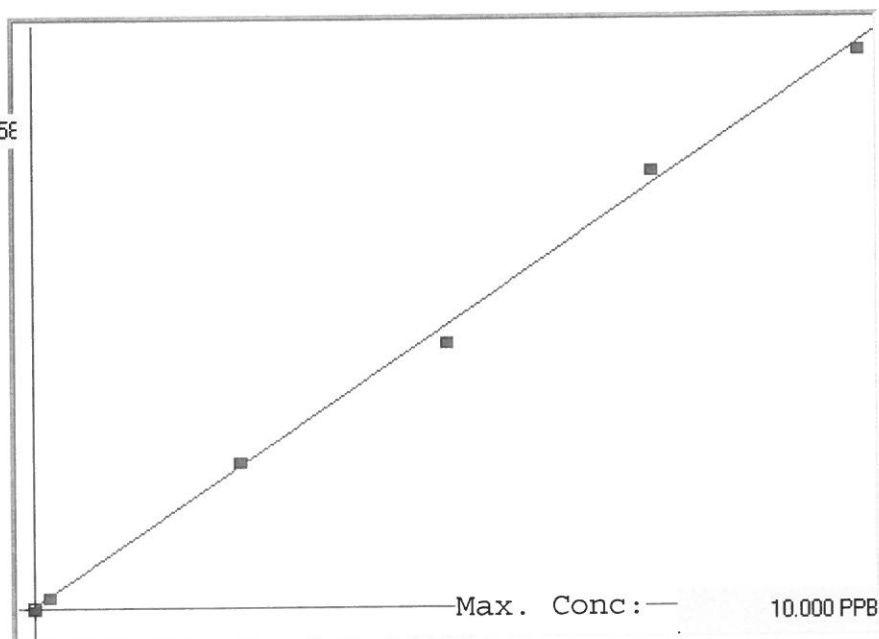

A= 0.0000e+000

B= 2.5087e-004

C= -1.3324e-002

Rho= 0.9989101

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.000	-0.000	52	0.000	52					4
0.2	0.200	0.208	0.008	883	0.0 %	883					4
2.5	2.500	2.605	0.105	10437	0.0 %	10437					6
5.0	5.000	4.724	-0.276	18882	0.0 %	18882					4
7.5	7.500	7.778	0.278	31058	0.0 %	31058					1
10.0	10.000	9.885	-0.115	39458	0.0 %	39458					

LB121188 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 22 Jul 2022 12:27:29					
Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	52	-	0.0000	7470A	PPB	22 Jul 2022 13:18:23	S	Std
0.2 - 1	50.2	883	-	0.2000	7470A	PPB	22 Jul 2022 13:20:40	S	Std
2.5 - 1	52.5	10437	-	2.5000	7470A	PPB	22 Jul 2022 13:22:57	S	Std
5.0 - 1	55	18882	-	5.0000	7470A	PPB	22 Jul 2022 13:25:13	S	Std
7.5 - 1	57.5	31058	-	7.5000	7470A	PPB	22 Jul 2022 13:30:08	S	Std
10.0 - 1	59.0	39458	-	10.0000	7470A	PPB	22 Jul 2022 13:40:04	S	Std
ICV49 - 1	ICV49	16930	4.2339	-	7470A	PPB	22 Jul 2022 13:42:51	U	SMPL
ICB49 - 1	ICB49	8	-0.0113	-	7470A	PPB	22 Jul 2022 13:45:05	U	SMPL
CCV68 - 1	CCV68	19882	4.9744	-	7470A	PPB	22 Jul 2022 13:47:20	U	SMPL
CCB68 - 1	CCB68	10	-0.0108	-	7470A	PPB	22 Jul 2022 13:49:36	U	SMPL
CRA - 1	CRA	867	0.2042	-	7470A	PPB	22 Jul 2022 13:51:51	U	SMPL
HighStd - 1	HighStd	39368	9.8628	-	7470A	PPB	22 Jul 2022 13:54:06	U	SMPL
ChkStd - 1	ChkStd	29242	7.3226	-	7470A	PPB	22 Jul 2022 13:56:21	U	SMPL
PB146395BL - 1	PBW	-45	-0.0246	-	7470A	PPB	22 Jul 2022 13:58:38	U	SMPL
PB146395BS - 1	LCSW	14761	3.6897	-	7470A	PPB	22 Jul 2022 14:03:31	U	SMPL
N3789-01 - 1	IDW-VB1-071922	108	0.0138	-	7470A	PPB	22 Jul 2022 14:05:47	U	SMPL
N3794-01 - 1	8187	147	0.0236	-	7470A	PPB	22 Jul 2022 14:08:03	U	SMPL
N3815-03 - 1	MH-190E	92	0.0098	-	7470A	PPB	22 Jul 2022 14:10:20	U	SMPL
N3830-06 - 1	HS-SOIL-0721	98	0.0113	-	7470A	PPB	22 Jul 2022 14:12:37	U	SMPL
N3832-01 - 1	MMC-DRUMS-0721	93	0.0100	-	7470A	PPB	22 Jul 2022 14:14:52	U	SMPL
CCV69 - 1	CCV69	20040	5.0141	-	7470A	PPB	22 Jul 2022 14:23:07	U	SMPL
CCB69 - 1	CCB69	45	-0.0020	-	7470A	PPB	22 Jul 2022 14:25:22	U	SMPL
N3835-03 - 1	MH-191E	108	0.0138	-	7470A	PPB	22 Jul 2022 14:27:37	U	SMPL
N3835-03DUP - 1	MH-191EDUP	115	0.0155	-	7470A	PPB	22 Jul 2022 14:29:52	U	SMPL
N3835-03MS - 1	MH-191EMS	15370	3.8425	-	7470A	PPB	22 Jul 2022 14:32:07	U	SMPL
N3835-03MSD - 1	MH-191EMSD	17324	4.3327	-	7470A	PPB	22 Jul 2022 14:34:23	U	SMPL
PB146396BL - 1	PBW	42	-0.0028	-	7470A	PPB	22 Jul 2022 14:36:39	U	SMPL
PB146396BS - 1	LCSW	13551	3.3862	-	7470A	PPB	22 Jul 2022 14:38:56	U	SMPL
N3806-02 - 1	FRAC-TANK-N48964	386	0.0835	-	7470A	PPB	22 Jul 2022 14:41:13	U	SMPL
N3813-05 - 1	QUEENS54A-WC-20220720	219	0.0416	-	7470A	PPB	22 Jul 2022 14:43:30	U	SMPL
N3813-05DUP - 1	QUEENS54A-WC-20220720DUP	107	0.0135	-	7470A	PPB	22 Jul 2022 14:45:47	U	SMPL
N3813-05MS - 1	QUEENS54A-WC-20220720MS	14371	3.5919	-	7470A	PPB	22 Jul 2022 14:48:02	U	SMPL
CCV70 - 1	CCV70	18618	4.6573	-	7470A	PPB	22 Jul 2022 14:55:32	U	SMPL
CCB70 - 1	CCB70	13	-0.0101	-	7470A	PPB	22 Jul 2022 14:57:47	U	SMPL
N3813-05MSD - 1	QUEENS54A-WC-20220720MSD	14917	3.7289	-	7470A	PPB	22 Jul 2022 15:00:04	U	SMPL
PB14648TB - 1	PB14648TB	63	0.0025	-	7470A	PPB	22 Jul 2022 15:02:19	U	SMPL
N3835-03LX5 - 1		4	-0.0123	-	7470A	PPB	22 Jul 2022 15:04:35	U	SMPL
N3835-03A - 1		16674	4.1696	-	7470A	PPB	22 Jul 2022 15:06:51	U	SMPL
N3813-05LX5 - 1		-11	-0.0161	-	7470A	PPB	22 Jul 2022 15:09:07	U	SMPL
N3813-05A - 1		16582	4.1466	-	7470A	PPB	22 Jul 2022 15:11:23	U	SMPL
CCV71 - 1	CCV71	19309	4.8307	-	7470A	PPB	22 Jul 2022 15:16:13	U	SMPL
CCB71 - 1	CCB71	-1	-0.0136	-	7470A	PPB	22 Jul 2022 15:18:29	U	SMPL