


LB121257

7470A

INSTRUMENT ID: CV1

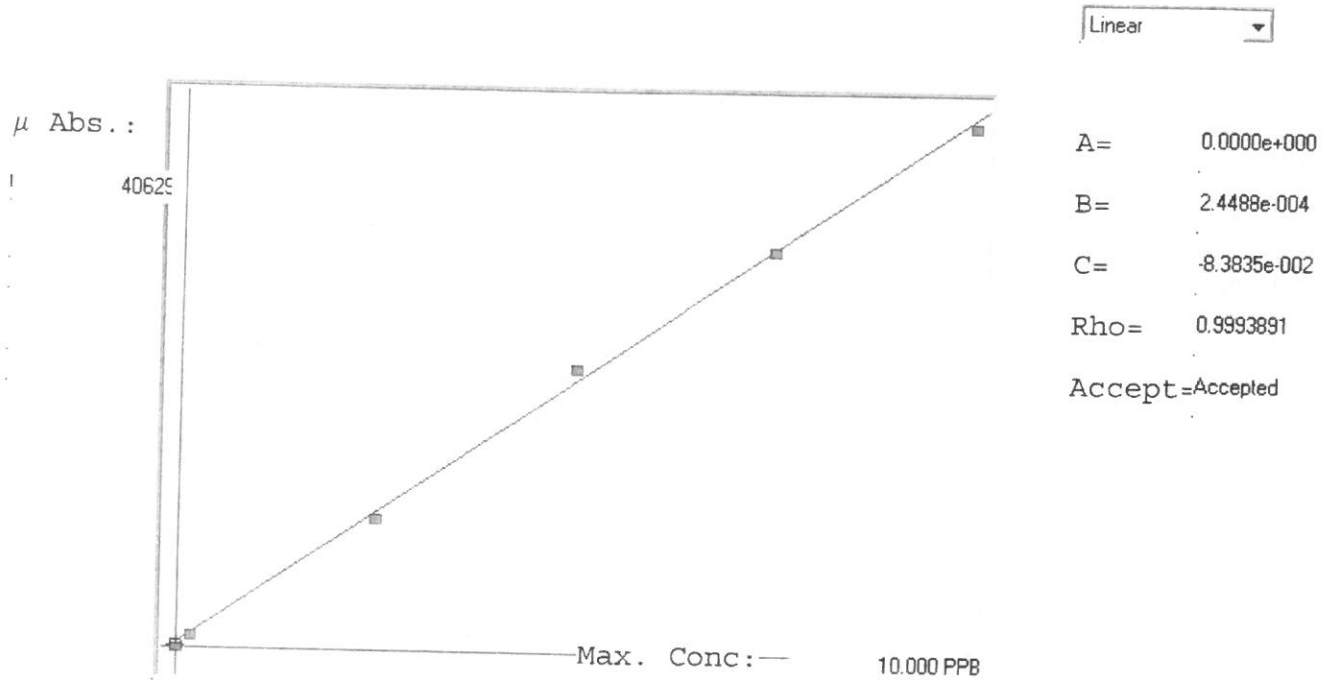

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.047	-0.047	150	0.000	150					
0.2	0.200	0.182	-0.018	1084	0.0 %	1084					-9
2.5	2.500	2.416	-0.084	10209	0.0 %	10209					-3
5.0	5.000	5.268	0.268	21855	0.0 %	21855					5
7.5	7.500	7.516	0.016	31035	0.0 %	31035					0
10.0	10.000	9.865	-0.135	40629	0.0 %	40629					-1

LB121257 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Jul 2022 09:36:10

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	150	-	0.00007470A	PPB	28 Jul 2022 09:42:22	S	Std
0.2 - 1	50.2	1084	-	0.20007470A	PPB	28 Jul 2022 09:44:38	S	Std
2.5 - 1	52.5	10209	-	2.50007470A	PPB	28 Jul 2022 09:46:55	S	Std
5.0 - 1	55	21855	-	5.00007470A	PPB	28 Jul 2022 09:49:13	S	Std
7.5 - 1	57.5	31035	-	7.50007470A	PPB	28 Jul 2022 09:51:29	S	Std
10.0 - 1	59.1	40629	-	10.00007470A	PPB	28 Jul 2022 09:53:45	S	Std
ICV57 - 1	ICV57	16823	4.0358	-7470A	PPB	28 Jul 2022 10:00:58	U	SMPL
ICB57 - 1	ICB57	-22	-0.0892	-7470A	PPB	28 Jul 2022 10:03:12	U	SMPL
CCV96 - 1	CCV96	21055	5.0721	-7470A	PPB	28 Jul 2022 10:05:29	U	SMPL
CCB96 - 1	CCB96	-25	-0.0900	-7470A	PPB	28 Jul 2022 10:07:44	U	SMPL
CRA - 1	CRA	843	0.1226	-7470A	PPB	28 Jul 2022 10:10:00	U	SMPL
CRA - 1	CRA	1138	0.1948	-7470A	PPB	28 Jul 2022 10:14:07	U	SMPL
HighStd - 1	HighStd	43129	10.4776	-7470A	PPB	28 Jul 2022 10:16:21	U	SMPL
ChkStd - 1	ChkStd	31315	7.5846	-7470A	PPB	28 Jul 2022 10:18:36	U	SMPL
PB146521BL - 1	PBW	118	-0.0549	-7470A	PPB	28 Jul 2022 10:23:34	U	SMPL
PB146521BS - 1	LCSW	15062	3.6045	-7470A	PPB	28 Jul 2022 10:25:49	U	SMPL
N3891-03 - 1	4553-E	14	-0.0804	-7470A	PPB	28 Jul 2022 10:28:06	U	SMPL
N3891-06 - 1	TP-1	112	-0.0564	-7470A	PPB	28 Jul 2022 10:30:25	U	SMPL
N3891-09 - 1	7897-W	109	-0.0571	-7470A	PPB	28 Jul 2022 10:32:41	U	SMPL
N3898-01 - 1	61422-A-OIL-LAYER	642	0.0734	-7470A	PPB	28 Jul 2022 10:34:59	U	SMPL
N3912-03 - 1	6601-S	84	-0.0633	-7470A	PPB	28 Jul 2022 10:37:15	U	SMPL
CCV97 - 1	CCV97	21895	5.2778	-7470A	PPB	28 Jul 2022 10:39:30	U	SMPL
CCB97 - 1	CCB97	230	-0.0275	-7470A	PPB	28 Jul 2022 10:44:23	U	SMPL
N3914-01 - 1	METRO-DISP	126	-0.0530	-7470A	PPB	28 Jul 2022 10:46:38	U	SMPL
N3914-01DUP - 1	METRO-DISPDUP	147	-0.0478	-7470A	PPB	28 Jul 2022 10:48:54	U	SMPL
N3914-01MS - 1	METRO-DISPMMS	14304	3.4189	-7470A	PPB	28 Jul 2022 10:51:09	U	SMPL
N3914-01MSD - 1	METRO-DISPMSD	15172	3.6315	-7470A	PPB	28 Jul 2022 10:55:59	U	SMPL
N3914-01LX5 - 1		13	-0.0807	-7470A	PPB	28 Jul 2022 11:00:34	U	SMPL
N3914-01A - 1		16218	3.8876	-7470A	PPB	28 Jul 2022 11:02:51	U	SMPL
PB146475TB - 1	PB146475TB	236	-0.0260	-7470A	PPB	28 Jul 2022 11:10:25	U	SMPL
CCV98 - 1	CCV98	22049	5.3155	-7470A	PPB	28 Jul 2022 11:12:55	U	SMPL
CCB98 - 1	CCB98	267	-0.0185	-7470A	PPB	28 Jul 2022 11:17:45	U	SMPL