


LB121279

7470A

INSTRUMENT ID: CV4

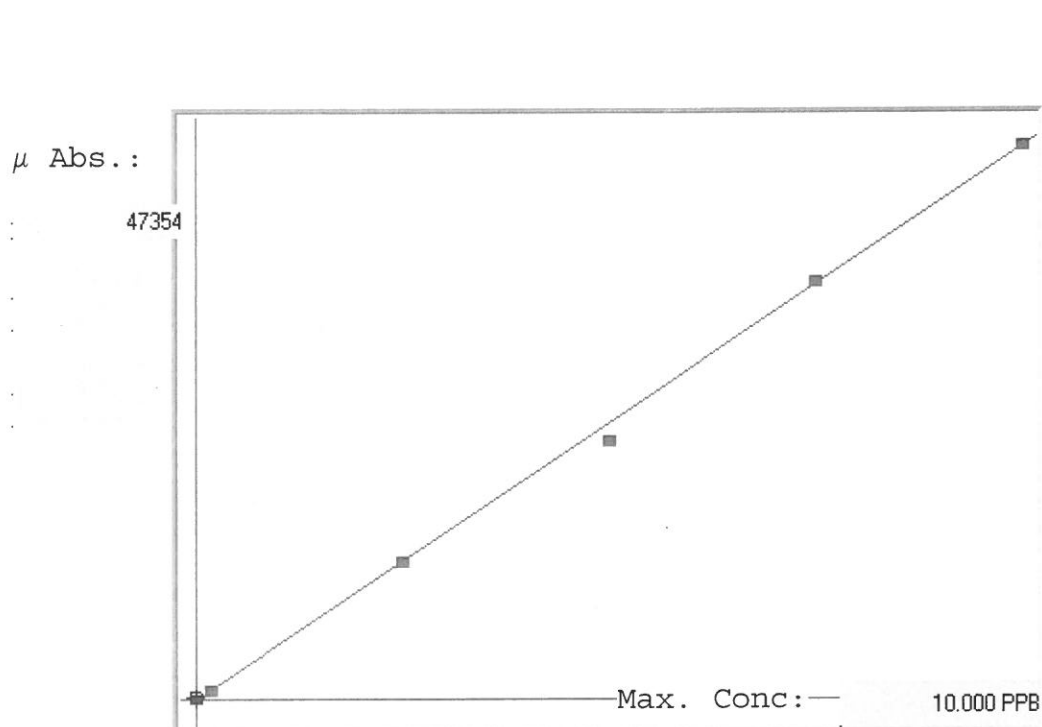

A= 0.0000e+000

B= 2.1144e-004

C= 2.4937e-002

Rho= 0.9994370

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	905
0.0	0.000	0.076	0.076	243	0.000	243					1
0.2	0.200	0.202	0.002	839	0.0 %	839					2
2.5	2.500	2.554	0.054	11959	0.0 %	11959					5
5.0	5.000	4.731	-0.269	22259	0.0 %	22259					0
7.5	7.500	7.599	0.099	35819	0.0 %	35819					
10.0	10.000	10.038	0.038	47354	0.0 %	47354					

LB121279 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Jul 2022 10:25:40				
Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	SP	243	-	0.00007470A	PPB	29 Jul 2022 10:46:39	S	Std
0.2 - 1	SP-2	839	-	0.20007470A	PPB	29 Jul 2022 10:48:55	S	Std
2.5 - 1	SP-1	11959	-	2.50007470A	PPB	29 Jul 2022 10:51:12	S	Std
5.0 - 1	SP-5	22259	-	5.00007470A	PPB	29 Jul 2022 10:53:29	S	Std
7.5 - 1	SP-10	35819	-	7.50007470A	PPB	29 Jul 2022 10:55:45	S	Std
10.0 - 1	SP-10	47354	-	10.00007470A	PPB	29 Jul 2022 10:58:01	S	Std
ICV59 - 1	ICV59	17437	3.7119	-7470A	PPB	29 Jul 2022 11:00:57	U	SMPL
ICB59 - 1	ICB59	-28	0.0190	-7470A	PPB	29 Jul 2022 11:03:12	U	SMPL
CCV08 - 1	CCV08	24682	5.2438	-7470A	PPB	29 Jul 2022 11:10:31	U	SMPL
CCB08 - 1	CCB08	-48	0.0148	-7470A	PPB	29 Jul 2022 11:12:46	U	SMPL
CRA - 1	CRA	829	0.2002	-7470A	PPB	29 Jul 2022 11:15:01	U	SMPL
HighStd - 1	HighStd	46157	9.7845	-7470A	PPB	29 Jul 2022 11:17:16	U	SMPL
ChkStd - 1	ChkStd	32174	6.8279	-7470A	PPB	29 Jul 2022 11:19:32	U	SMPL
PB146522BL - 1	PBW	-1	0.0247	-7470A	PPB	29 Jul 2022 11:23:42	U	SMPL
PB146522BS - 1	LCSW	19308	4.1075	-7470A	PPB	29 Jul 2022 11:29:20	U	SMPL
N3898-02 - 1	61422-A	928	0.2212	-7470A	PPB	29 Jul 2022 11:31:36	U	SMPL
N3898-04 - 1	61422-D	764	0.1865	-7470A	PPB	29 Jul 2022 11:36:28	U	SMPL
N3898-07 - 1	62422	23085	4.9061	-7470A	PPB	29 Jul 2022 11:38:44	U	SMPL
N3916-03 - 1	998	154	0.0575	-7470A	PPB	29 Jul 2022 11:41:01	U	SMPL
CCV09 - 1	CCV09	24161	5.1336	-7470A	PPB	29 Jul 2022 11:45:54	U	SMPL
CCB09 - 1	CCB09	-29	0.0188	-7470A	PPB	29 Jul 2022 11:50:38	U	SMPL
N3953-01 - 1	IRV-OILY-WATER	231	0.0738	-7470A	PPB	29 Jul 2022 11:52:53	U	SMPL
N3953-01DUP - 1	IRV-OILY-WATERDUP	216	0.0706	-7470A	PPB	29 Jul 2022 11:55:09	U	SMPL
N3953-01MS - 1	IRV-OILY-WATERMS	17981	3.8269	-7470A	PPB	29 Jul 2022 11:59:55	U	SMPL
N3953-01MSD - 1	IRV-OILY-WATERMSD	18561	3.9495	-7470A	PPB	29 Jul 2022 12:02:10	U	SMPL
N3958-02 - 1	RW9-IDWGW-20220727	-60	0.0123	-7470A	PPB	29 Jul 2022 12:04:26	U	SMPL
N3964-07 - 1	HMGP-WATER-1	455	0.1211	-7470A	PPB	29 Jul 2022 12:06:42	U	SMPL
N3964-08 - 1	HMGP-WATER-2	3137	0.6882	-7470A	PPB	29 Jul 2022 12:08:58	U	SMPL
N3953-01LX5 - 1		-14	0.0220	-7470A	PPB	29 Jul 2022 12:11:14	U	SMPL
N3953-01A - 1		19345	4.1153	-7470A	PPB	29 Jul 2022 12:13:31	U	SMPL
CCV10 - 1	CCV10	25675	5.4538	-7470A	PPB	29 Jul 2022 12:15:48	U	SMPL
CCB10 - 1	CCB10	-102	0.0034	-7470A	PPB	29 Jul 2022 12:18:03	U	SMPL