


LB121319

7471B

INSTRUMENT ID: CV1

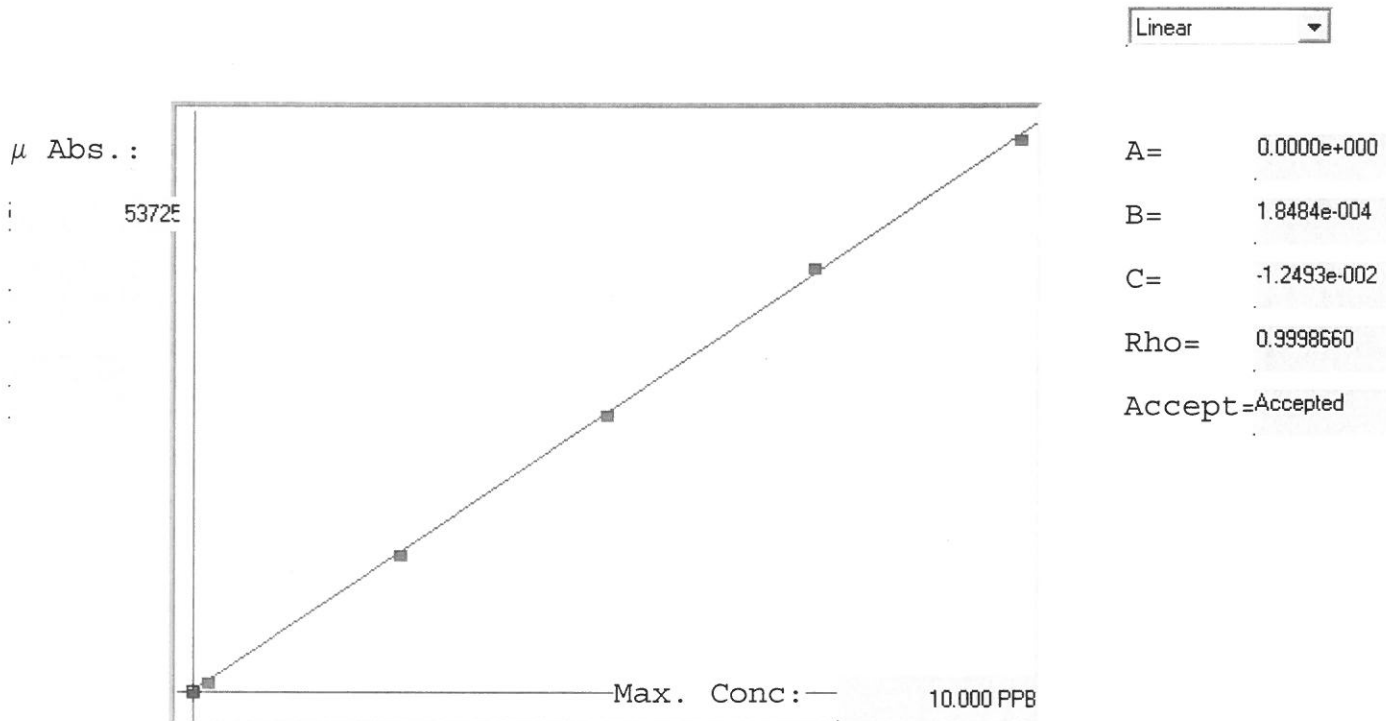

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%1)
0.0	0.000	0.002	0.002	78	0.000	78					
0.2	0.200	0.188	-0.012	1086	0.0 %	1086					-6
2.5	2.500	2.485	-0.015	13511	0.0 %	13511					-1
5.0	5.000	4.986	-0.014	27040	0.0 %	27040					0
7.5	7.500	7.621	0.121	41297	0.0 %	41297					2
10.0	10.000	9.918	-0.082	53725	0.0 %	53725					-1

LB121319 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Aug 2022 07:02:19

Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	78	-	0.0000	7471B	PPB	02 Aug 2022 07:11:22	S	Std
0.2 - 1	502	1086	-	0.2000	7471B	PPB	02 Aug 2022 07:13:39	S	Std
2.5 - 1	52.5	13511	-	2.5000	7471B	PPB	02 Aug 2022 07:15:56	S	Std
5.0 - 1	55	27040	-	5.0000	7471B	PPB	02 Aug 2022 07:18:14	S	Std
7.5 - 1	59.5	41297	-	7.5000	7471B	PPB	02 Aug 2022 07:20:30	S	Std
10.0 - 1	510	53725	-	10.0000	7471B	PPB	02 Aug 2022 07:25:22	S	Std
ICV62 - 1	ICV62	22036	4.0607	-	7471B	PPB	02 Aug 2022 07:28:09	U	SMPL
ICB62 - 1	ICB62	-43	-0.0204	-	7471B	PPB	02 Aug 2022 07:30:24	U	SMPL
CCV23 - 1	CCV23	25410	4.6844	-	7471B	PPB	02 Aug 2022 07:32:41	U	SMPL
CCB23 - 1	CCB23	-56	-0.0228	-	7471B	PPB	02 Aug 2022 07:34:56	U	SMPL
CRA - 1	CRA	1074	0.1860	-	7471B	PPB	02 Aug 2022 07:37:13	U	SMPL
HighStd - 1	HighStd	54867	10.1293	-	7471B	PPB	02 Aug 2022 07:39:28	U	SMPL
ChkStd - 1	ChkStd	38796	7.1587	-	7471B	PPB	02 Aug 2022 07:41:44	U	SMPL
PB146644BL - 1	PBS	-44	-0.0206	-	7471B	PPB	02 Aug 2022 07:44:02	U	SMPL
PB146644BS - 1	LCSS	18493	3.4058	-	7471B	PPB	02 Aug 2022 07:51:31	U	SMPL
N3970-01 - 1	MHB-UPPER	18595	3.4247	-	7471B	PPB	02 Aug 2022 07:53:48	U	SMPL
N3970-04 - 1	MHB-LOWER	681	0.1134	-	7471B	PPB	02 Aug 2022 07:56:06	U	SMPL
N3970-04DUP - 1	MHB-LOWERDUP	850	0.1446	-	7471B	PPB	02 Aug 2022 08:01:09	U	SMPL
N3970-04MS - 1	MHB-LOWERMS	20895	3.8498	-	7471B	PPB	02 Aug 2022 08:03:26	U	SMPL
N3970-04MSD - 1	MHB-LOWERMSD	22053	4.0639	-	7471B	PPB	02 Aug 2022 08:05:41	U	SMPL
CCV24 - 1	CCV24	27522	5.0748	-	7471B	PPB	02 Aug 2022 08:07:58	U	SMPL
CCB24 - 1	CCB24	-60	-0.0236	-	7471B	PPB	02 Aug 2022 08:10:14	U	SMPL
N3973-01 - 1	RO-72-11940	1171	0.2040	-	7471B	PPB	02 Aug 2022 08:12:31	U	SMPL
N3976-01 - 1	TP1-0729	1453	0.2561	-	7471B	PPB	02 Aug 2022 08:15:23	U	SMPL
N3976-03 - 1	TP2-0729	80308	14.8319	-	7471B	PPB	02 Aug 2022 08:17:38	U	SMPL
N3976-05 - 1	TP3-0729	673645	HIGH	-	7471B	PPB	02 Aug 2022 08:19:54	X	
N3979-01 - 1	TR-06-072922	1648	0.2921	-	7471B	PPB	02 Aug 2022 08:21:47	U	SMPL
N3982-01 - 1	OR-3-072922	1110	0.1927	-	7471B	PPB	02 Aug 2022 08:24:14	U	SMPL
PB146645BL - 1	PBS	12	-0.0103	-	7471B	PPB	02 Aug 2022 08:26:30	U	SMPL
PB146645BS - 1	LCSS	20873	3.8457	-	7471B	PPB	02 Aug 2022 08:28:47	U	SMPL
N3927-01 - 1	RVE-75	723	0.1211	-	7471B	PPB	02 Aug 2022 08:31:04	U	SMPL
N3927-01DUP - 1	RVE-75DUP	820	0.1391	-	7471B	PPB	02 Aug 2022 08:33:20	U	SMPL
CCV25 - 1	CCV25	27349	5.0428	-	7471B	PPB	02 Aug 2022 08:35:36	U	SMPL
CCB25 - 1	CCB25	-46	-0.0210	-	7471B	PPB	02 Aug 2022 08:37:51	U	SMPL
N3927-01MS - 1	RVE-75MS	22667	4.1774	-	7471B	PPB	02 Aug 2022 08:40:08	U	SMPL
N3927-01MSD - 1	RVE-75MSD	20359	3.7507	-	7471B	PPB	02 Aug 2022 08:47:36	U	SMPL
N3927-02 - 1	RVE-76	150	0.0152	-	7471B	PPB	02 Aug 2022 08:49:51	U	SMPL
N3927-03 - 1	RVE-77	326	0.0478	-	7471B	PPB	02 Aug 2022 09:05:40	U	SMPL
N3927-04 - 1	RVE-78	218	0.0278	-	7471B	PPB	02 Aug 2022 09:07:56	U	SMPL
N3927-05 - 1	RVE-79	236	0.0311	-	7471B	PPB	02 Aug 2022 09:10:13	U	SMPL
N3927-06 - 1	RVE-79D	222	0.0285	-	7471B	PPB	02 Aug 2022 09:12:29	U	SMPL
N3927-07 - 1	RVE-80	341	0.0505	-	7471B	PPB	02 Aug 2022 09:14:46	U	SMPL
N3927-08 - 1	RVE-81	1046	0.1809	-	7471B	PPB	02 Aug 2022 09:17:03	U	SMPL
N3927-09 - 1	RVE-82	5222	0.9528	-	7471B	PPB	02 Aug 2022 09:19:19	U	SMPL
CCV26 - 1	CCV26	27217	5.0184	-	7471B	PPB	02 Aug 2022 09:21:35	U	SMPL
CCB26 - 1	CCB26	-22	-0.0166	-	7471B	PPB	02 Aug 2022 09:23:50	U	SMPL
N3927-10 - 1	RVE-83	7315	1.3396	-	7471B	PPB	02 Aug 2022 09:26:07	U	SMPL
N3927-11 - 1	RVE-84	2197	0.3936	-	7471B	PPB	02 Aug 2022 09:28:22	U	SMPL
N3927-12 - 1	RVE-85	4269	0.7766	-	7471B	PPB	02 Aug 2022 09:30:38	U	SMPL
N3927-13 - 1	RVE-86	3494	0.6334	-	7471B	PPB	02 Aug 2022 09:32:54	U	SMPL
N3927-14 - 1	RVE-87	3508	0.6359	-	7471B	PPB	02 Aug 2022 09:35:11	U	SMPL
N3927-15 - 1	RVE-88	2585	0.4653	-	7471B	PPB	02 Aug 2022 09:37:27	U	SMPL
N3927-16 - 1	RVE-89	2821	0.5090	-	7471B	PPB	02 Aug 2022 09:39:44	U	SMPL
N3927-17 - 1	RVE-90	2643	0.4760	-	7471B	PPB	02 Aug 2022 09:42:01	U	SMPL
N3927-18 - 1	RVE-91	3026	0.5468	-	7471B	PPB	02 Aug 2022 09:44:18	U	SMPL
N3927-19 - 1	RVE-92	3138	0.5675	-	7471B	PPB	02 Aug 2022 09:46:33	U	SMPL
CCV27 - 1	CCV27	27757	5.1182	-	7471B	PPB	02 Aug 2022 09:48:49	U	SMPL
CCB27 - 1	CCB27	-27	-0.0175	-	7471B	PPB	02 Aug 2022 09:51:05	U	SMPL
N3927-20 - 1	RVE-93	2560	0.4607	-	7471B	PPB	02 Aug 2022 09:53:21	U	SMPL
PB146646BL - 1	PBS	16	-0.0095	-	7471B	PPB	02 Aug 2022 09:55:37	U	SMPL
PB146646BS - 1	LCSS	20467	3.7707	-	7471B	PPB	02 Aug 2022 09:57:53	U	SMPL
N3930-01 - 1	RVE-94	2700	0.4866	-	7471B	PPB	02 Aug 2022 10:00:09	U	SMPL
N3930-01DUP - 1	RVE-94DUP	2659	0.4790	-	7471B	PPB	02 Aug 2022 10:04:41	U	SMPL
N3930-01MS - 1	RVE-94MS	23314	4.2970	-	7471B	PPB	02 Aug 2022 10:06:57	U	SMPL
N3930-01MSD - 1	RVE-94MSD	22794	4.2008	-	7471B	PPB	02 Aug 2022 10:09:14	U	SMPL
N3930-02 - 1	RVE-95	3572	0.6478	-	7471B	PPB	02 Aug 2022 10:11:32	U	SMPL
N3930-03 - 1	RVE-96	3813	0.6923	-	7471B	PPB	02 Aug 2022 10:13:50	U	SMPL
N3930-04 - 1	RVE-97	3293	0.5962	-	7471B	PPB	02 Aug 2022 10:16:06	U	SMPL
CCV28 - 1	CCV28	27872	5.1395	-	7471B	PPB	02 Aug 2022 10:18:23	U	SMPL
CCB28 - 1	CCB28	-27	-0.0175	-	7471B	PPB	02 Aug 2022 10:20:39	U	SMPL
N3930-05 - 1	RVE-98	2852	0.5147	-	7471B	PPB	02 Aug 2022 10:22:57	U	SMPL
N3930-06 - 1	RVE-99	2543	0.4576	-	7471B	PPB	02 Aug 2022 10:25:13	U	SMPL
N3930-07 - 1	RVE-99D	2890	0.5217	-	7471B	PPB	02 Aug 2022 10:27:29	U	SMPL
N3930-08 - 1	RVE-100	2591	0.4664	-	7471B	PPB	02 Aug 2022 10:29:45	U	SMPL
N3930-09 - 1	RVE-101	7632	1.3982	-	7471B	PPB	02 Aug 2022 10:32:01	U	SMPL
N3930-10 - 1	RVE-102	2583	0.4650	-	7471B	PPB	02 Aug 2022 10:34:17	U	SMPL
N3930-11 - 1	RVE-103	1875	0.3341	-	7471B	PPB	02 Aug 2022 10:36:34	U	SMPL
N3930-12 - 1	RVE-104	4534	0.8256	-	7471B	PPB	02 Aug 2022 10:38:51	U	SMPL
N3930-13 - 1	RVE-105	1064	0.1842	-	7471B	PPB	02 Aug 2022 10:41:08	U	SMPL
N3930-14 - 1	RVE-106	1314	0.2304	-	7471B	PPB	02 Aug 2022 10:43:24	U	SMPL
CCV29 - 1	CCV29	27672	5.1025	-	7471B	PPB	02 Aug 2022 10:45:40	U	SMPL

LB121319 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Aug 2022 07:02:19

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
CCB29 - 1	CCB29	-49	-0.0216		-7471B	PPB	02 Aug 2022 10:47:56	U	SMPL
N3930-15 - 1	RVE-107	1621	0.2871		-7471B	PPB	02 Aug 2022 10:50:14	U	SMPL
N3930-16 - 1	RVE-108	3494	0.6334		-7471B	PPB	02 Aug 2022 10:52:30	U	SMPL
N3930-17 - 1	RVE-109	2071	0.3703		-7471B	PPB	02 Aug 2022 10:54:46	U	SMPL
N3930-18 - 1	RVE-110	5099	0.9300		-7471B	PPB	02 Aug 2022 10:57:03	U	SMPL
N3930-19 - 1	RVE-111	1466	0.2585		-7471B	PPB	02 Aug 2022 10:59:19	U	SMPL
N3930-20 - 1	RVE-112	2020	0.3609		-7471B	PPB	02 Aug 2022 11:01:35	U	SMPL
N3976-03DLX5 - 1		17211	3.1688		-7471B	PPB	02 Aug 2022 11:03:51	U	SMPL
N3976-05DLX10 - 1		130721	24.1504		-7471B	PPB	02 Aug 2022 11:06:08	U	SMPL
N3976-05DL2X50 - 1		27325	5.0384		-7471B	PPB	02 Aug 2022 11:08:25	U	SMPL
CCV30 - 1	CCV30	27687	5.1053		-7471B	PPB	02 Aug 2022 11:10:43	U	SMPL
CCB30 - 1	CCB30	-51	-0.0219		-7471B	PPB	02 Aug 2022 11:13:01	U	SMPL
N3970-04LX5 - 1		144	0.0141		-7471B	PPB	02 Aug 2022 11:15:19	U	SMPL
N3970-04A - 1		22287	4.1071		-7471B	PPB	02 Aug 2022 11:17:35	U	SMPL
N3927-01LX5 - 1		69	0.0003		-7471B	PPB	02 Aug 2022 11:19:50	U	SMPL
N3927-01A - 1		24395	4.4968		-7471B	PPB	02 Aug 2022 11:22:07	U	SMPL
N3930-01LX5 - 1		663	0.1101		-7471B	PPB	02 Aug 2022 11:24:24	U	SMPL
N3930-01A - 1		23346	4.3029		-7471B	PPB	02 Aug 2022 11:26:41	U	SMPL
CCV31 - 1	CCV31	24676	4.5487		-7471B	PPB	02 Aug 2022 11:38:26	U	SMPL
CCB31 - 1	CCB31	0	-0.0125		-7471B	PPB	02 Aug 2022 11:43:21	U	SMPL