

===== LB121358 =====
Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

8/4/2022 15:56

Reviewed by : 12 Instrument ID : Konelab

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.422	0.0	0.076	
ICB1	0.401	0.0	0.001	
CCV1	243.486	0.0	0.192	
CCB1	0.330	0.0	0.001	
PB146753BL	0.505	0.0	0.001	
N3997-11	0.493	0.0	0.001	
N3997-11DUP	0.859	0.0	0.002	
N3997-12	0.120	0.0	0.001	
N3997-13	0.348	0.0	0.001	
N3997-14	0.621	0.0	0.001	
N4017-01	0.438	0.0	0.001	
N4017-02	0.475	0.0	0.001	
N4017-03	0.466	0.0	0.001	
N4017-04	0.284	0.0	0.001	
CCV2	245.622	0.0	0.193	
CCB2	0.750	0.0	0.002	
N4017-05	0.241	0.0	0.001	
N4017-06	0.471	0.0	0.001	
N4017-07	0.674	0.0	0.002	
N4017-08	0.573	0.0	0.001	
N4017-09	0.703	0.0	0.002	
N4017-10	0.559	0.0	0.001	
N4023-02	0.576	0.0	0.001	
N4023-05	0.431	0.0	0.001	
N4023-08	0.767	0.0	0.002	
PB146754BL	0.494	0.0	0.001	
CCV3	246.988	0.0	0.194	
CCB3	0.361	0.0	0.001	
N3997-15	0.466	0.0	0.001	
N3997-15DUP	0.554	0.0	0.001	
CCV4	251.274	0.0	0.198	
CCB4	0.518	0.0	0.001	

N	32
Mean	34.290
SD	83.3641
CV%	243.12

Aquakem v. 7.2AQ1

Results from time period:

Thu Aug 04 14:45:13 2022

Thu Aug 04 15:53:42 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.3312	µg/l	8/4/2022 14:45:13	
5.0PPBCN	A	Total CN	P	5.4457	µg/l	8/4/2022 14:45:14	
10PPBCN	A	Total CN	P	10.0502	µg/l	8/4/2022 14:45:15	
50PPBCN	A	Total CN	P	49.7053	µg/l	8/4/2022 14:45:16	
100PPBCN	A	Total CN	P	99.1683	µg/l	8/4/2022 14:45:17	
250PPBCN	A	Total CN	P	250.2178	µg/l	8/4/2022 14:45:18	
500PPBCN	A	Total CN	P	500.0814	µg/l	8/4/2022 14:45:19	
ICV1	S	Total CN	P	96.4223	µg/l	8/4/2022 15:32:47	
ICB1	S	Total CN	P	0.4013	µg/l	8/4/2022 15:32:48	
CCV1	S	Total CN	P	243.4857	µg/l	8/4/2022 15:32:51	
CCB1	S	Total CN	P	0.3304	µg/l	8/4/2022 15:32:53	
PB146753BL	S	Total CN	P	0.5047	µg/l	8/4/2022 15:32:54	
N3997-11	S	Total CN	P	0.4927	µg/l	8/4/2022 15:32:56	
N3997-11DUP	S	Total CN	P	0.8593	µg/l	8/4/2022 15:40:20	
N3997-12	S	Total CN	P	0.12	µg/l	8/4/2022 15:40:21	
N3997-13	S	Total CN	P	0.3479	µg/l	8/4/2022 15:40:22	
N3997-14	S	Total CN	P	0.6213	µg/l	8/4/2022 15:40:23	
N4017-01	S	Total CN	P	0.4379	µg/l	8/4/2022 15:40:24	
N4017-02	S	Total CN	P	0.475	µg/l	8/4/2022 15:40:25	
N4017-03	S	Total CN	P	0.4657	µg/l	8/4/2022 15:40:26	
N4017-04	S	Total CN	P	0.2837	µg/l	8/4/2022 15:40:27	
CCV2	S	Total CN	P	245.6223	µg/l	8/4/2022 15:40:29	
CCB2	S	Total CN	P	0.7498	µg/l	8/4/2022 15:40:30	
N4017-05	S	Total CN	P	0.2415	µg/l	8/4/2022 15:47:53	
N4017-06	S	Total CN	P	0.4707	µg/l	8/4/2022 15:47:54	
N4017-07	S	Total CN	P	0.6742	µg/l	8/4/2022 15:47:55	
N4017-08	S	Total CN	P	0.5731	µg/l	8/4/2022 15:47:56	
N4017-09	S	Total CN	P	0.703	µg/l	8/4/2022 15:47:57	
N4017-10	S	Total CN	P	0.5588	µg/l	8/4/2022 15:47:58	
N4023-02	S	Total CN	P	0.5758	µg/l	8/4/2022 15:47:59	
N4023-05	S	Total CN	P	0.4312	µg/l	8/4/2022 15:48:00	
N4023-08	S	Total CN	P	0.7669	µg/l	8/4/2022 15:48:01	
PB146754BL	S	Total CN	P	0.4936	µg/l	8/4/2022 15:48:02	
CCV3	S	Total CN	P	246.9875	µg/l	8/4/2022 15:53:36	
CCB3	S	Total CN	P	0.3615	µg/l	8/4/2022 15:53:37	
N3997-15	S	Total CN	P	0.466	µg/l	8/4/2022 15:53:38	
N3997-15DUP	S	Total CN	P	0.554	µg/l	8/4/2022 15:53:39	
CCV4	S	Total CN	P	251.2744	µg/l	8/4/2022 15:53:41	
CCB4	S	Total CN	P	0.5179	µg/l	8/4/2022 15:53:42	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

8/4/2022 14:45


Test Total CN

Accepted 8/4/2022 14:45

Factor 1278
Bias 0.001

Coeff. of det. 0.999994

Errors

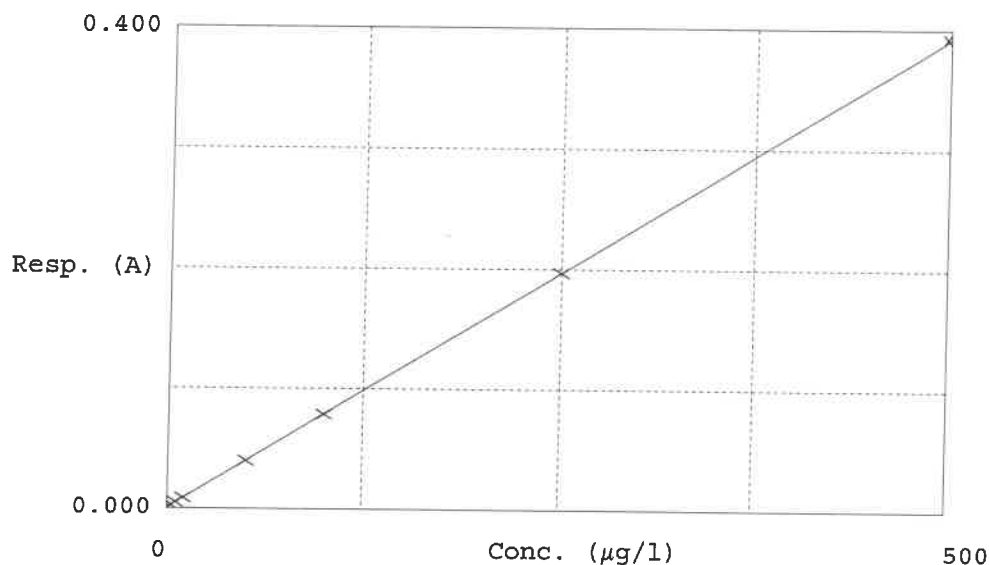

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.3312	0.0000	-
2	5.0PPBCN	0.005	5.4457	5.0000	8.9
3	10PPBCN	0.009	10.0502	10.0000	0.5
4	50PPBCN	0.040	49.7053	50.0000	-0.6
5	100PPBCN	0.079	99.1683	100.0000	-0.8
6	250PPBCN	0.197	250.2178	250.0000	0.1
7	500PPBCN	0.392	500.0814	500.0000	0.0

12
8/4/22