


7471B

LB121562
INSTRUMENT ID: CV1

Linear

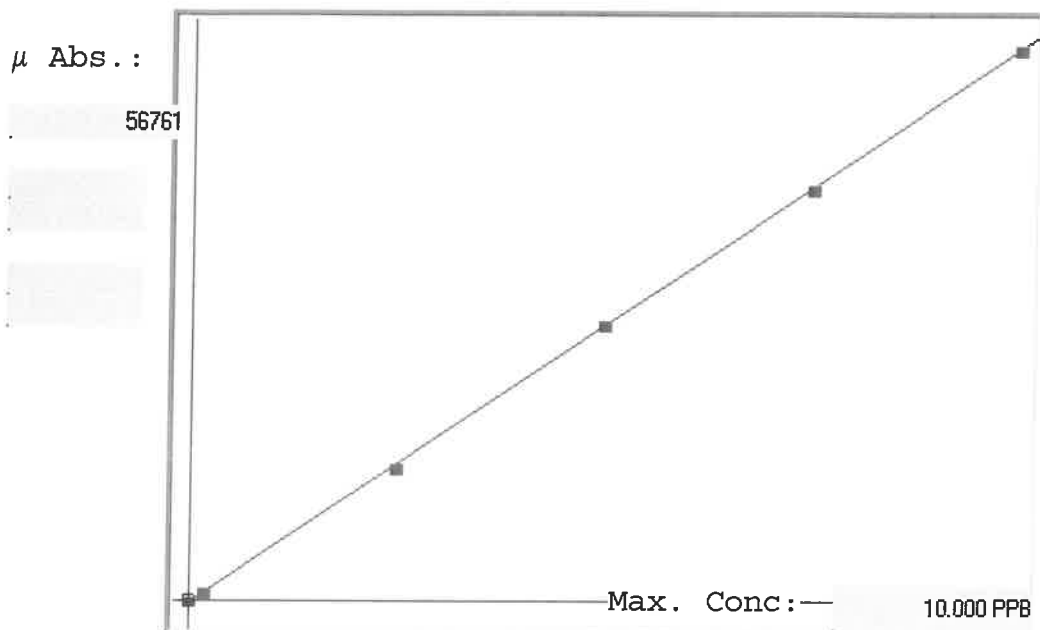

A= 0.0000e+000

B= 1.7573e-004

C= 3.8248e-002

Rho= 0.9999617

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.035	0.035	-20	0.000	-20					
0.2	0.200	0.201	0.001	928	0.0 %	928					
2.5	2.500	2.439	-0.061	13661	0.0 %	13661					
5.0	5.000	5.029	0.029	28403	0.0 %	28403					
7.5	7.500	7.483	-0.017	42366	0.0 %	42366					
10.0	10.000	10.013	0.013	56761	0.0 %	56761					

0.0
-1
-2

LB121562 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 17 Aug 2022 13:40:56

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-20	-	0.0000	7471B	PPB	17 Aug 2022 13:43:01	S	Std
0.2 - 1	50.2	928	-	0.2000	7471B	PPB	17 Aug 2022 13:45:18	S	Std
2.5 - 1	52.5	13661	-	2.5000	7471B	PPB	17 Aug 2022 13:47:35	S	Std
5.0 - 1	55	28403	-	5.0000	7471B	PPB	17 Aug 2022 13:49:52	S	Std
7.5 - 1	57.5	42366	-	7.5000	7471B	PPB	17 Aug 2022 13:52:08	S	Std
10.0 - 1	57.5	56761	-	10.0000	7471B	PPB	17 Aug 2022 13:54:25	S	Std
ICV91 - 1	ICV91	22413	3.9768	-	7471B	PPB	17 Aug 2022 13:57:21	U	SMPL
ICB91 - 1	ICB91	-129	0.0156	-	7471B	PPB	17 Aug 2022 13:59:36	U	SMPL
CCV57 - 1	CCV57	28783	5.0962	-	7471B	PPB	17 Aug 2022 14:01:52	U	SMPL
CCB57 - 1	CCB57	-136	0.0143	-	7471B	PPB	17 Aug 2022 14:04:08	U	SMPL
CRA - 1	CRA	903	0.1969	-	7471B	PPB	17 Aug 2022 14:06:24	U	SMPL
HighStd - 1	HighStd	57408	10.1263	-	7471B	PPB	17 Aug 2022 14:08:39	U	SMPL
ChkStd - 1	ChkStd	39723	7.0186	-	7471B	PPB	17 Aug 2022 14:10:55	U	SMPL
PB147068BL - 1	PBS	-168	0.0087	-	7471B	PPB	17 Aug 2022 14:13:13	U	SMPL
PB147068BS - 1	LCSS	22632	4.0153	-	7471B	PPB	17 Aug 2022 14:15:31	U	SMPL
N4213-01 - 1	VNJ-209	2040	0.3967	-	7471B	PPB	17 Aug 2022 14:17:48	U	SMPL
N4213-03 - 1	VNJ-226	1561	0.3126	-	7471B	PPB	17 Aug 2022 14:20:05	U	SMPL
N4214-01 - 1	ETGI-354	5918	1.0782	-	7471B	PPB	17 Aug 2022 14:22:23	U	SMPL
N4214-03 - 1	ETGI-357	4107	0.7600	-	7471B	PPB	17 Aug 2022 14:24:39	U	SMPL
N4215-01 - 1	WC-1	2952	0.5570	-	7471B	PPB	17 Aug 2022 14:26:55	U	SMPL
CCV58 - 1	CCV58	28316	5.0141	-	7471B	PPB	17 Aug 2022 14:29:10	U	SMPL
CCB58 - 1	CCB58	-109	0.0191	-	7471B	PPB	17 Aug 2022 14:31:25	U	SMPL
N4215-03 - 1	WC-2	1637	0.3259	-	7471B	PPB	17 Aug 2022 14:33:42	U	SMPL
N4215-05 - 1	WC-3	1708	0.3384	-	7471B	PPB	17 Aug 2022 14:35:57	U	SMPL
N4216-01 - 1	NB-08-081522	1146	0.2396	-	7471B	PPB	17 Aug 2022 14:38:13	U	SMPL
N4217-04 - 1	TP1-0815	1074	0.2270	-	7471B	PPB	17 Aug 2022 14:40:29	U	SMPL
N4217-06 - 1	TP2-0815	1708	0.3384	-	7471B	PPB	17 Aug 2022 14:42:45	U	SMPL
N4217-08 - 1	TP3-0815	686	0.1588	-	7471B	PPB	17 Aug 2022 14:45:02	U	SMPL
N4217-10 - 1	TP4-0815	431	0.1140	-	7471B	PPB	17 Aug 2022 14:47:18	U	SMPL
N4218-01 - 1	OR-02-081522	4050	0.7499	-	7471B	PPB	17 Aug 2022 14:49:35	U	SMPL
N4218-01DUP - 1	OR-02-081522DUP	3854	0.7155	-	7471B	PPB	17 Aug 2022 14:51:52	U	SMPL
N4218-01MS - 1	OR-02-081522MS	26062	4.6180	-	7471B	PPB	17 Aug 2022 14:54:08	U	SMPL
CCV59 - 1	CCV59	28330	5.0166	-	7471B	PPB	17 Aug 2022 14:56:23	U	SMPL
CCB59 - 1	CCB59	-97	0.0212	-	7471B	PPB	17 Aug 2022 14:58:40	U	SMPL
N4218-01MSD - 1	OR-02-081522MSD	28200	4.9937	-	7471B	PPB	17 Aug 2022 15:00:58	U	SMPL
N4218-01LX5 - 1		715	0.1639	-	7471B	PPB	17 Aug 2022 15:03:14	U	SMPL
N4218-01A - 1		26871	4.7602	-	7471B	PPB	17 Aug 2022 15:05:31	U	SMPL
CCV60 - 1	CCV60	28248	5.0022	-	7471B	PPB	17 Aug 2022 15:07:47	U	SMPL
CCB60 - 1	CCB60	-112	0.0186	-	7471B	PPB	17 Aug 2022 15:10:03	U	SMPL