


LB 121572

245.1

INSTRUMENT ID: CV2

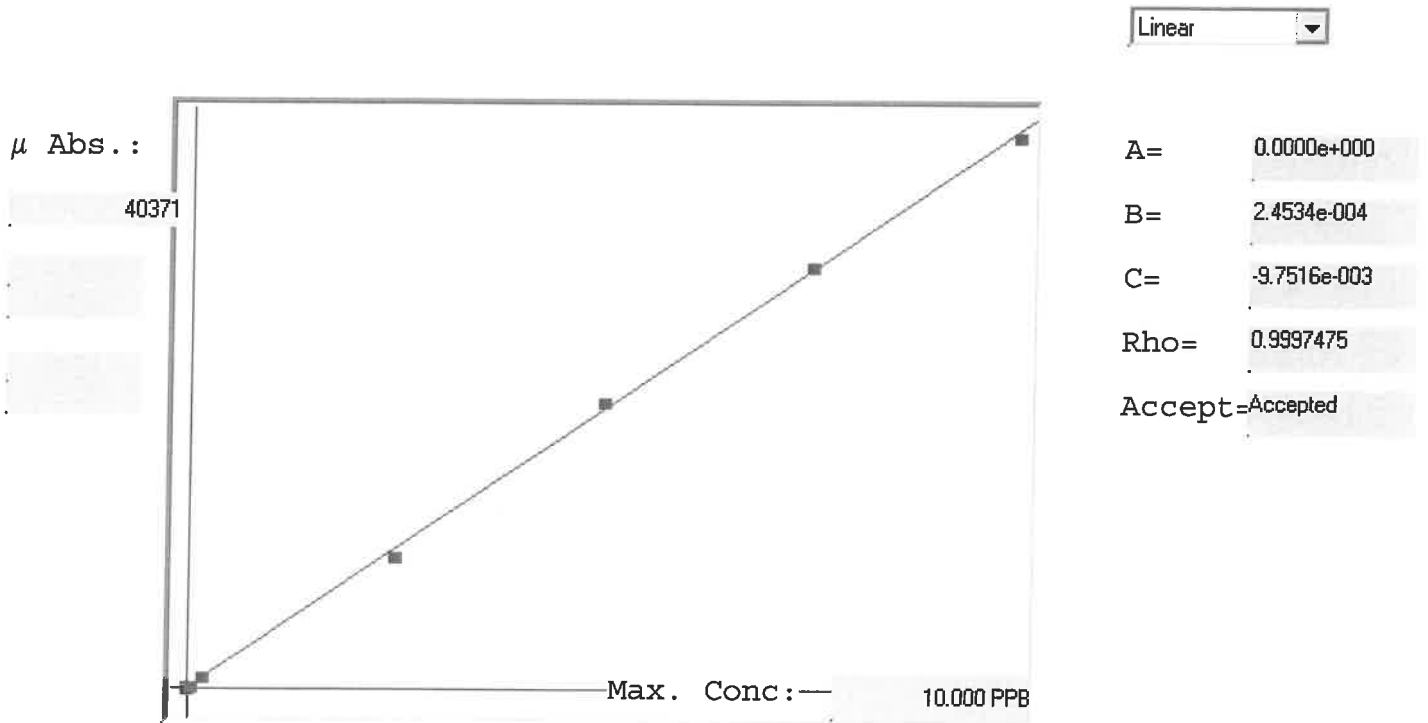

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.005	0.005	61	0.000	61					0
0.05	0.050	0.050	-0.000	243	0.0 %	243	0				-1
0.2	0.200	0.198	-0.002	847	0.0 %	847					-5
2.5	2.500	2.386	-0.114	9765	0.0 %	9765					3
5.0	5.000	5.133	0.133	20961	0.0 %	20961					1
7.5	7.500	7.583	0.083	30950	0.0 %	30950					-1
10.0	10.000	9.895	-0.105	40371	0.0 %	40371					

LB121572 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 18 Aug 2022 10:58:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SP	61	-	0.0000	245.1	PPB	18 Aug 2022 11:15:31	S	Std
0.05 - 1	SP.05	243	-	0.0500	245.1	PPB	18 Aug 2022 11:17:48	S	Std
0.2 - 1	SP.2	847	-	0.2000	245.1	PPB	18 Aug 2022 11:22:37	S	Std
2.5 - 1	SP.5	9765	-	2.5000	245.1	PPB	18 Aug 2022 11:24:54	S	Std
5.0 - 1	SP.5	20961	-	5.0000	245.1	PPB	18 Aug 2022 11:27:10	S	Std
7.5 - 1	SP.5	30950	-	7.5000	245.1	PPB	18 Aug 2022 11:29:25	S	Std
10.0 - 1	SP.10	40371	-	10.0000	245.1	PPB	18 Aug 2022 11:31:42	S	Std
ICV93 - 1	ICV93	15582	3.8131	-245.1	PPB	PPB	18 Aug 2022 11:34:31	U	SMPL
ICB93 - 1	ICB93	-47	-0.0213	-245.1	PPB	PPB	18 Aug 2022 11:36:45	U	SMPL
CCV64 - 1	CCV64	21257	5.2054	-245.1	PPB	PPB	18 Aug 2022 11:41:01	U	SMPL
CCB64 - 1	CCB64	-65	-0.0257	-245.1	PPB	PPB	18 Aug 2022 11:43:16	U	SMPL
CRA - 1	CRA	217	0.0435	-245.1	PPB	PPB	18 Aug 2022 11:45:31	U	SMPL
HighStd - 1	HighStd	40418	9.9063	-245.1	PPB	PPB	18 Aug 2022 11:47:46	U	SMPL
ChkStd - 1	ChkStd	28992	7.1031	-245.1	PPB	PPB	18 Aug 2022 11:50:01	U	SMPL
PB147114BL - 1	PBW	-125	-0.0404	-245.1	PPB	PPB	18 Aug 2022 11:52:19	U	SMPL
PB147114BS - 1	LCSW	16515	4.0420	-245.1	PPB	PPB	18 Aug 2022 11:54:36	U	SMPL
N3734-05 - 1	WS-TRACE-ELEMENTS-1	23285	5.7029	-245.1	PPB	PPB	18 Aug 2022 11:56:52	U	SMPL
N4024-01 - 1	MANHOLE	36	-0.0009	-245.1	PPB	PPB	18 Aug 2022 11:59:08	U	SMPL
N4024-01DUP - 1	MANHOLEDUP	126	0.0212	-245.1	PPB	PPB	18 Aug 2022 12:01:26	U	SMPL
N4024-01MS - 1	MANHOLEMS	16402	4.0143	-245.1	PPB	PPB	18 Aug 2022 12:03:43	U	SMPL
N4024-01MSD - 1	MANHOLEMSD	15670	3.8347	-245.1	PPB	PPB	18 Aug 2022 12:05:58	U	SMPL
CCV65 - 1	CCV65	21681	5.3094	-245.1	PPB	PPB	18 Aug 2022 12:08:14	U	SMPL
CCB65 - 1	CCB65	-116	-0.0382	-245.1	PPB	PPB	18 Aug 2022 12:10:29	U	SMPL
N4099-01 - 1	EFF-DAY-1-METALS	651	0.1500	-245.1	PPB	PPB	18 Aug 2022 12:12:45	U	SMPL
N4024-01LX5 - 1		-94	-0.0328	-245.1	PPB	PPB	18 Aug 2022 12:15:01	U	SMPL
N4024-01A - 1		17526	4.2900	-245.1	PPB	PPB	18 Aug 2022 12:17:16	U	SMPL
CCV66 - 1	CCV66	21813	5.3418	-245.1	PPB	PPB	18 Aug 2022 12:26:23	U	SMPL
CCB66 - 1	CCB66	-115	-0.0380	-245.1	PPB	PPB	18 Aug 2022 12:28:41	U	SMPL