

LB121611

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/19/2022 15:26

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.008	0.0	0.114	
ICB1	0.003	0.0	0.009	
CCV1	1.007	0.0	0.114	
CCB1	0.002	0.0	0.009	
PB147149BL	0.002	0.0	0.009	
PB147149BS	1.002	0.0	0.113	
N3980-01	0.027	0.0	0.011	
N3980-02	0.053	0.0	0.014	
PB147150BL	0.000	0.0	0.008	
PB147150BS	1.008	0.0	0.114	
N3980-07	0.029	0.0	0.012	
N3980-08	0.053	0.0	0.014	
CCV2	1.009	0.0	0.114	
CCB2	-0.001	0.0	0.008	

N	14
Mean	0.372
SD	0.4916
CV%	132.25

Aquakem v. 7.2AQ1

Results from time period:

Fri Aug 19 15:07:57 2022

Fri Aug 19 15:22:56 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
0.00PPM	A	Phenolics-	P	0.001	mg/l	8/19/2022 13:54:26
0.05PPM	A	Phenolics-	P	0.052	mg/l	8/19/2022 13:54:27
0.1PPM	A	Phenolics-	P	0.1052	mg/l	8/19/2022 13:54:28
0.25PPM	A	Phenolics-	P	0.2537	mg/l	8/19/2022 13:54:29
0.50PPM	A	Phenolics-	P	0.4978	mg/l	8/19/2022 13:54:30
1.0PPM	A	Phenolics-	P	0.9811	mg/l	8/19/2022 13:54:31
2.0PPM	A	Phenolics-	P	2.0092	mg/l	8/19/2022 13:54:32
ICV1	S	Phenolics-	P	1.0082	mg/l	8/19/2022 15:07:58
ICB1	S	Phenolics-	P	0.003	mg/l	8/19/2022 15:08:00
CCV1	S	Phenolics-	P	1.0074	mg/l	8/19/2022 15:08:01
CCB1	S	Phenolics-	P	0.002	mg/l	8/19/2022 15:08:04
PB147149BL	S	Phenolics-	P	0.0017	mg/l	8/19/2022 15:08:05
PB147149BS	S	Phenolics-	P	1.0018	mg/l	8/19/2022 15:08:08
N3980-01	S	Phenolics-	P	0.0274	mg/l	8/19/2022 15:18:00
N3980-02	S	Phenolics-	P	0.0534	mg/l	8/19/2022 15:18:01
PB147150BL	S	Phenolics-	P	0.0004	mg/l	8/19/2022 15:18:04
PB147150BS	S	Phenolics-	P	1.0083	mg/l	8/19/2022 15:18:06
N3980-07	S	Phenolics-	P	0.0293	mg/l	8/19/2022 15:18:07
N3980-08	S	Phenolics-	P	0.0532	mg/l	8/19/2022 15:18:10
CCV2	S	Phenolics-	P	1.0089	mg/l	8/19/2022 15:22:54
CCB2	S	Phenolics-	P	-0.0007	mg/l	8/19/2022 15:22:56

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/19/2022 13:55


Test Phenolics-

Accepted 8/19/2022 13:55

Factor 9.577
Bias 0.008

Coeff. of det. 0.999844

Errors

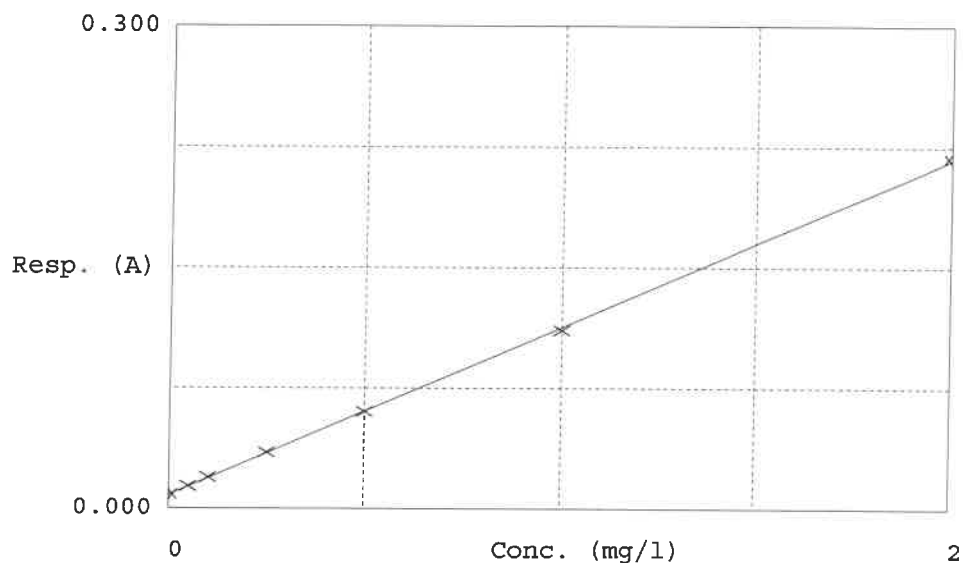

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.009	0.0010	0.0000	
2	Phenol-2	0.014	0.0520	0.0500	
3	Phenol-2	0.019	0.1052	0.1000	
4	Phenol-2	0.035	0.2537	0.2500	
5	Phenol-2	0.060	0.4978	0.5000	
6	Phenol-2	0.111	0.9811	1.0000	
7	Phenol-2	0.218	2.0092	2.0000	

De
Errors

4.00
5.2
1.5
0.4
1.4
0.5

12
8/19/22