

Clear table

Instrument ID: IC-2										Analyst : IZ		Method: 300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-16_	8/16/22 9:55		IZ/MA		
STD2	0.5060	0.6450	0.6970	2.1910	0.5530	1.0290	3.4450	2022-08-16_	8/16/22 10:25		IZ/MA		
STD3	0.8250	1.1920	1.2250	3.9610	0.9970	1.8870	6.0020	2022-08-16_	8/16/22 10:54		IZ/MA		
STD4	0.9310	1.5300	1.5170	5.0650	1.2680	2.4800	7.5950	2022-08-16_	8/16/22 11:24		IZ/MA		
STD5	1.8850	2.9380	2.9110	9.8030	2.4350	5.1310	14.4450	2022-08-16_	8/16/22 11:59		IZ/MA		
STD6	4.0620	5.9080	5.7350	19.6760	4.9070	10.0410	29.3950	2022-08-16_	8/16/22 12:28		IZ/MA		
STD7	4.9910	7.5870	7.7150	25.3050	6.3390	12.4310	38.1170	2022-08-16_	8/16/22 12:58		IZ/MA		
ICV	1.8430	2.9550	2.9380	9.7100	2.4270	5.0090	14.3640	2022-08-16_	8/16/22 14:34		IZ/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-16_	8/16/22 15:04		IZ/MA		
CCV	1.9430	2.9230	2.9540	9.6700	2.4080	5.4970	14.2740	2022-08-19_	8/19/22 17:40		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-19_	8/19/22 18:10		IZ/MA		
LB121643BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-19_	8/19/22 18:40		IZ/MA		
LB121643BSW	1.9890	2.9540	3.0410	9.7900	2.4380	5.5470	14.4800	2022-08-19_	8/19/22 19:09		IZ/MA		
N4264-02	0.1820	351.5690	0.0000	0.0000	9.4700	0.0000	55.1410	2022-08-19_	8/19/22 19:39		IZ/MA		
N4264-02MS	2.8750	338.6270	2.8310	10.4290	11.9030	10.6210	68.7720	2022-08-19_	8/19/22 20:09		IZ/MA		
N4264-02MSD	2.7870	338.1070	2.9220	10.5490	12.0250	10.9130	69.4730	2022-08-19_	8/19/22 20:38		IZ/MA		
N4262-01	0.1800	341.5280	0.0000	1.2080	8.8620	1.2300	85.7470	2022-08-19_	8/19/22 21:08		IZ/MA		
N4262-02	0.1800	12.2130	0.0000	0.0000	2.3840	0.2870	19.0910	2022-08-19_	8/19/22 21:37		IZ/MA		
N4262-03	0.0000	271.9180	0.0000	0.0000	11.5210	0.1910	96.9300	2022-08-19_	8/19/22 22:07		IZ/MA		
N4262-04	0.1530	213.9390	0.0000	0.0000	3.0340	0.2260	30.2470	2022-08-19_	8/19/22 22:37		IZ/MA		
N4262-05	0.0000	364.1170	0.0000	0.0000	7.8720	0.0000	64.2570	2022-08-19_	8/19/22 23:06		IZ/MA		
CCV	1.9450	2.9580	3.1030	9.8050	2.4150	6.4110	14.3520	2022-08-19_	8/19/22 23:36		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-20_	8/20/22 0:06		IZ/MA		
N4262-06	0.1220	303.8760	0.0000	0.0000	13.3620	0.1900	82.1560	2022-08-20_	8/20/22 0:35		IZ/MA		
N4262-07	0.0000	271.5780	0.0000	0.0000	11.5340	0.1720	95.8380	2022-08-20_	8/20/22 1:05		IZ/MA		
CCV	1.9680	2.9570	3.0250	9.9140	2.4250	6.5380	14.2790	2022-08-20_	8/20/22 1:35		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-20_	8/20/22 2:04		IZ/MA		
CCV	1.8750	2.9080	3.0180	9.8510	2.3830	5.0440	14.3390	2022-08-22_	8/22/22 10:55		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-22_	8/22/22 11:27		IZ/MA		
LB121643BLW2	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-22_	8/22/22 11:59		IZ/MA		
LB121643BSW2	1.9230	2.9130	2.9690	9.8640	2.3990	5.0600	14.3840	2022-08-22_	8/22/22 12:30		IZ/MA		
N4277-02	0.1620	261.5700	0.0000	0.0000	3.4500	0.0000	28.4950	2022-08-22_	8/22/22 13:02		IZ/MA		
N4277-03	0.1500	72.6390	0.0000	0.0000	1.9490	0.0000	32.7550	2022-08-22_	8/22/22 13:34		IZ/MA		
N4264-02DLX2	0.0000	213.4690	0.0000	0.0000	4.2870	0.0000	25.1890	2022-08-22_	8/22/22 14:06		IZ/MA		

N4262-01DLX100	0.0000	3.1750	0.0000	0.0000	0.1760	0.0000	1.5600	2022-08-22	8/22/22 14:37	IZ/MA
N4262-02DLX2	0.0000	5.8180	0.0000	0.0000	1.1840	0.0000	9.7460	2022-08-22	8/22/22 15:09	IZ/MA
N4262-03DLX50	0.0000	4.3500	0.0000	0.0000	0.2710	0.0000	2.2290	2022-08-22	8/22/22 15:41	IZ/MA
N4262-04DLX50	0.0000	3.0450	0.0000	0.0000	0.0000	0.0000	1.3840	2022-08-22	8/22/22 16:12	IZ/MA
N4262-05DLX100	0.0000	3.3040	0.0000	0.0000	0.1610	0.0000	1.3550	2022-08-22	8/22/22 16:44	IZ/MA
CCV	1.9370	2.9310	2.9860	9.9250	2.4060	5.5930	14.4430	2022-08-22	8/22/22 17:16	IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-22	8/22/22 17:47	IZ/MA
N4262-06DLX100	0.0000	2.5610	0.0000	0.0000	0.2000	0.0000	1.5120	2022-08-22	8/22/22 18:19	IZ/MA
N4262-07DLX100	0.0000	2.0870	0.0000	0.0000	0.1900	0.0000	1.5570	2022-08-22	8/22/22 18:51	IZ/MA
CCV	1.9760	2.9200	2.8320	9.8090	2.3880	5.5390	14.4010	2022-08-22	8/22/22 19:54	IZ/MA
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-22	8/22/22 20:26	IZ/MA


Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A

ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-08-16	8/16/22 9:55		IZ/MA
STD2	0.5060	0.6450	0.6970	2.1910	0.5530	1.0290	3.4450	2022-08-16	8/16/22 10:25		IZ/MA
STD3	0.8250	1.1920	1.2250	3.9610	0.9970	1.8870	6.0020	2022-08-16	8/16/22 10:54		IZ/MA
STD4	0.9310	1.5300	1.5170	5.0650	1.2680	2.4800	7.5950	2022-08-16	8/16/22 11:24		IZ/MA
STD5	1.8850	2.9380	2.9110	9.8030	2.4350	5.1310	14.4450	2022-08-16	8/16/22 11:59		IZ/MA
STD6	4.0620	5.9080	5.7350	19.6760	4.9070	10.0410	29.3950	2022-08-16	8/16/22 12:28		IZ/MA
STD7	4.9910	7.5870	7.7150	25.3050	6.3390	12.4310	38.1170	2022-08-16	8/16/22 12:58		IZ/MA
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	26.5000	7.5000	16.1667	9.5500	10.6000	2.9000	14.8333				
STD3	3.1250	-0.6667	2.0833	-0.9750	-0.3000	-5.6500	0.0333				
STD4	-6.9000	2.0000	1.1333	1.3000	1.4400	-0.8000	1.2667				
STD5	-5.7500	-2.0667	-2.9667	-1.9700	-2.6000	2.6200	-3.7000				
STD6	1.5500	-1.5333	-4.4167	-1.6200	-1.8600	0.4100	-2.0167				
STD7	-0.1800	1.1600	2.8667	1.2200	1.4240	-0.5520	3.0189				

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.0693891 \cdot A + 0.576427$
 RSD: 4.170 %
 Correlation coefficient: 0.999052

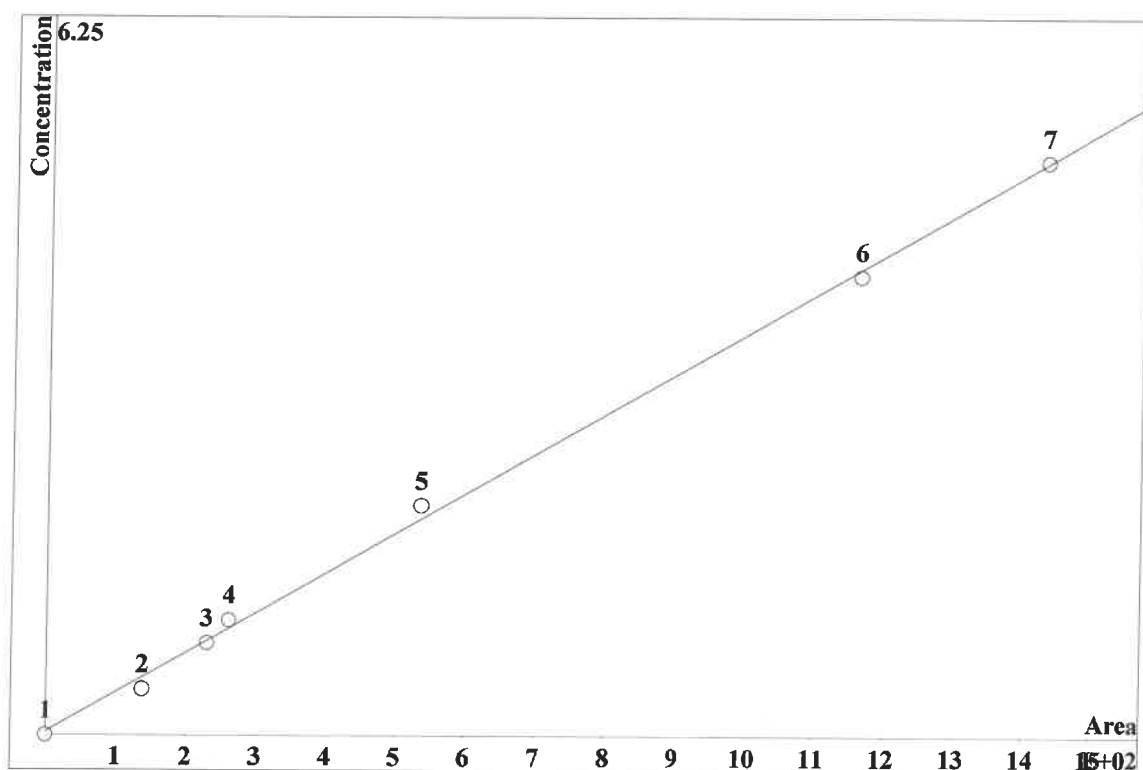


K3 = 0 K2 = 0 K1 = 0.0693891 K0 = 0.576427
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.281	137.6	0.4	20	6.252		
3	5.025	229.4	0.8	20	6.252		
4	6.186	260	1	20	6.195		
5	14.98	535.1	2	20	6.195		
6	32.04	1162	4	20	6.195		
7	41.73	1430	5	20	6.195		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.126214 \cdot A + 2.35707$
 RSD: 2.295 %
 Correlation coefficient: 0.999713

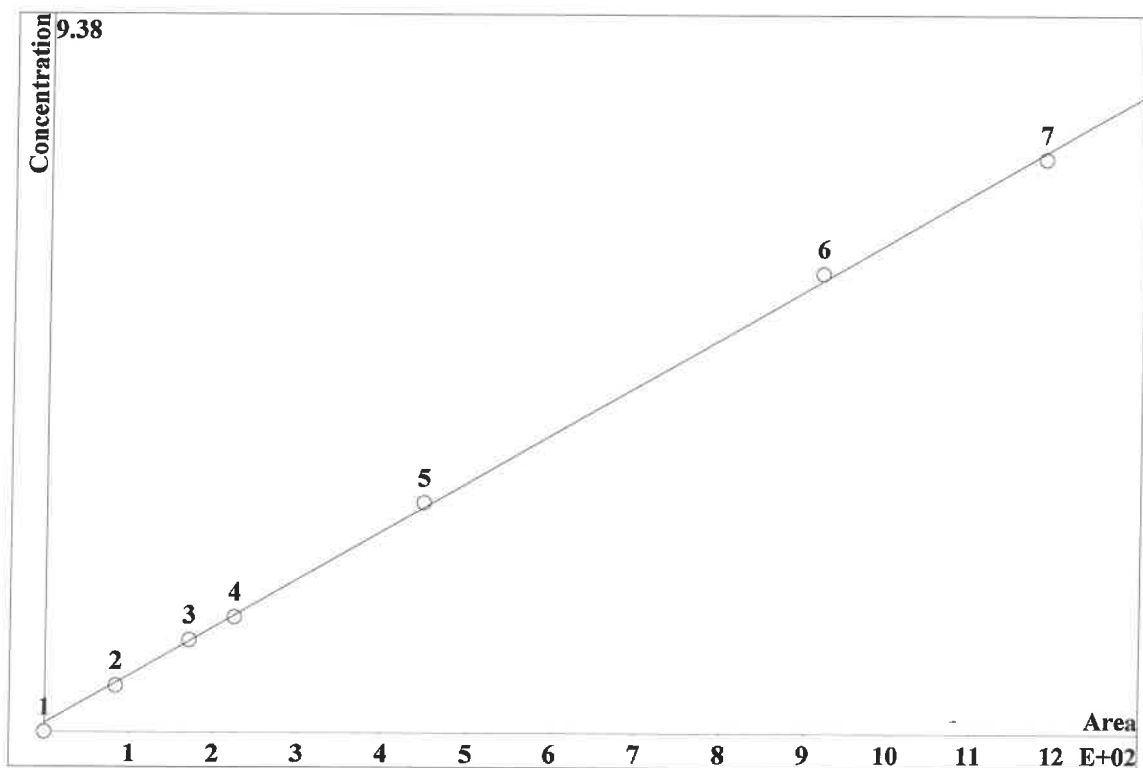

K3 = 0 K2 = 0 K1 = 0.126214 K0 = 2.35707

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.5	83.45	0.6	20	9.385		
3	8.802	170.3	1.2	20	9.385		
4	11.84	223.8	1.5	20	9.331		
5	23.7	446.8	3	20	9.331		
6	48.66	917.5	6	20	9.331		
7	66.44	1184	7.5	20	9.331		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.0579711 \cdot A + 4.95017$
 RSD: 5.563 %
 Correlation coefficient: 0.998312

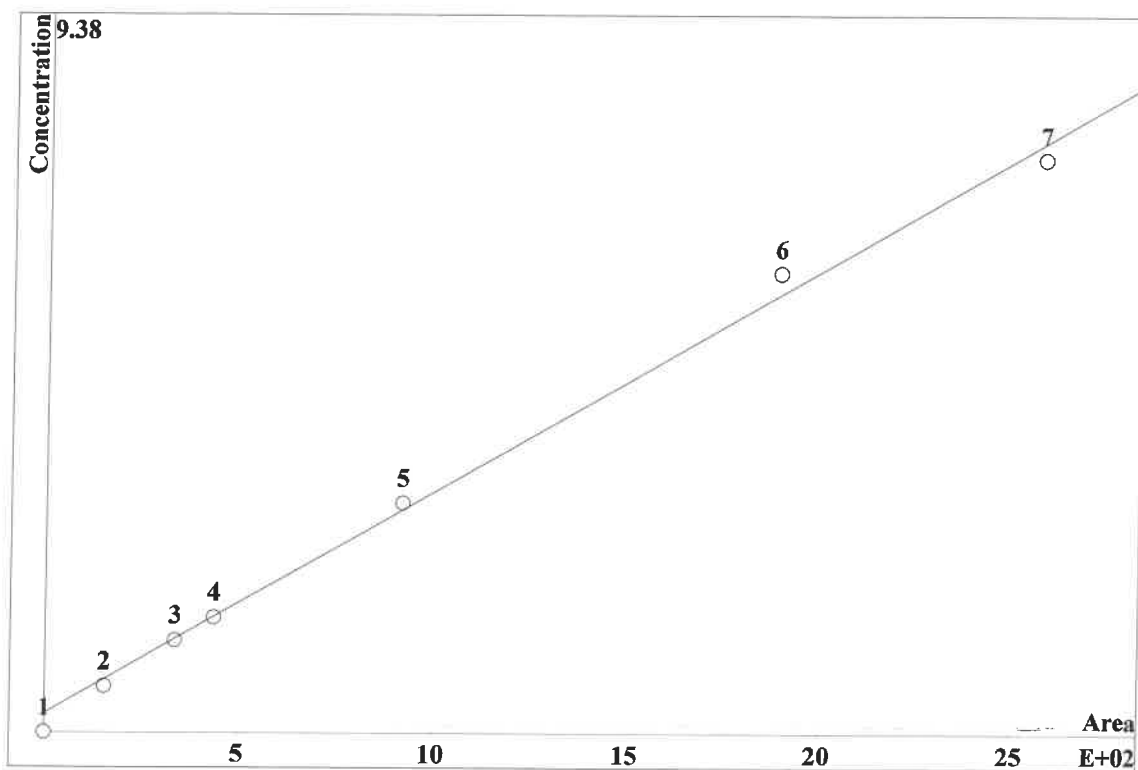


K3 = 0 K2 = 0 K1 = 0.0579711 K0 = 4.95017
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.4	155.2	0.6	20	11.29		
3	15.04	337.3	1.2	20	11.29		
4	20.6	437.9	1.5	20	11.24		
5	43.31	919.1	3	20	11.24		
6	89.85	1893	6	20	11.24		
7	123.2	2576	7.5	20	11.24		
1.□							

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.282012 \cdot A + 11.9662$
 RSD: 2.400 %
 Correlation coefficient: 0.999686

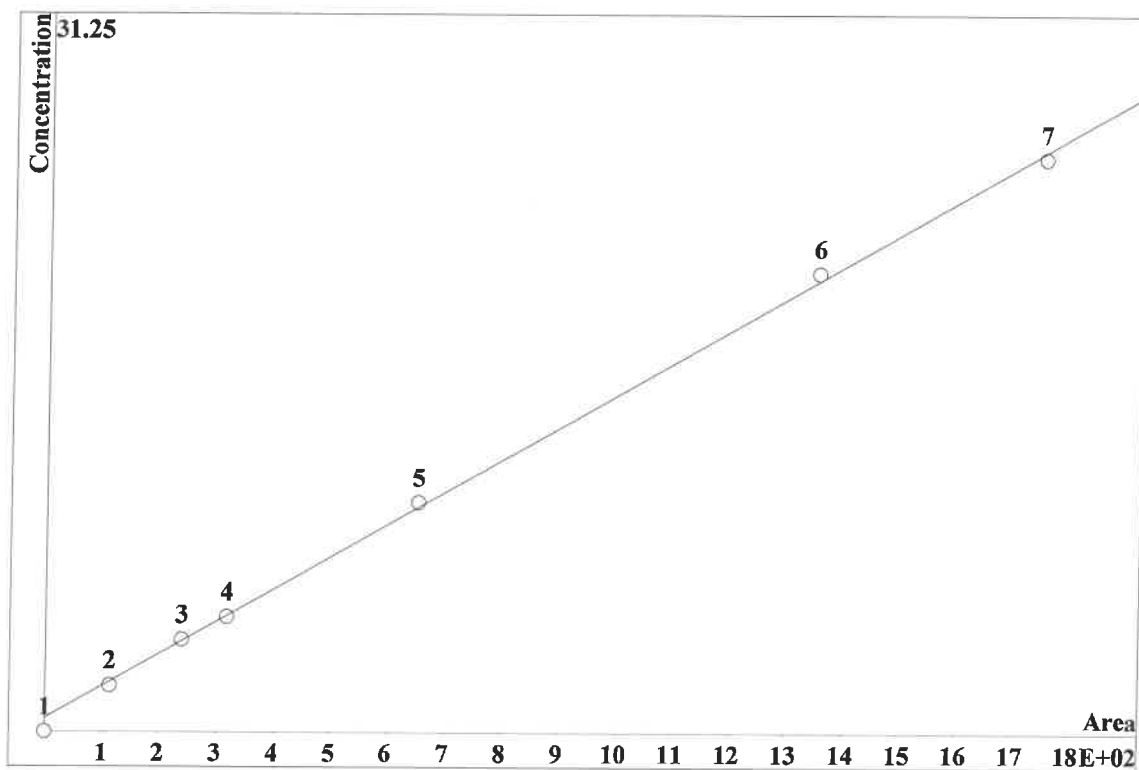

K3 = 0 K2 = 0 K1 = 0.282012 K0 = 11.9662

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.858	112.9	2	20			14.56
3	9.861	238.5	4	20			14.56
4	13.34	316.7	5	20			13.53
5	27.09	652.8	10	20			13.53
6	55.18	1353	20	20			13.53
7	73.96	1752	25	20			13.53

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.0486843 \cdot A + 2.38133$
 RSD: 2.818 %
 Correlation coefficient: 0.999567

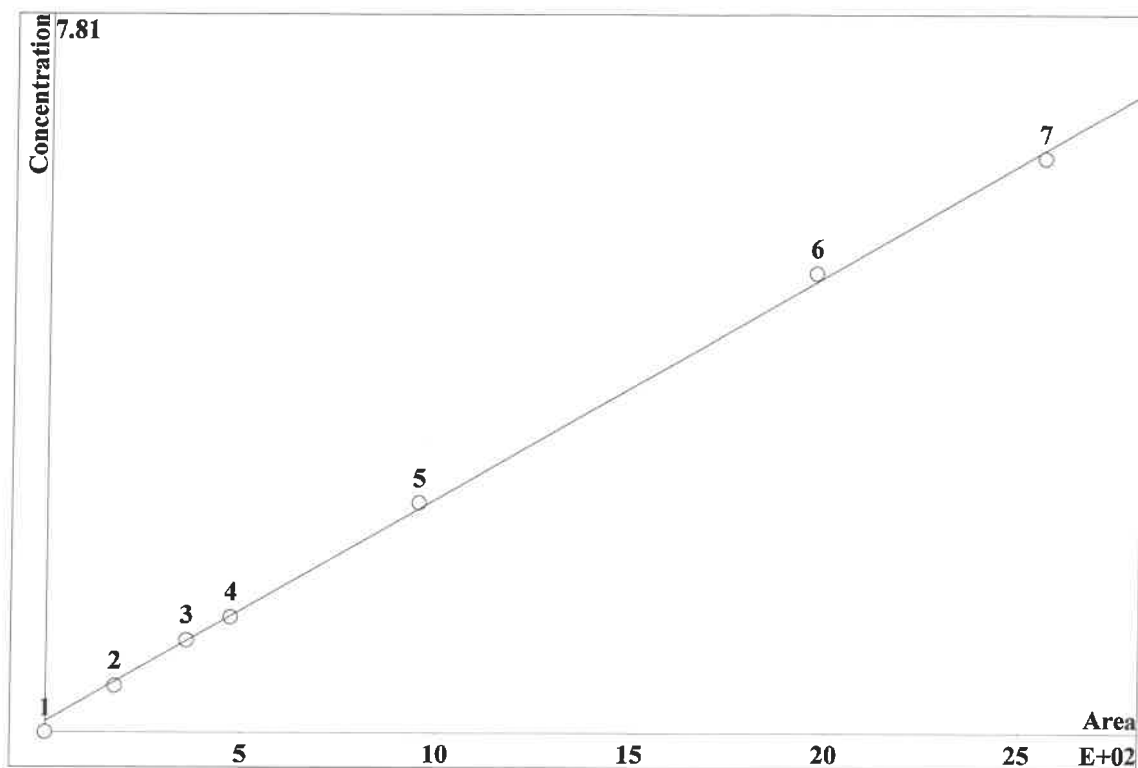


K3 = 0 K2 = 0 K1 = 0.0486843 K0 = 2.38133
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.142	178.4	0.5	20	16.64		
3	12.22	360.6	1	20	16.64		
4	16.44	472.2	1.25	20	15.58		
5	33.14	951.5	2.5	20	15.58		
6	68.77	1967	5	20	15.58		
7	93.41	2555	6.25	20	15.58		
1.□							

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.0564191 \cdot A + 1.30946$
 RSD: 1.764 %
 Correlation coefficient: 0.999830

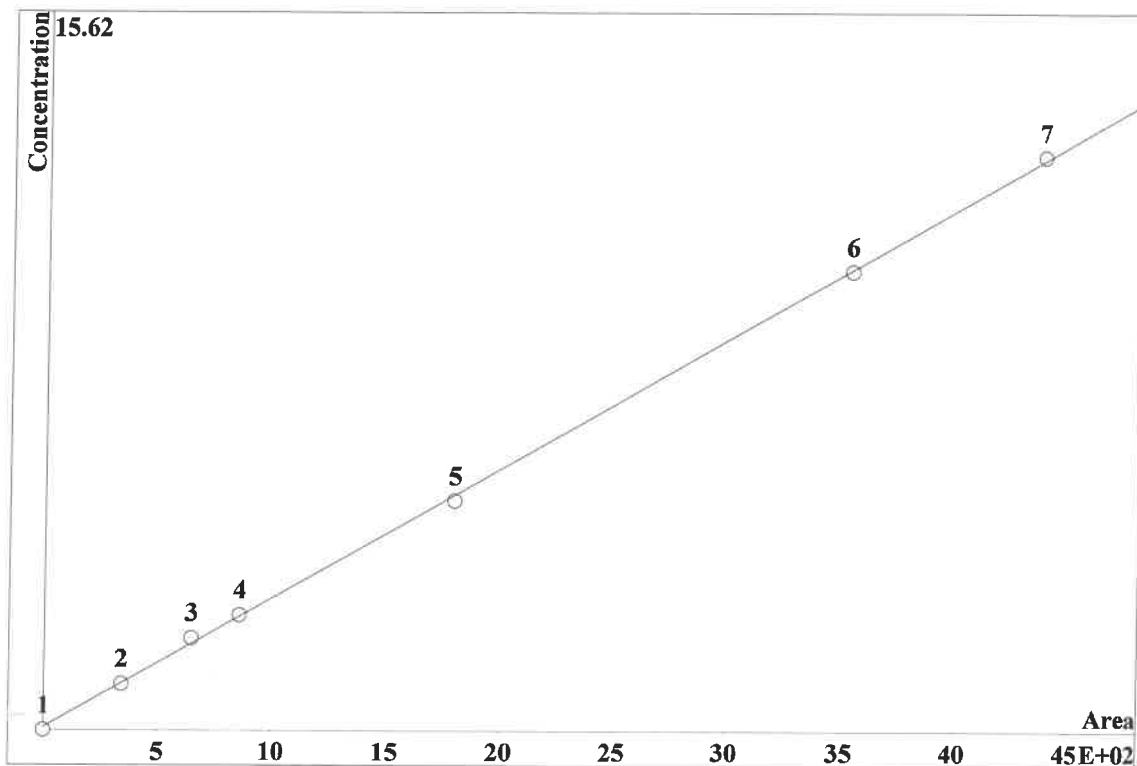


K3 = 0 K2 = 0 K1 = 0.0564191 K0 = 1.30946
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.536	341.7	1	20	21.97		
3	12.7	645.7	2	20	21.97		
4	17.29	855.9	2.5	20	20.18		
5	37.82	1796	5	20	20.18		
6	78.17	3536	10	20	20.18		
7	100.3	4384	12.5	20	20.18		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-081622.mtw
 Equation: $Q = 0.159092 \cdot A + 15.88$
 RSD: 3.404 %
 Correlation coefficient: 0.999368

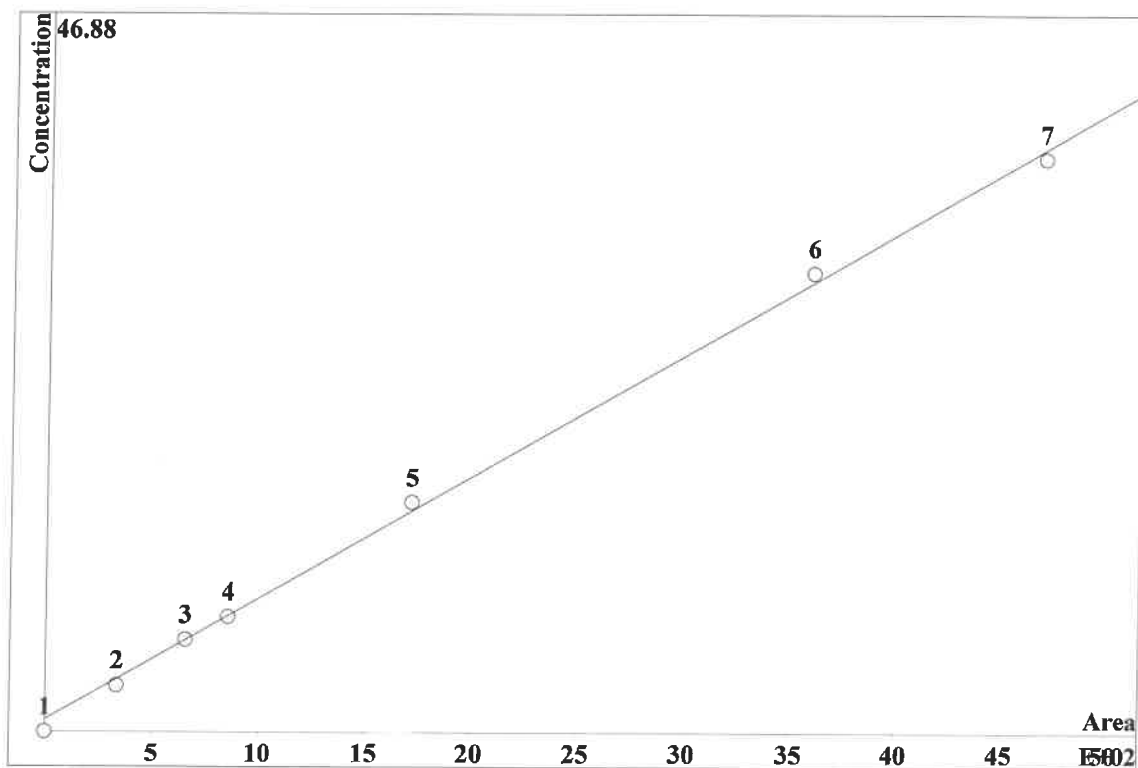

K3 = 0 K2 = 0 K1 = 0.159092 K0 = 15.88
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	8.988	333.3	3	20	24.98		
3	17.69	654.8	6	20	24.98		
4	23.65	855	7.5	20	24.81		
5	47.84	1716	15	20	24.81		
6	101.1	3596	30	20	24.81		
7	136.7	4692	37.5	20	24.81		

Report date: 8/17/2022 9:45:02 AM
Printed by: wet


Ident: STD1
Analysis from: 8/16/2022 9:55:22 AM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31381

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

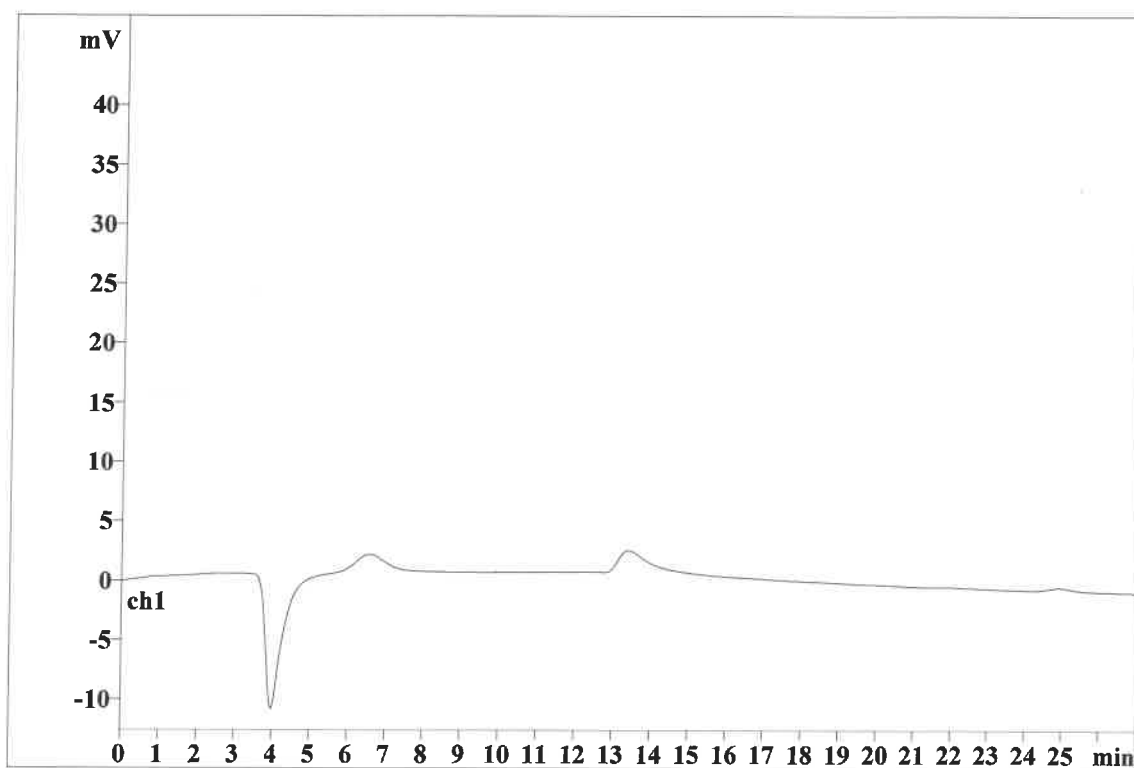

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2022 9:45:13 AM
Printed by: wet


Ident: STD2
Analysis from: 8/16/2022 10:25:00 AM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31382

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

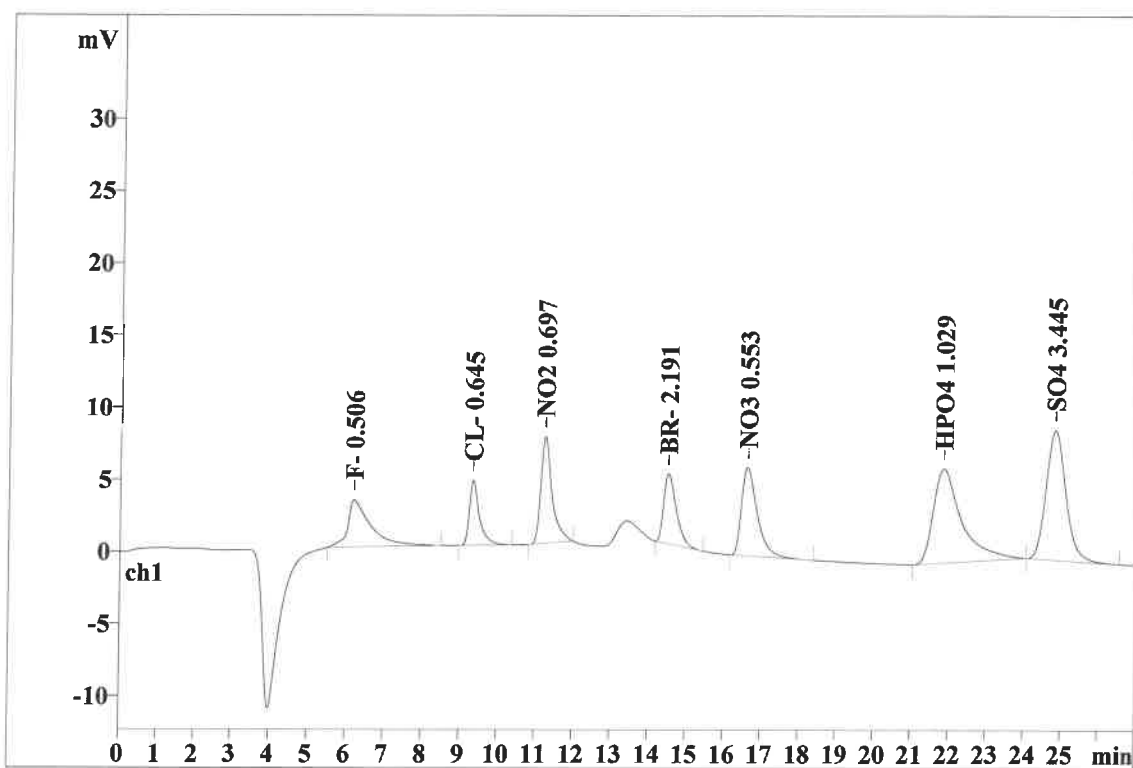

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.20	0.540	3.28	7.86	137.554	10.25
2	9.33	0.255	4.50	10.79	83.454	6.22
3	11.24	0.296	7.40	17.74	155.219	11.56
4	14.52	0.351	4.86	11.65	112.947	8.41
5	16.61	0.425	6.14	14.73	178.434	13.29
6	21.84	0.713	6.54	15.67	341.716	25.45
7	24.81	0.561	8.99	21.55	333.290	24.82
7	27.00	0.448	41.70	99.99	1342.614	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2022 9:45:24 AM
Printed by: wet


Ident: STD3
Analysis from: 8/16/2022 10:54:38 AM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31383

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

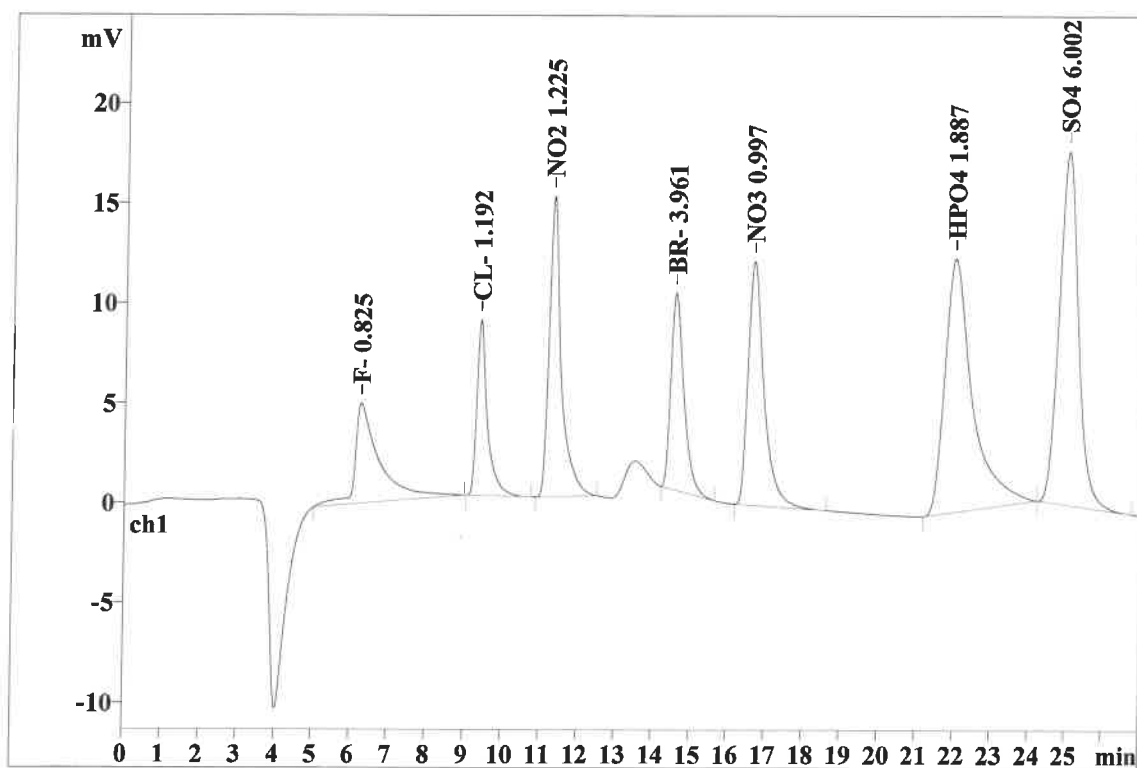

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.25	0.534	5.02	6.18	229.393	8.70
2	9.38	0.258	8.80	10.82	170.279	6.46
3	11.29	0.299	15.03	18.48	337.258	12.79
4	14.56	0.360	9.86	12.12	238.453	9.04
5	16.64	0.428	12.22	15.02	360.604	13.68
6	21.97	0.693	12.70	15.61	645.675	24.49
7	24.98	0.560	17.69	21.75	654.751	24.83
7	27.00	0.448	81.34	99.99	2636.411	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2022 9:45:32 AM
Printed by: wet


Ident: STD4
Analysis from: 8/16/2022 11:24:16 AM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31384

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

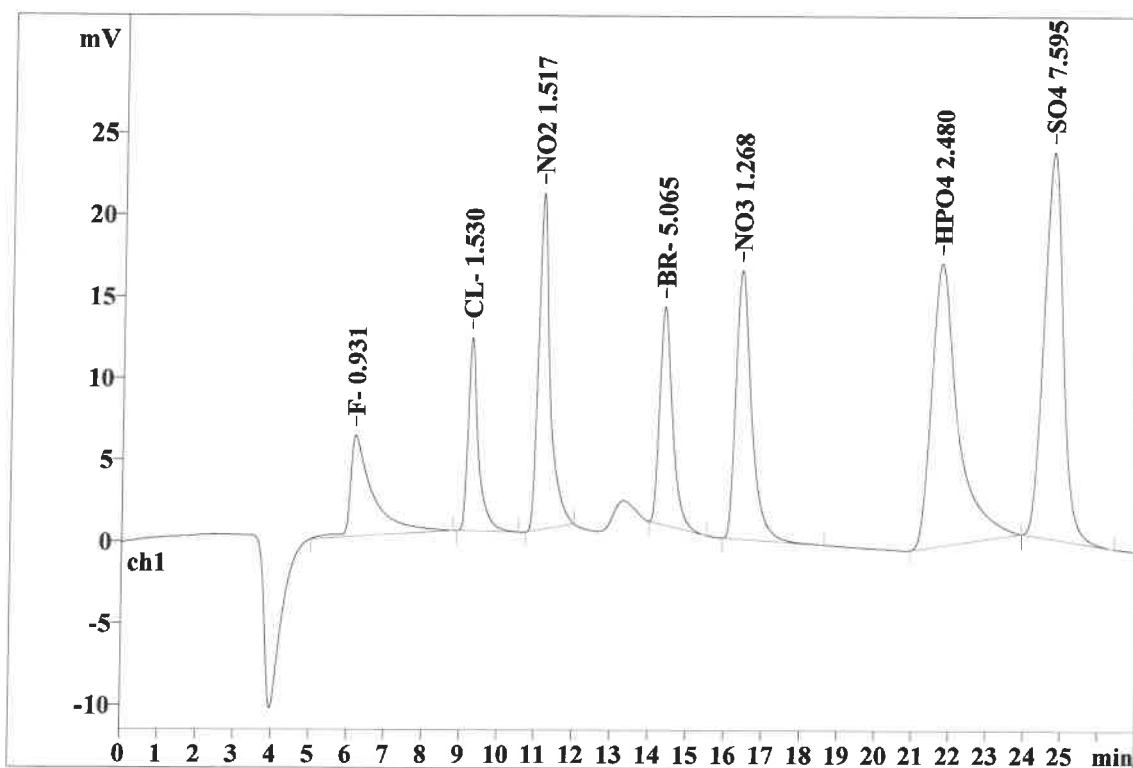

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.16	0.504	6.19	5.66	260.016	7.60
2	9.24	0.253	11.84	10.83	223.840	6.54
3	11.12	0.292	20.60	18.84	437.937	12.80
4	14.32	0.353	13.34	12.20	316.741	9.26
5	16.35	0.418	16.44	15.03	472.192	13.80
6	21.69	0.674	17.29	15.81	855.943	25.02
7	24.66	0.547	23.65	21.63	854.953	24.99
7	27.00	0.435	109.33	100.00	3421.622	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2022 9:45:40 AM
Printed by: wet


Ident: STD5
Analysis from: 8/16/2022 11:59:02 AM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31385

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

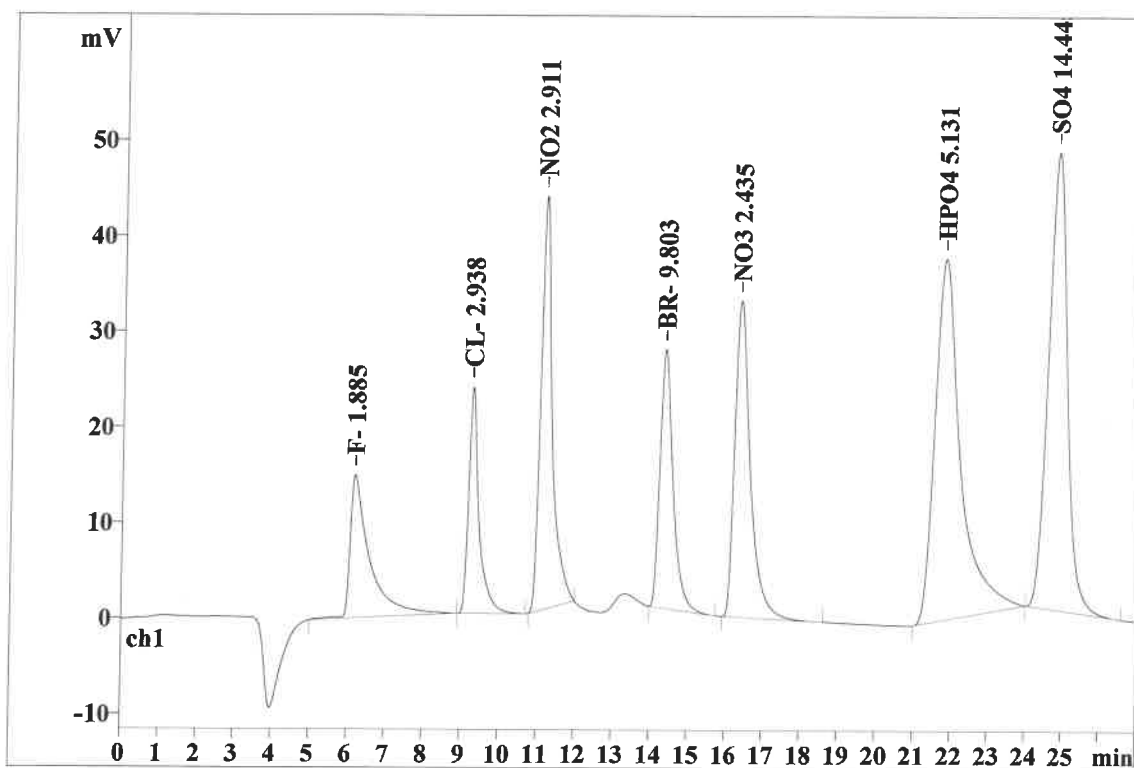

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.18	0.442	14.98	6.57	535.142	7.63
2	9.27	0.249	23.70	10.40	446.811	6.37
3	11.14	0.291	43.31	19.00	919.055	13.10
4	14.34	0.354	27.09	11.89	652.770	9.30
5	16.34	0.414	33.13	14.54	951.545	13.56
6	21.76	0.646	37.82	16.60	1795.735	25.59
7	24.77	0.542	47.84	20.99	1716.178	24.46
7	27.00	0.420	227.87	100.00	7017.235	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2022 9:49:44 AM
Printed by: wet


Ident: STD6
Analysis from: 8/16/2022 12:28:40 PM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31386

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

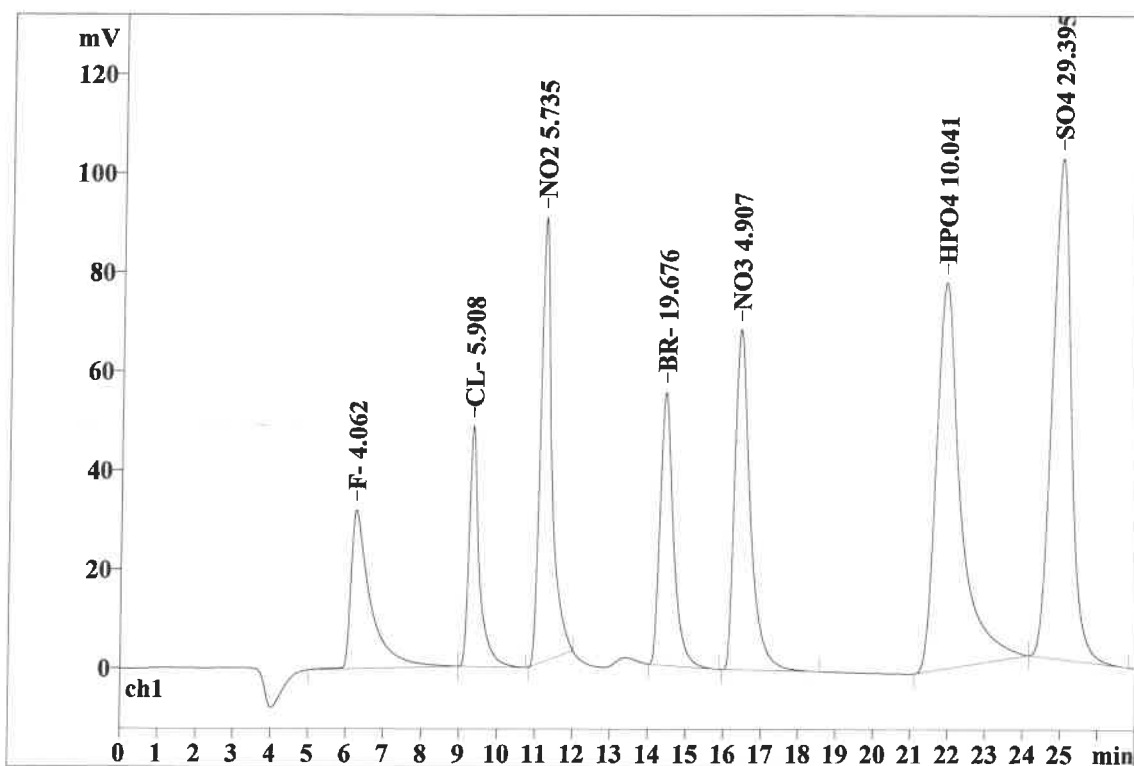

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.23	0.474	32.03	6.76	1162.463	8.06
2	9.31	0.247	48.66	10.27	917.492	6.36
3	11.18	0.291	89.84	18.96	1893.022	13.12
4	14.40	0.361	55.18	11.65	1352.985	9.38
5	16.37	0.412	68.77	14.52	1966.852	13.64
6	21.85	0.617	78.17	16.50	3536.231	24.52
7	24.91	0.535	101.09	21.34	3595.543	24.93
7	27.00	0.420	473.73	100.00	14424.587	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/17/2022 9:49:52 AM
Printed by: wet


Ident: STD7
Analysis from: 8/16/2022 12:58:18 PM
File: _2022-08-16_

Last save: 8/16/2022 2:27:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31387

Last save: 8/16/2022 2:10:

SAMPLE:
: IZ/MA
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

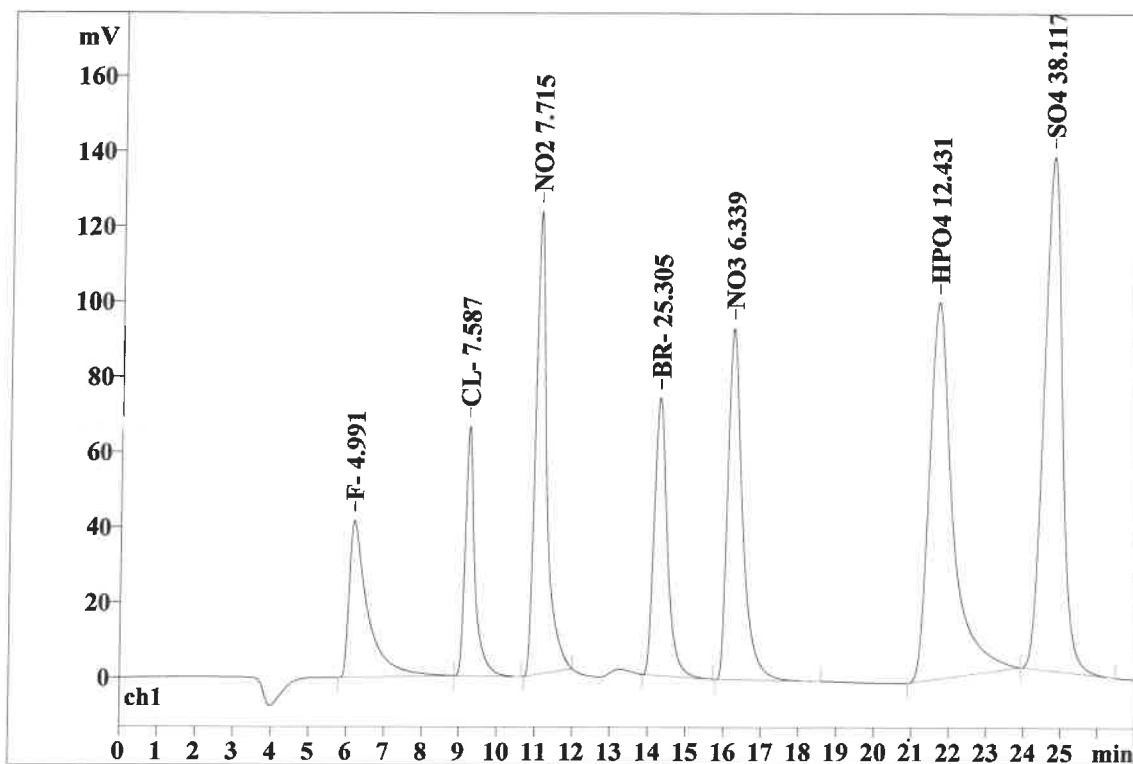

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.17	0.446	41.73	6.56	1430.221	7.70
2	9.22	0.239	66.43	10.45	1183.590	6.37
3	11.05	0.289	123.21	19.38	2576.153	13.87
4	14.25	0.350	73.96	11.63	1752.160	9.43
5	16.18	0.395	93.40	14.69	2555.259	13.76
6	21.63	0.597	100.33	15.78	4383.613	23.60
7	24.67	0.519	136.67	21.50	4692.029	25.26
7	27.00	0.405	635.73	100.00	18573.025	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/18/2022 9:38:21 AM
Printed by: wet


Ident: ICV
Analysis from: 8/16/2022 2:34:12 PM
File: _2022-08-16_

Last save: 8/16/2022 3:01:12 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31390

Last save: 8/16/2022 2:27:

SAMPLE:
: IZ/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

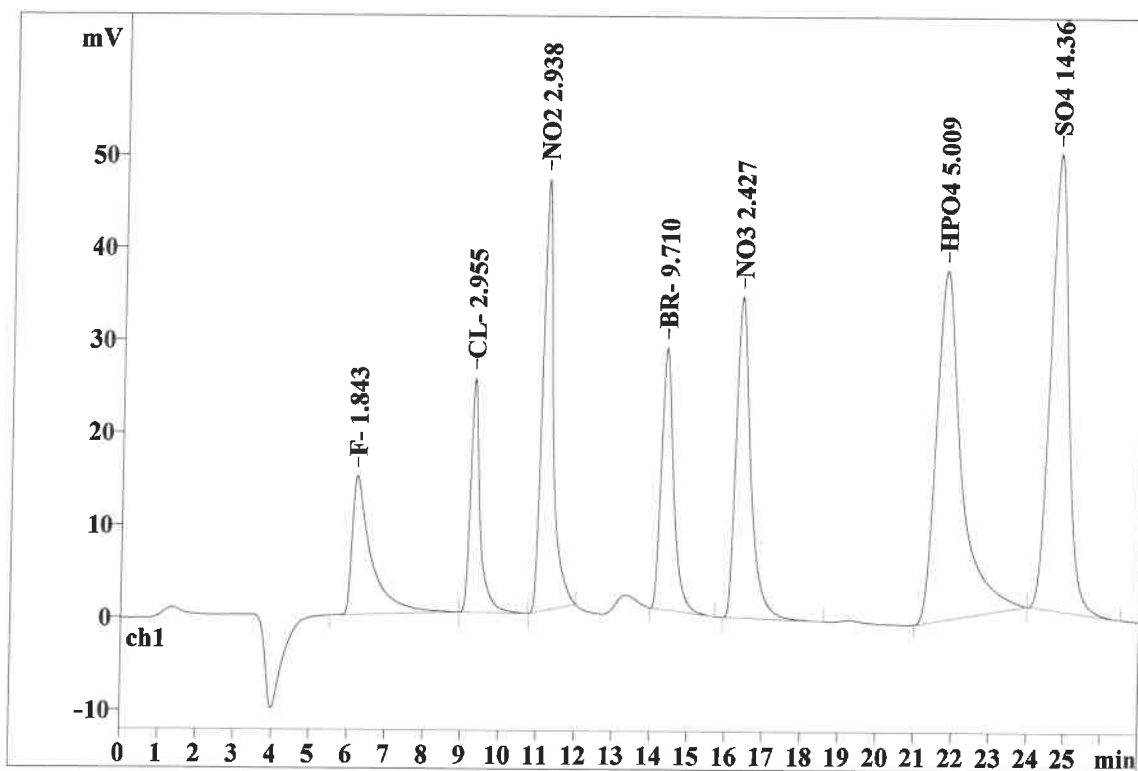

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.19	0.440	15.04	6.34	522.792	7.52
2	9.28	0.238	25.29	10.66	449.568	6.47
3	11.14	0.277	46.65	19.67	928.358	13.35
4	14.34	0.334	28.32	11.94	646.221	9.29
5	16.33	0.395	34.67	14.62	948.156	13.64
6	21.73	0.629	37.79	15.94	1752.406	25.20
7	24.74	0.522	49.39	20.82	1705.890	24.53
7	27.00	0.405	237.16	100.00	6953.390	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/18/2022 9:38:31 AM
Printed by: wet


Ident: ICB
Analysis from: 8/16/2022 3:04:25 PM
File: _2022-08-16_

Last save: 8/16/2022 3:31:25 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31391

Last save: 8/16/2022 2:27:

SAMPLE:
: IZ/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

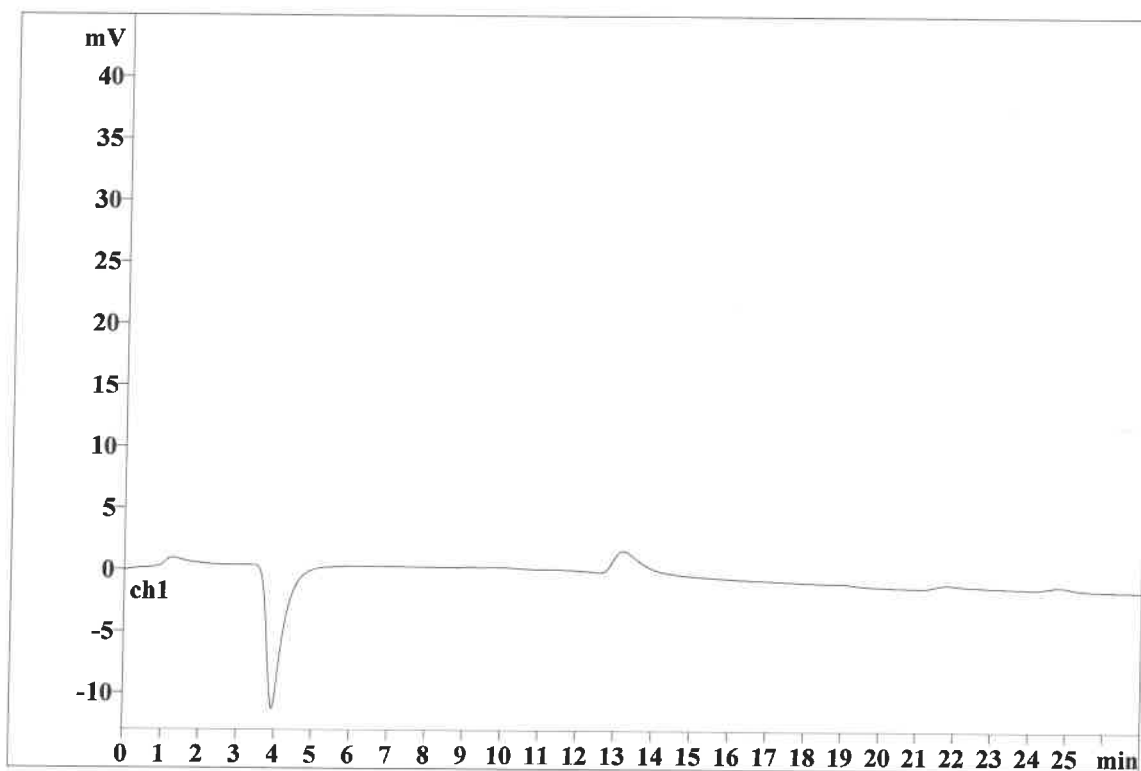

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:13:43 AM
Printed by: wet


Ident: CCV
Analysis from: 8/19/2022 5:40:50 PM
File: _2022-08-19_

Last save: 8/19/2022 6:07:51 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31484

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

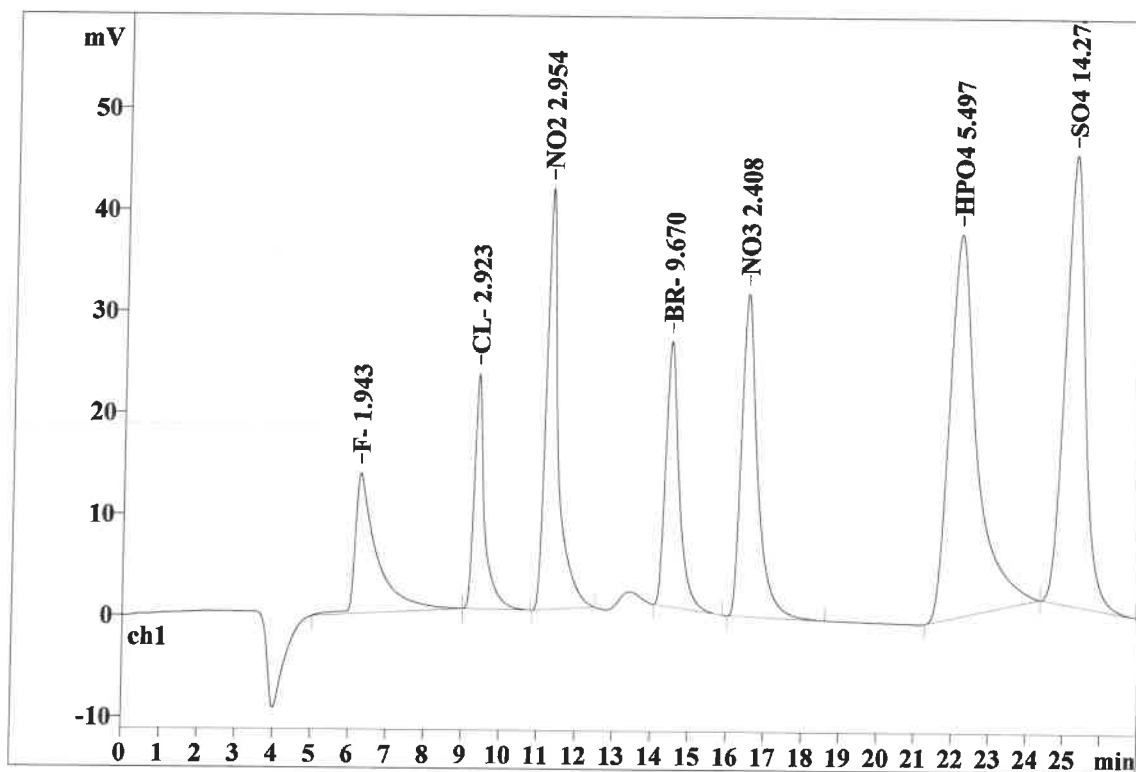

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.24	0.489	13.84	6.33	551.580	7.73
2	9.35	0.245	23.17	10.60	444.509	6.23
3	11.23	0.289	41.52	18.99	933.680	13.09
4	14.43	0.355	26.15	11.96	643.366	9.02
5	16.44	0.420	31.76	14.53	940.159	13.18
6	22.09	0.696	37.76	17.27	1925.516	26.99
7	25.15	0.572	44.39	20.31	1694.613	23.76
7	27.00	0.438	218.58	100.00	7133.423	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:13:53 AM
Printed by: wet


Ident: CCB
Analysis from: 8/19/2022 6:10:28 PM
File: _2022-08-19_

Last save: 8/19/2022 6:37:28 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31485

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

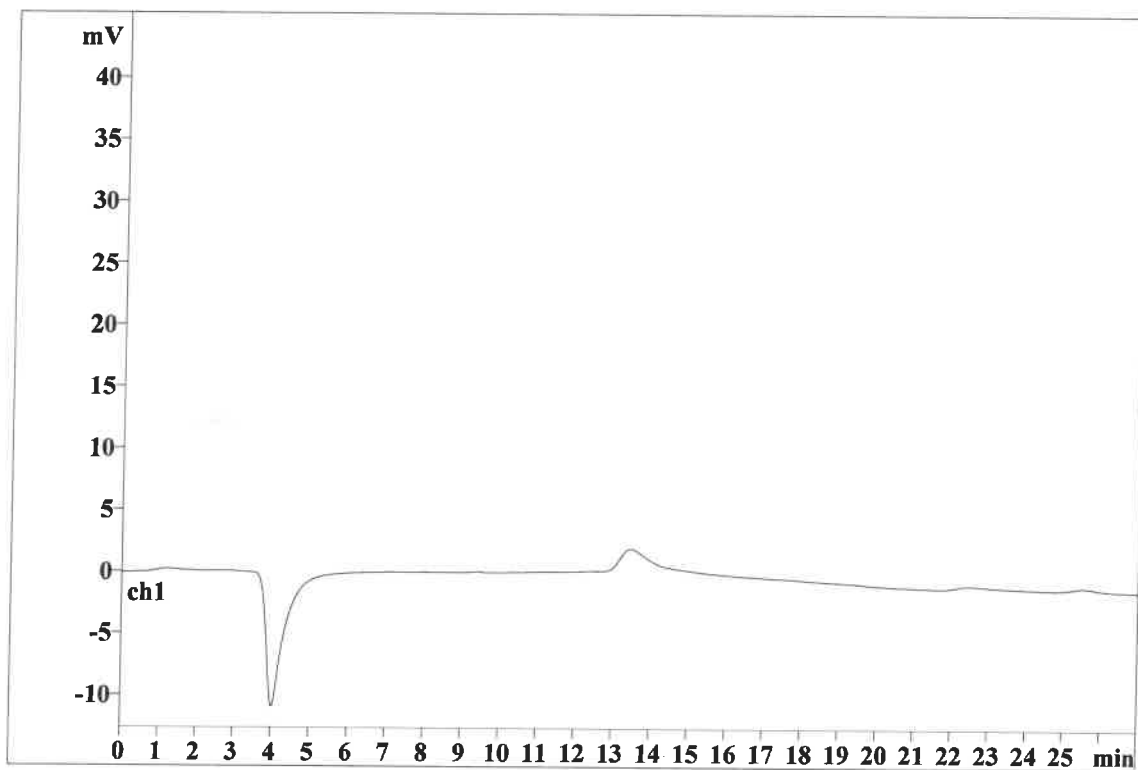

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:14:03 AM
Printed by: wet


Ident: LB121643BLW
Analysis from: 8/19/2022 6:40:06 PM
File: _2022-08-19_

Last save: 8/23/2022 9:13:12 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31486

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

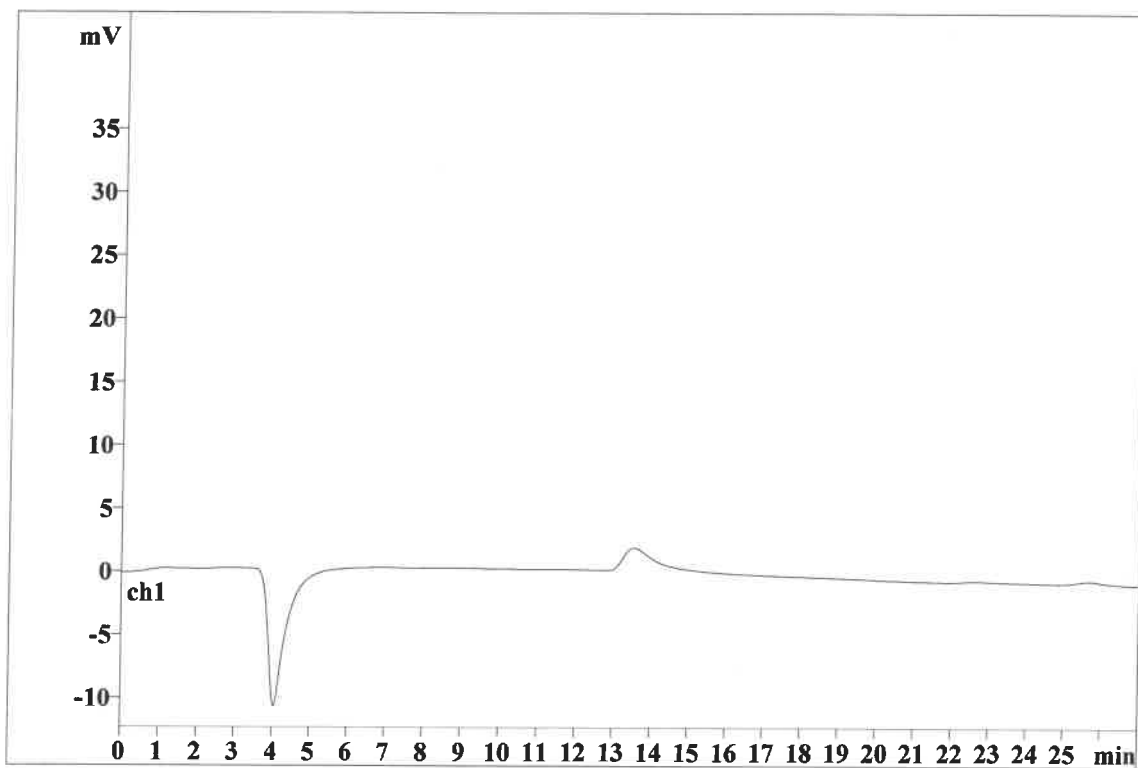

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:14:13 AM
Printed by: wet


Ident: LB121643BSW
Analysis from: 8/19/2022 7:09:44 PM
File: _2022-08-19_

Last save: 8/23/2022 9:13:12 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31487

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

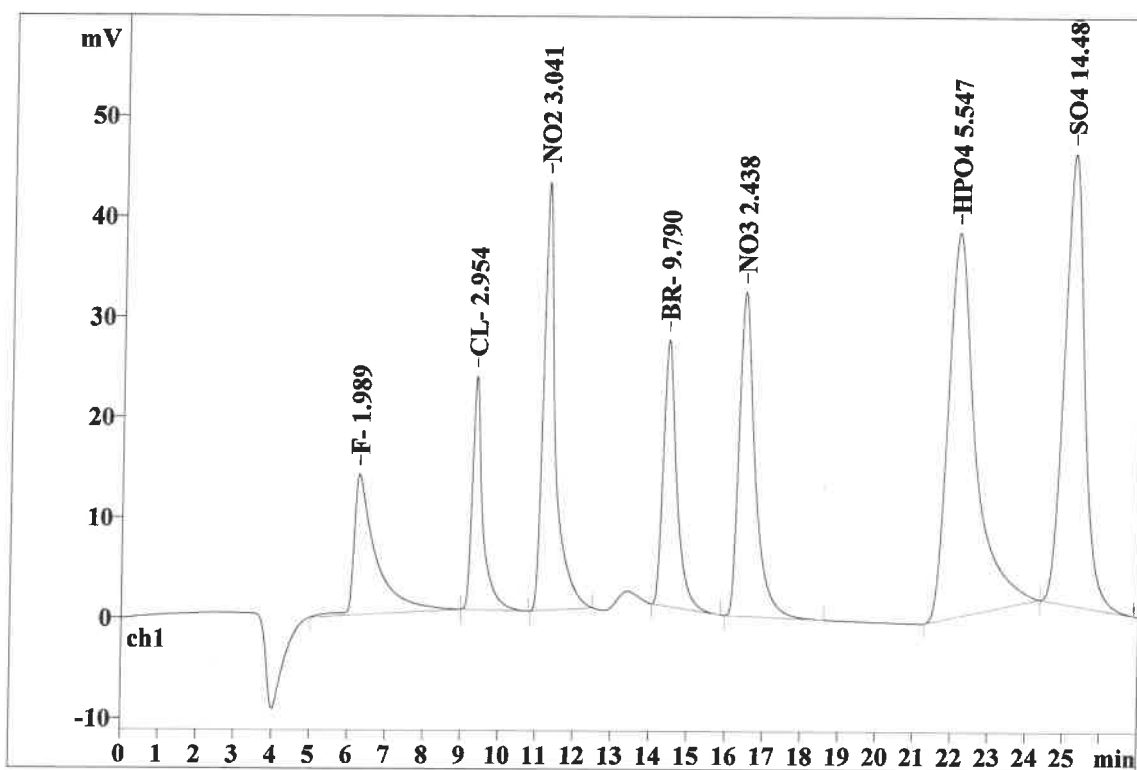

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.25	0.497	14.01	6.31	564.939	7.80
2	9.35	0.247	23.26	10.48	449.353	6.20
3	11.22	0.290	42.63	19.20	963.601	13.30
4	14.42	0.357	26.53	11.95	651.863	9.00
5	16.43	0.421	32.28	14.54	952.674	13.15
6	22.11	0.694	38.31	17.26	1943.068	26.82
7	25.18	0.575	44.97	20.26	1720.531	23.74
7	27.00	0.440	221.99	100.00	7246.030	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:14:26 AM
Printed by: wet


Ident: N4264-02
Analysis from: 8/19/2022 7:39:27 PM
File: _2022-08-19_

Last save: 8/19/2022 8:06:27 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31488

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 45
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

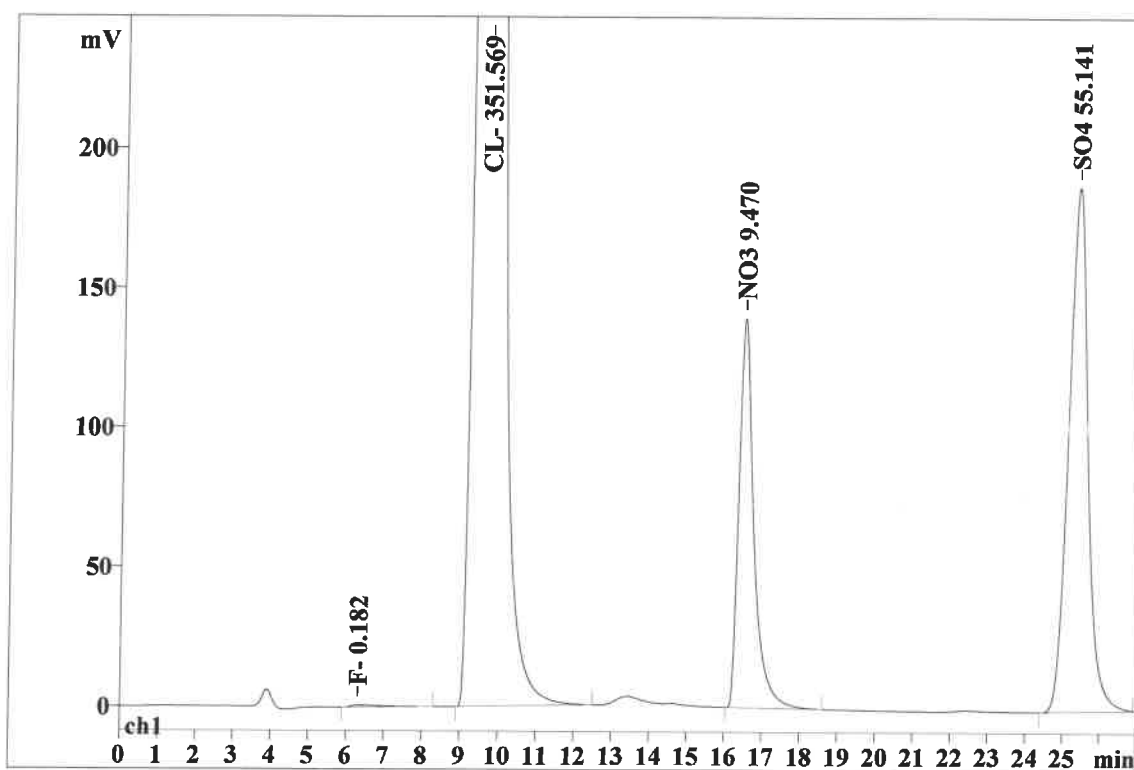

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.33	0.896	0.73	0.04	44.100	0.07
2	9.65	0.535	1576.88	82.79	55691.137	83.86
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.46	0.391	139.32	7.31	3841.262	5.78
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.29	0.543	187.76	9.86	6832.155	10.29
7	27.00	0.338	1904.69	100.00	66408.655	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:14:39 AM
Printed by: wet


Ident: N4264-02MS
Analysis from: 8/19/2022 8:09:05 PM
File: _2022-08-19_

Last save: 8/19/2022 8:36:06 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31489

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 46
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

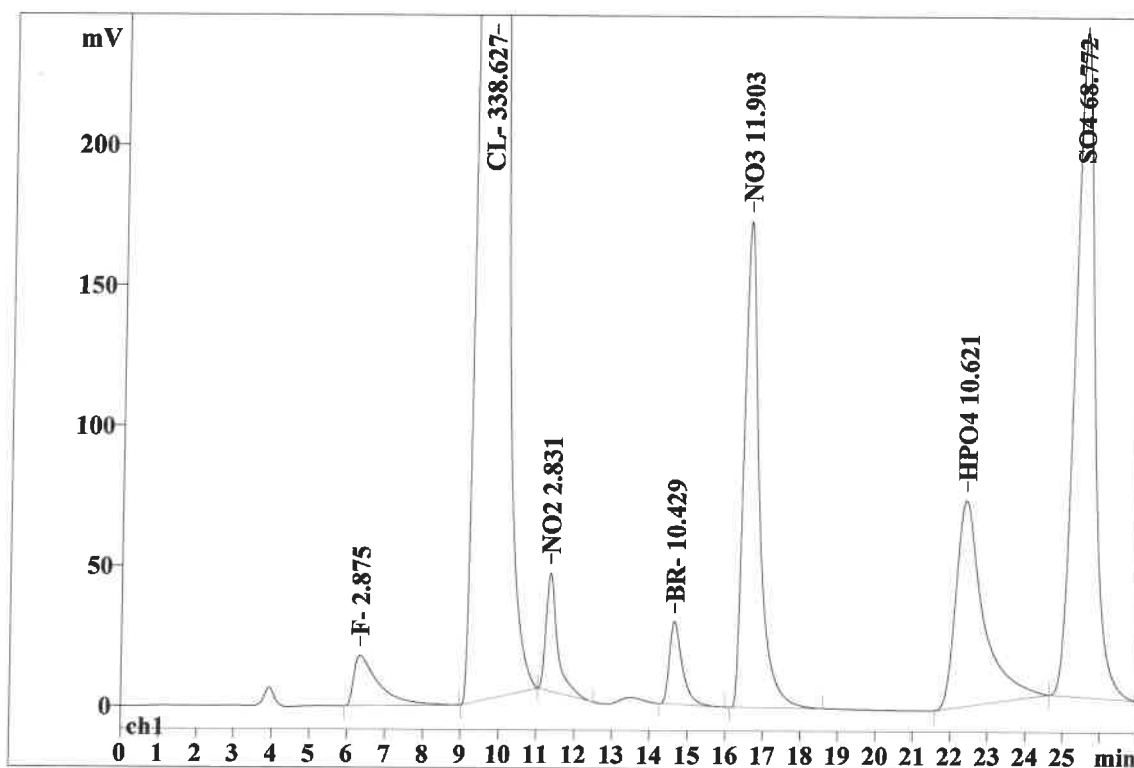

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.32	0.619	17.99	0.84	820.356	1.12
2	9.69	0.519	1566.92	73.23	53640.233	73.30
3	11.34	0.282	42.07	1.97	891.164	1.22
4	14.63	0.344	29.54	1.38	697.187	0.95
5	16.53	0.395	173.30	8.10	4841.069	6.62
6	22.36	0.683	73.50	3.43	3741.746	5.11
7	25.42	0.541	236.45	11.05	8545.755	11.68
7	27.00	0.483	2139.77	100.00	73177.509	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:14:52 AM
Printed by: wet


Ident: N4264-02MSD
Analysis from: 8/19/2022 8:38:44 PM
File: _2022-08-19_

Last save: 8/19/2022 9:05:44 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31490

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 47
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

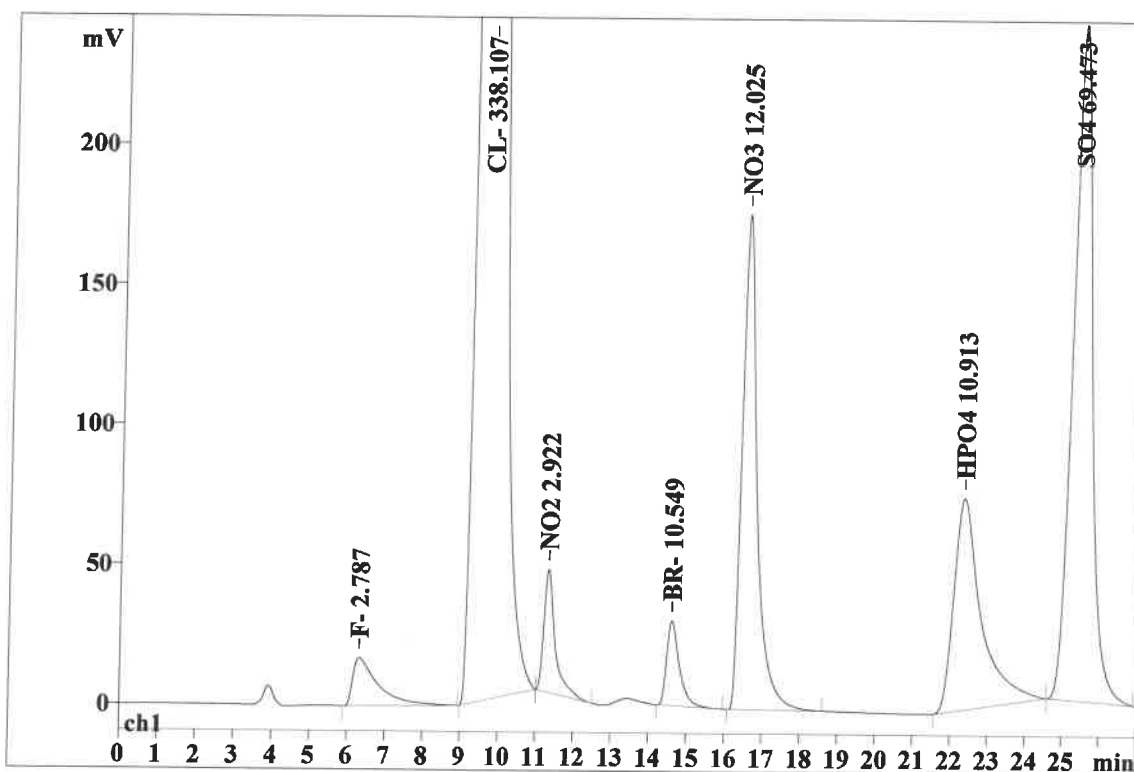

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.31	0.624	17.17	0.80	794.848	1.08
2	9.67	0.519	1569.50	72.86	53557.968	73.02
3	11.31	0.281	43.88	2.04	922.855	1.26
4	14.59	0.340	30.30	1.41	705.696	0.96
5	16.49	0.392	176.74	8.20	4891.097	6.67
6	22.31	0.681	75.64	3.51	3845.337	5.24
7	25.37	0.536	240.96	11.19	8633.914	11.77
7	27.00	0.482	2154.19	100.00	73351.714	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:15:14 AM
Printed by: wet


Ident: N4262-01
Analysis from: 8/19/2022 9:08:21 PM
File: _2022-08-19_

Last save: 8/19/2022 9:35:21 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31491

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 48
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

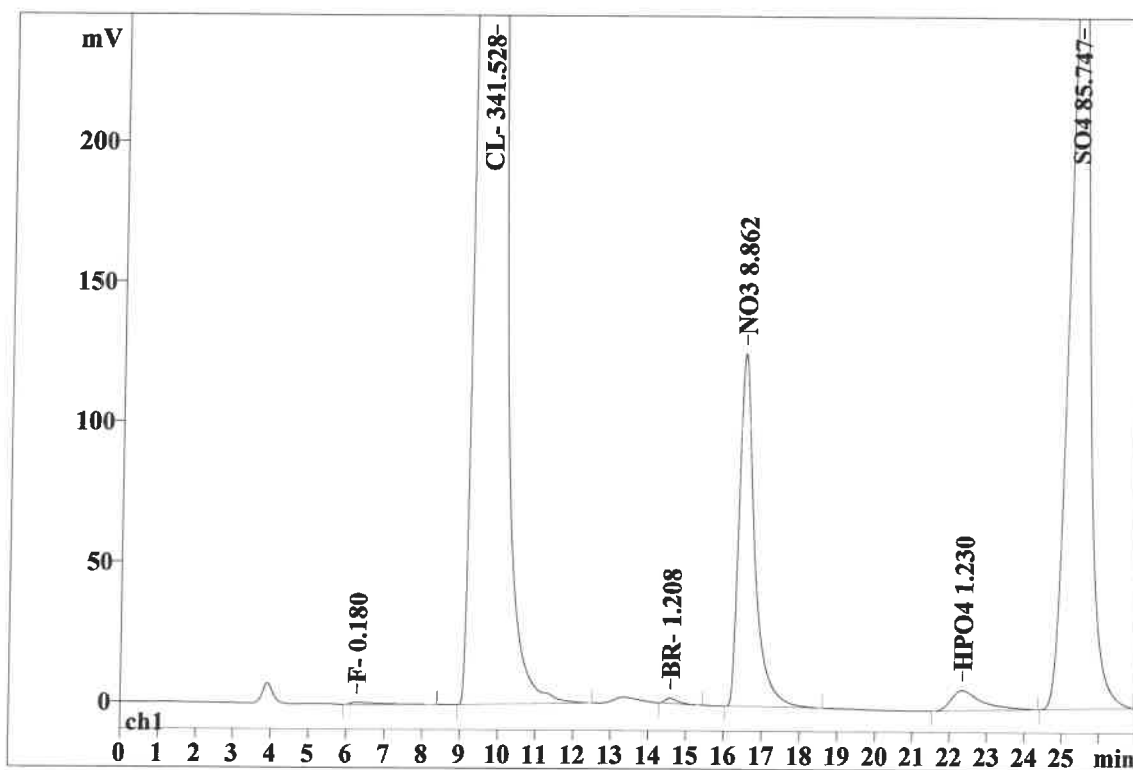

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.27	0.735	0.81	0.04	43.594	0.06
2	9.67	0.520	1570.37	78.70	54099.947	78.55
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.58	0.345	1.90	0.10	43.271	0.06
5	16.46	0.402	125.91	6.31	3591.586	5.21
6	22.33	0.787	7.27	0.36	412.660	0.60
7	25.29	0.551	289.28	14.50	10679.773	15.51
7	27.00	0.477	1995.53	100.00	68870.831	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:15:24 AM
Printed by: wet


Ident: N4262-02
Analysis from: 8/19/2022 9:37:59 PM
File: _2022-08-19_

Last save: 8/19/2022 10:05:00 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31492

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 49
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

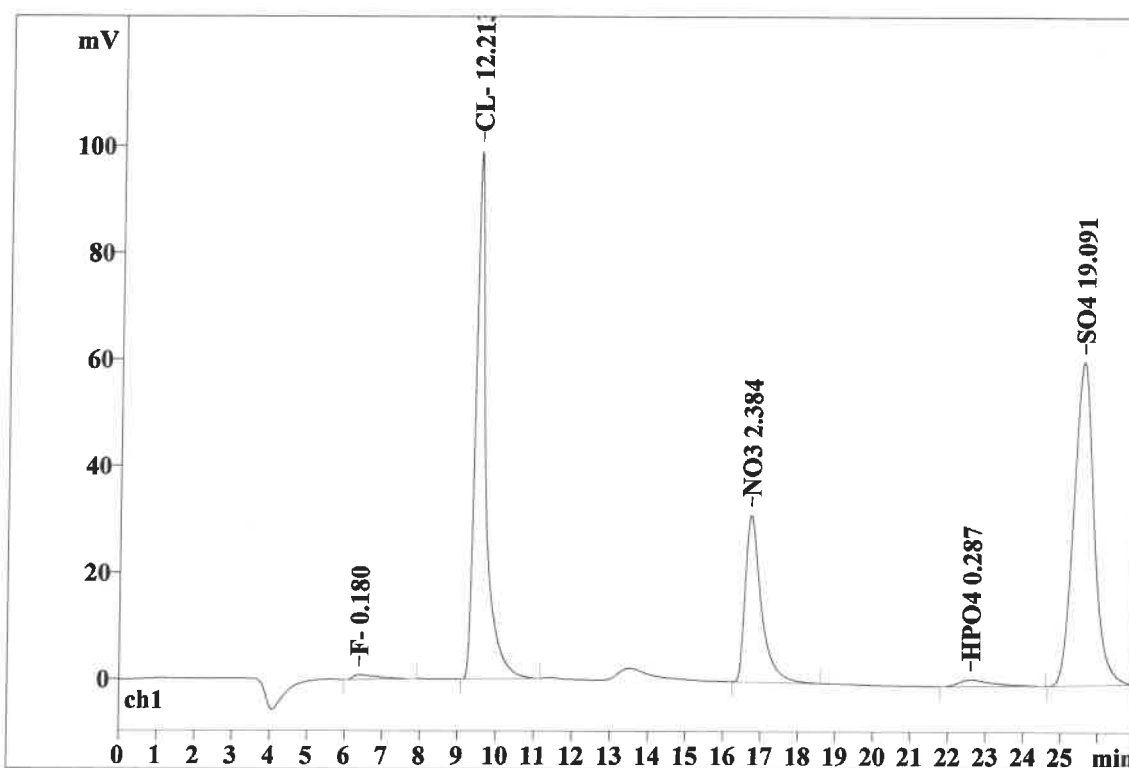

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.37	0.729	0.93	0.48	43.713	0.83
2	9.48	0.245	99.01	51.25	1916.675	36.37
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.71	0.423	31.32	16.21	930.522	17.66
6	22.59	0.883	1.26	0.65	78.405	1.49
7	25.54	0.567	60.67	31.40	2300.139	43.65
7	27.00	0.407	193.19	100.00	5269.454	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:15:34 AM
Printed by: wet


Ident: N4262-03
Analysis from: 8/19/2022 10:07:37 PM
File: _2022-08-19_

Last save: 8/19/2022 10:34:37 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31493

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 50
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

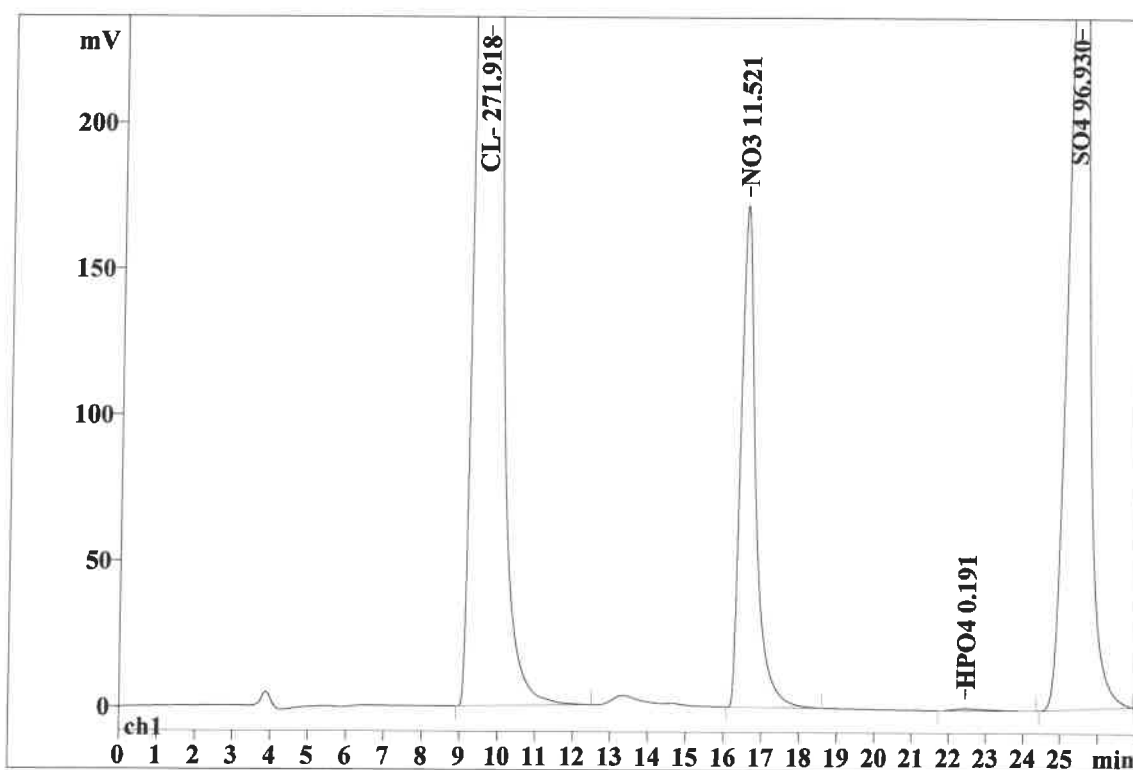

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.56	0.412	1507.21	74.53	43069.486	71.92
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.49	0.386	171.87	8.50	4683.836	7.82
6	22.44	0.880	0.72	0.04	44.429	0.07
7	25.29	0.528	342.44	16.93	12085.625	20.18
7	27.00	0.315	2022.24	100.00	59883.376	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:15:48 AM
 Printed by: wet


Ident: N4262-04
 Analysis from: 8/19/2022 10:37:16 PM
 File: _2022-08-19_

Last save: 8/19/2022 11:04:16 PM

Method: AnionsIC2-081622.mtw
 Run operator: wet
 Analysis number: 31494

Last save: 8/19/2022 9:42:

SAMPLE:
 : IZ/MA
 Vial number: 51
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

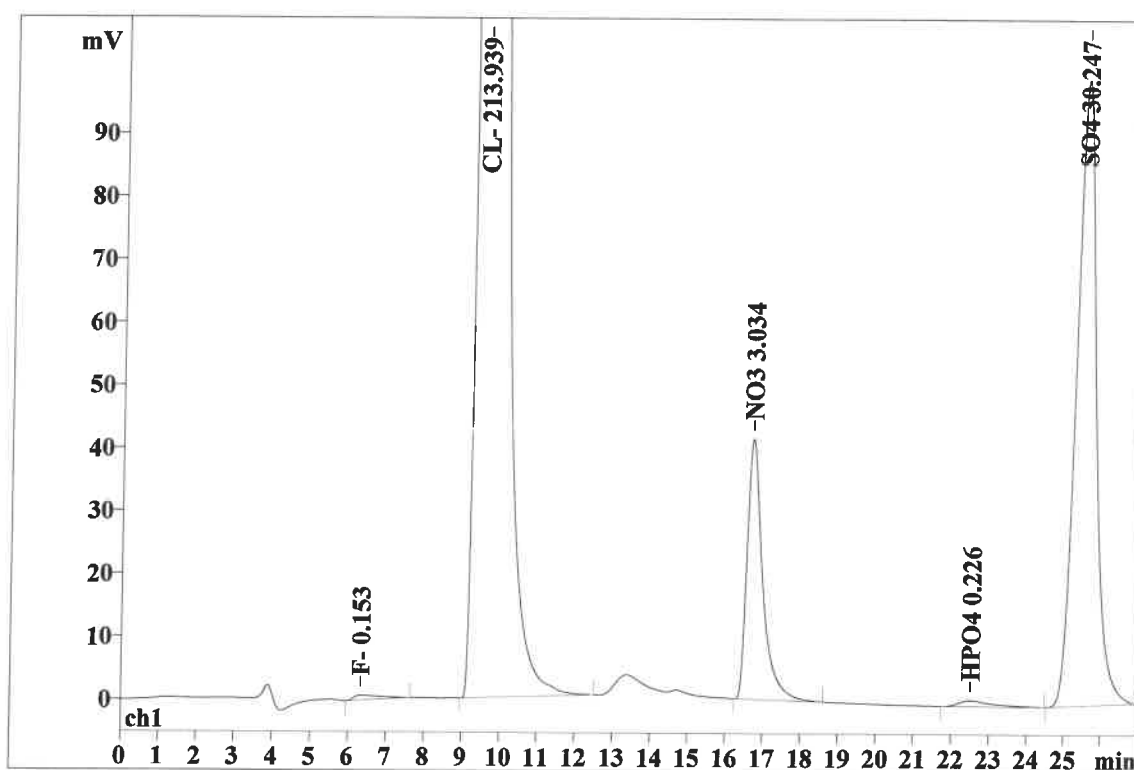

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.33	0.727	0.77	0.05	35.668	0.09
2	9.55	0.332	1399.08	90.76	33882.233	87.16
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.68	0.413	41.38	2.68	1197.595	3.08
6	22.51	0.854	0.95	0.06	56.768	0.15
7	25.46	0.558	99.33	6.44	3702.599	9.52
7	27.00	0.412	1541.51	100.00	38874.863	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 8/23/2022 9:15:58 AM
Printed by: wet


Ident: N4262-05
Analysis from: 8/19/2022 11:06:53 PM
File: _2022-08-19_

Last save: 8/19/2022 11:33:53 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31495

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 52
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

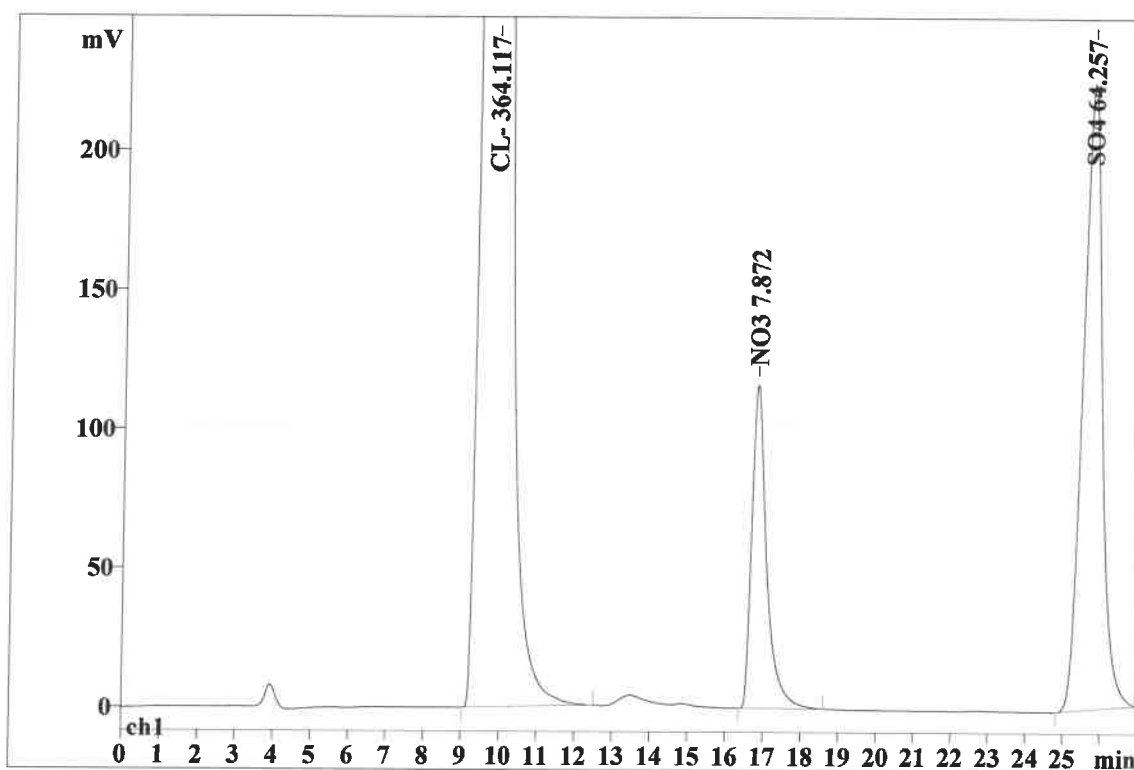

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.79	0.551	1580.90	82.26	57679.470	83.78
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.78	0.391	116.09	6.04	3185.124	4.63
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.64	0.535	224.87	11.70	7978.135	11.59
7	27.00	0.211	1921.86	100.00	68842.729	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:16:10 AM
Printed by: wet


Ident: CCV
Analysis from: 8/19/2022 11:36:33 PM
File: _2022-08-19_

Last save: 8/20/2022 12:03:33 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31496

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

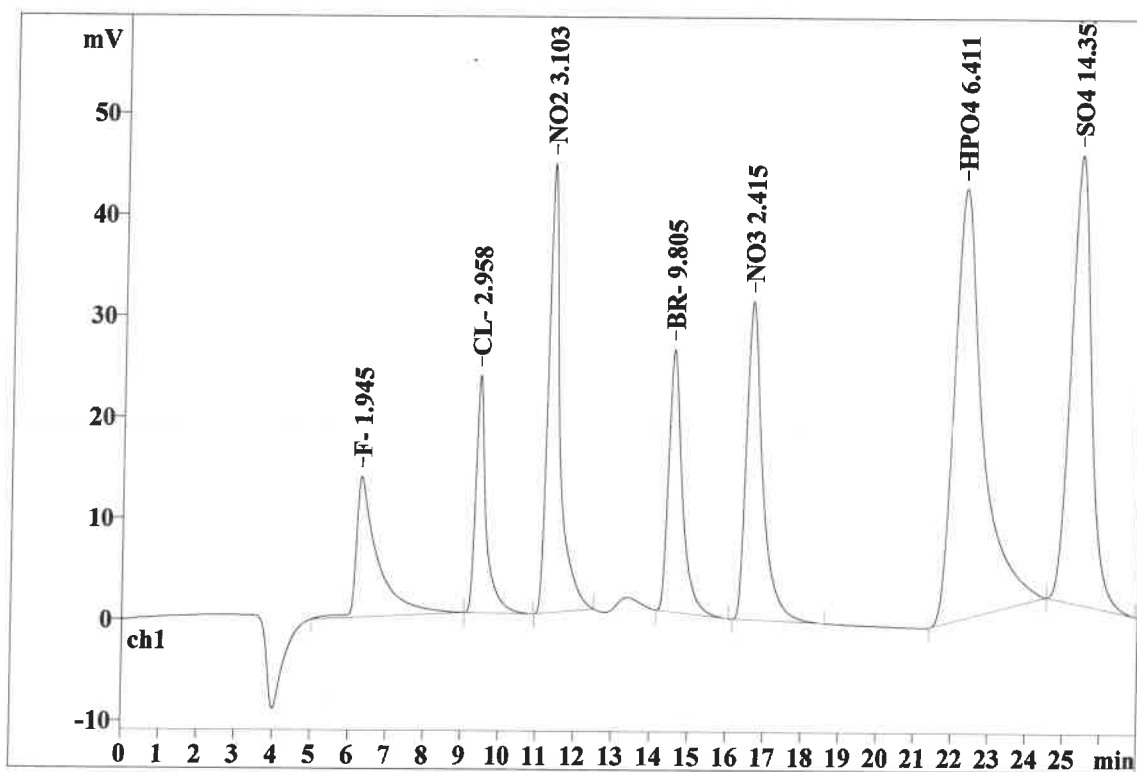

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.29	0.482	13.89	6.14	552.334	7.33
2	9.43	0.247	23.47	10.38	450.065	5.97
3	11.33	0.291	44.40	19.63	985.082	13.07
4	14.54	0.359	25.94	11.47	652.934	8.66
5	16.60	0.425	31.45	13.91	943.173	12.51
6	22.25	0.719	42.59	18.84	2249.261	29.84
7	25.34	0.577	44.37	19.62	1704.411	22.61
7	27.00	0.443	226.12	100.00	7537.259	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:16:19 AM
Printed by: wet


Ident: CCB
Analysis from: 8/20/2022 12:06:10 AM
File: _2022-08-20_

Last save: 8/20/2022 12:33:10 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31497

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

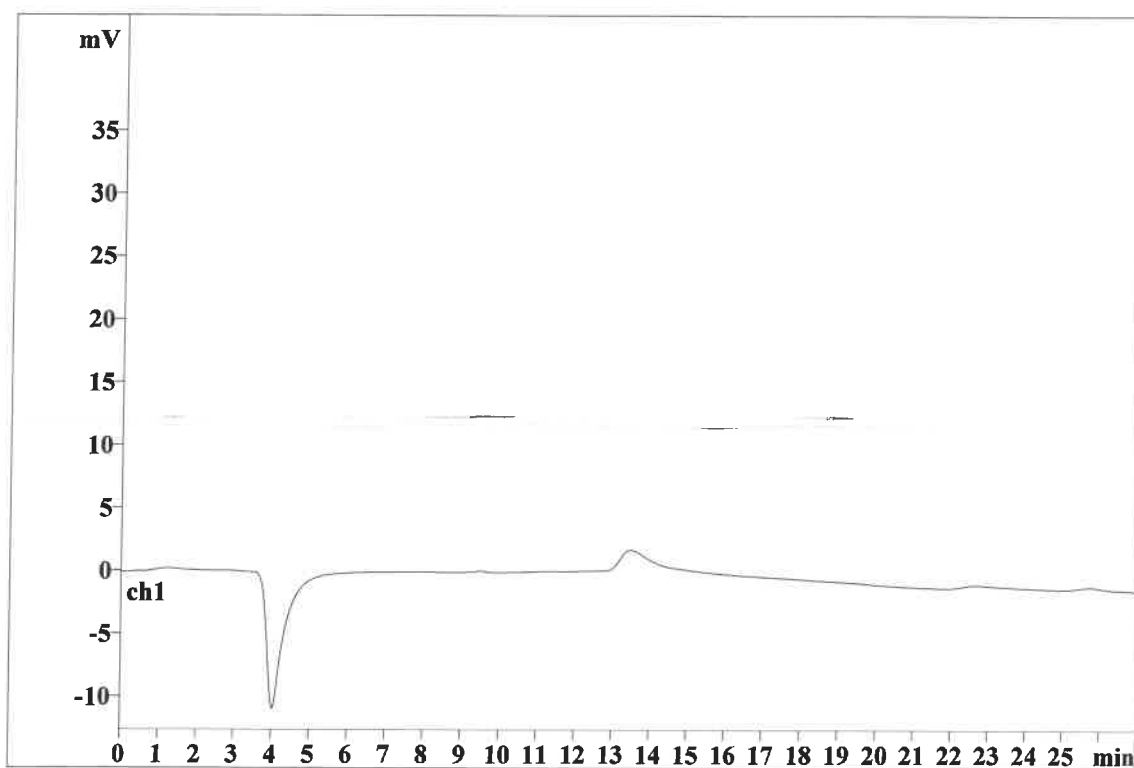

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:16:29 AM
 Printed by: wet


Ident: N4262-06
 Analysis from: 8/20/2022 12:35:50 AM
 File: _2022-08-20_

Last save: 8/20/2022 1:02:51 AM

Method: AnionsIC2-081622.mtw
 Run operator: wet
 Analysis number: 31498

Last save: 8/19/2022 9:42:

SAMPLE:
 : IZ/MA
 Vial number: 53
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

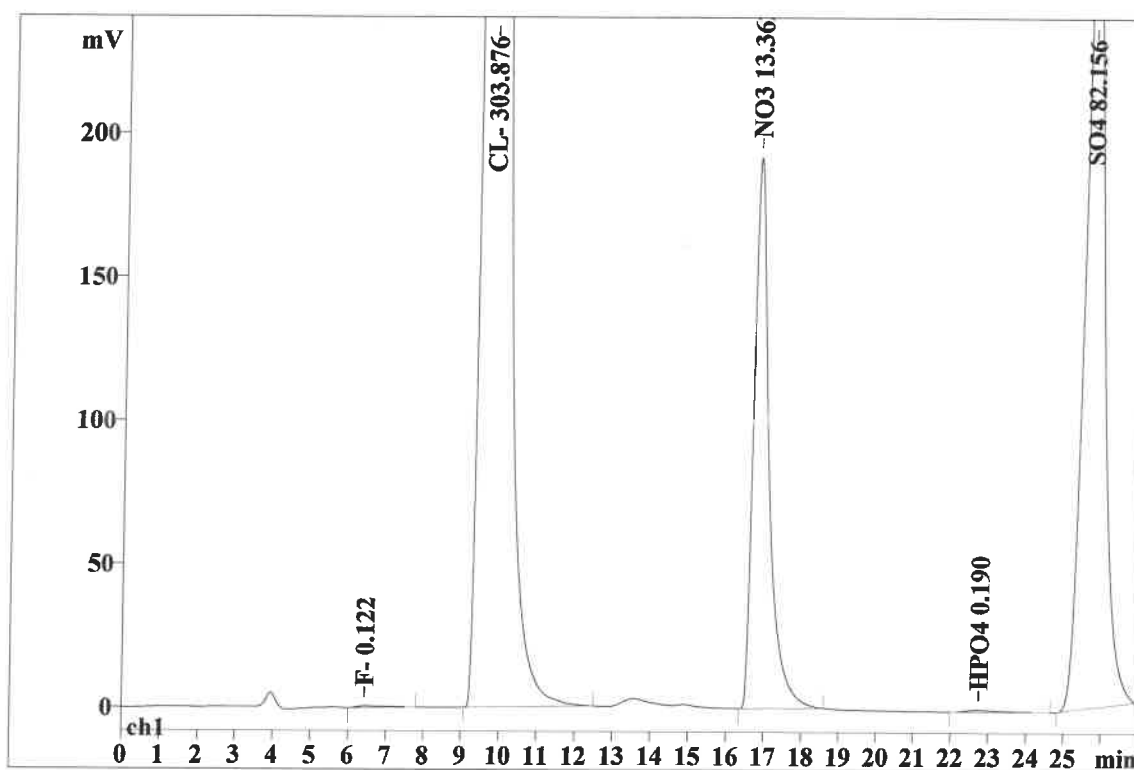

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.42	0.847	0.51	0.03	26.879	0.04
2	9.75	0.458	1532.69	76.35	48133.605	75.36
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.77	0.400	191.90	9.56	5440.276	8.52
6	22.74	0.862	0.73	0.04	43.982	0.07
7	25.65	0.546	281.65	14.03	10228.317	16.01
7	27.00	0.445	2007.48	100.00	63873.058	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 8/23/2022 9:16:39 AM
Printed by: wet


Ident: N4262-07
Analysis from: 8/20/2022 1:05:28 AM
File: _2022-08-20_

Last save: 8/20/2022 1:32:28 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31499

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 54
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

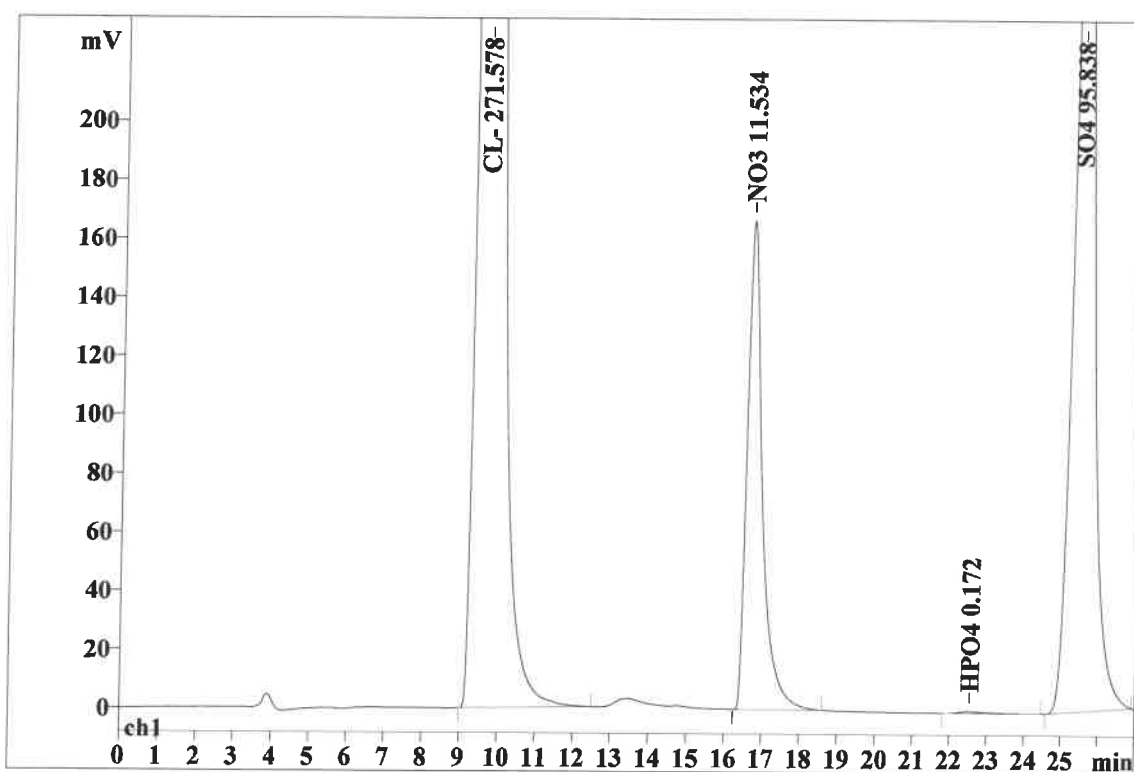

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.63	0.407	1499.00	75.05	43015.625	72.06
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.65	0.398	166.40	8.33	4689.253	7.86
6	22.54	0.859	0.63	0.03	37.843	0.06
7	25.43	0.539	331.47	16.59	11948.363	20.02
7	27.00	0.315	1997.49	100.00	59691.084	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:16:51 AM
Printed by: wet


Ident: CCV
Analysis from: 8/20/2022 1:35:08 AM
File: _2022-08-20_

Last save: 8/20/2022 2:02:08 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31500

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

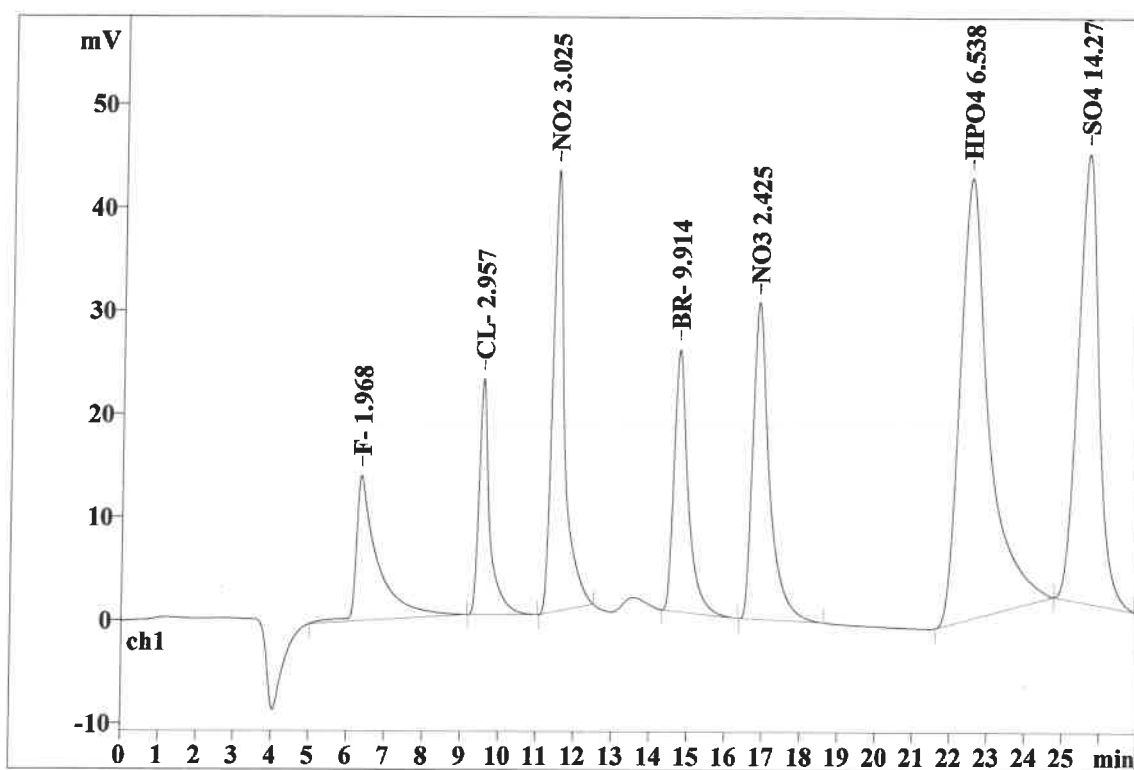

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.34	0.469	14.12	6.35	558.828	7.39
2	9.53	0.251	22.91	10.30	449.888	5.95
3	11.46	0.297	42.79	19.25	958.233	12.67
4	14.72	0.368	25.39	11.42	660.693	8.73
5	16.82	0.435	30.74	13.83	947.258	12.52
6	22.44	0.731	42.82	19.26	2294.382	30.33
7	25.57	0.586	43.53	19.58	1695.258	22.41
7	27.00	0.448	222.28	100.00	7564.539	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:17:41 AM
Printed by: wet


Ident: CCB
Analysis from: 8/20/2022 2:04:47 AM
File: _2022-08-20_

Last save: 8/20/2022 2:31:47 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31501

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

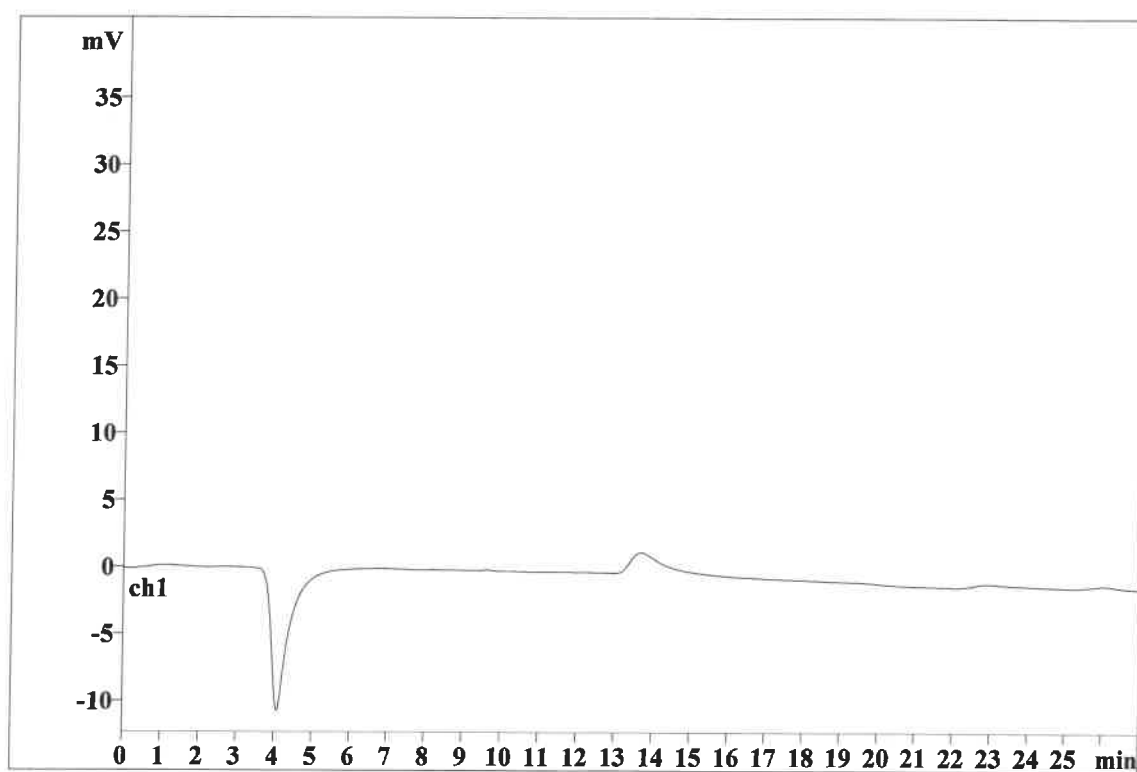

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:17:54 AM
Printed by: wet


Ident: CCV
Analysis from: 8/22/2022 10:55:15 AM
File: _2022-08-22_

Last save: 8/22/2022 11:26:08 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31507

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 36
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

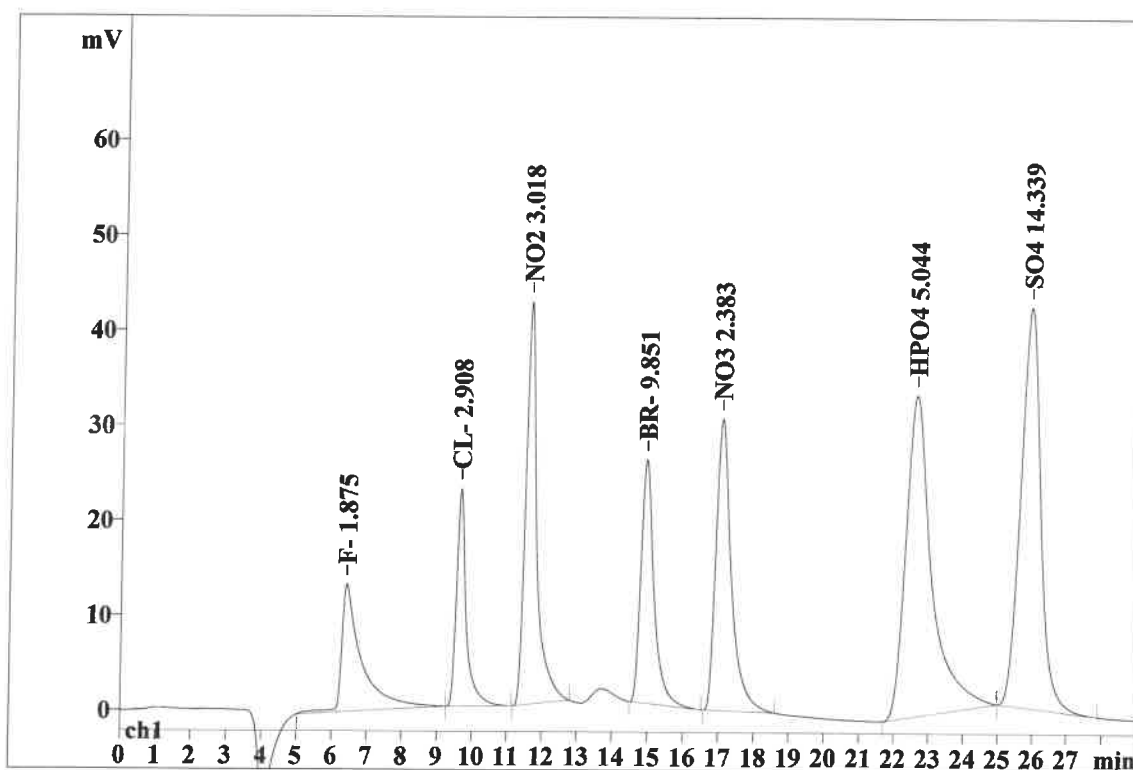

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.40	0.458	13.44	6.37	532.203	7.62
2	9.63	0.255	22.91	10.85	442.089	6.33
3	11.58	0.302	42.41	20.09	955.983	13.69
4	14.90	0.365	25.68	12.16	656.210	9.40
5	17.02	0.433	30.70	14.54	930.169	13.32
6	22.56	0.708	33.82	16.02	1764.819	25.27
7	25.84	0.605	42.16	19.97	1702.748	24.38
7	29.00	0.447	211.11	100.00	6984.220	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:18:02 AM
Printed by: wet


Ident: CCB
Analysis from: 8/22/2022 11:27:42 AM
File: _2022-08-22_

Last save: 8/22/2022 11:56:43 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31508

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

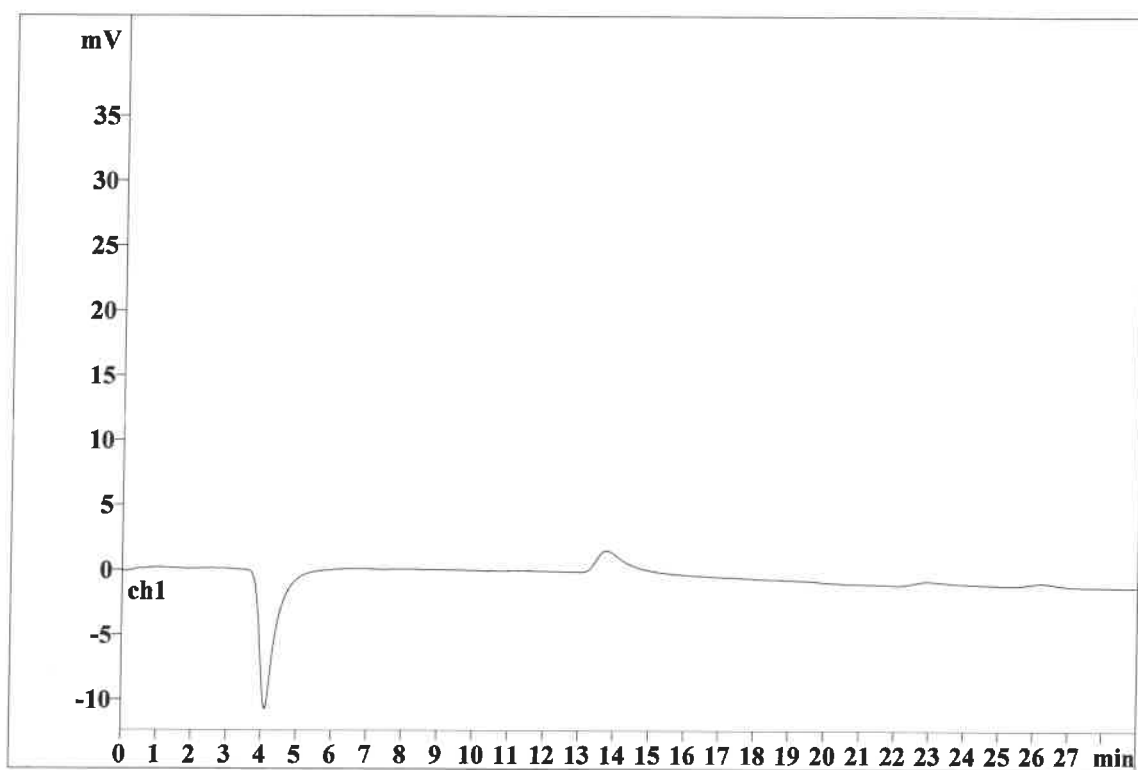

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:18:12 AM
Printed by: wet


Ident: LB121643BLW2
Analysis from: 8/22/2022 11:59:20 AM
File: _2022-08-22_

Last save: 8/23/2022 9:13:12 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31509

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

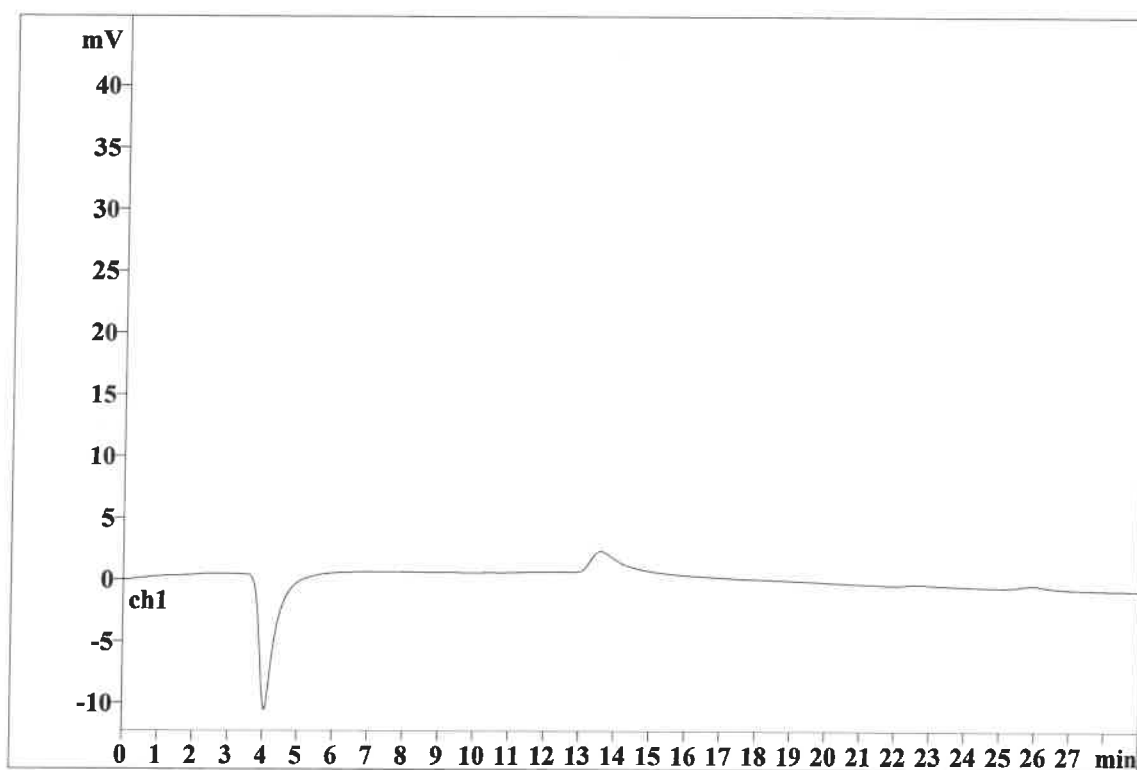

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:18:24 AM
Printed by: wet


Ident: LB121643BSW2
Analysis from: 8/22/2022 12:30:58 PM
File: _2022-08-22_

Last save: 8/23/2022 9:13:12 AM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31510

Last save: 8/19/2022 9:42:

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

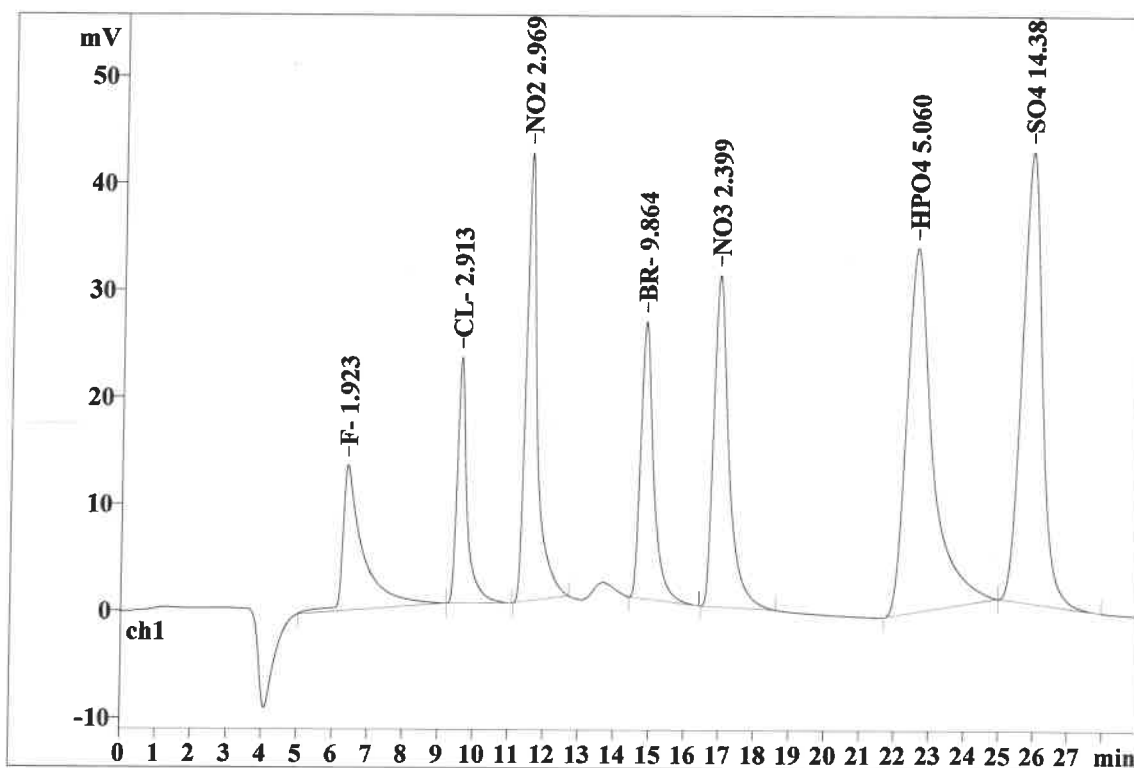

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.38	0.462	13.61	6.43	545.842	7.80
2	9.59	0.253	23.01	10.87	442.864	6.33
3	11.52	0.300	41.91	19.80	939.016	13.41
4	14.82	0.362	25.91	12.24	657.120	9.39
5	16.91	0.430	31.01	14.65	936.452	13.38
6	22.54	0.707	34.08	16.10	1770.670	25.29
7	25.82	0.607	42.17	19.92	1708.495	24.41
7	29.00	0.446	211.70	100.00	7000.459	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:18:36 AM
 Printed by: wet


Ident: N4277-02
 Analysis from: 8/22/2022 1:02:55 PM
 File: _2022-08-22_

Last save: 8/22/2022 1:31:55 PM

Method: AnionsIC2-081622.mtw
 Run operator: wet
 Analysis number: 31511

Last save: 8/22/2022 10:53

SAMPLE:
 : IZ/MA
 Vial number: 18
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

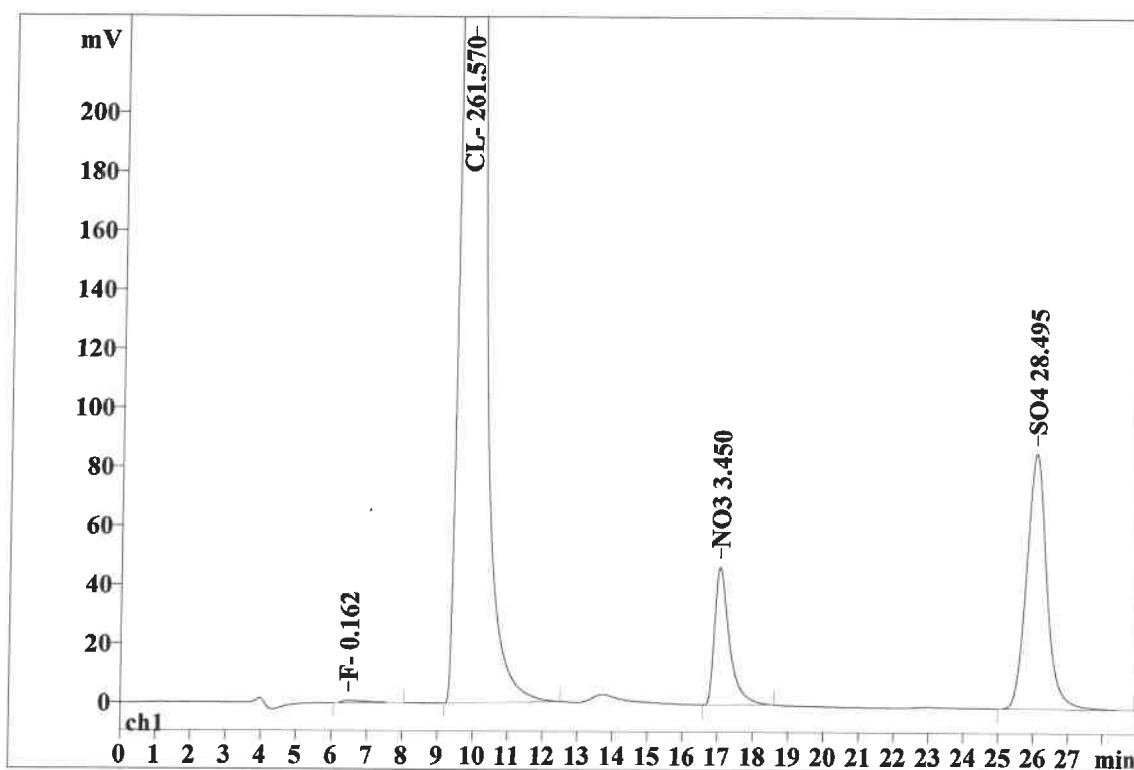

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.48	0.756	0.78	0.05	38.509	0.08
2	9.80	0.398	1490.65	91.76	41429.847	89.44
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.04	0.420	46.70	2.87	1368.429	2.95
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.01	0.596	86.42	5.32	3482.434	7.52
7	29.00	0.310	1624.56	100.00	46319.218	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 8/23/2022 9:18:46 AM
Printed by: wet


Ident: N4277-03
Analysis from: 8/22/2022 1:34:32 PM
File: _2022-08-22_

Last save: 8/22/2022 2:03:33 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31512

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

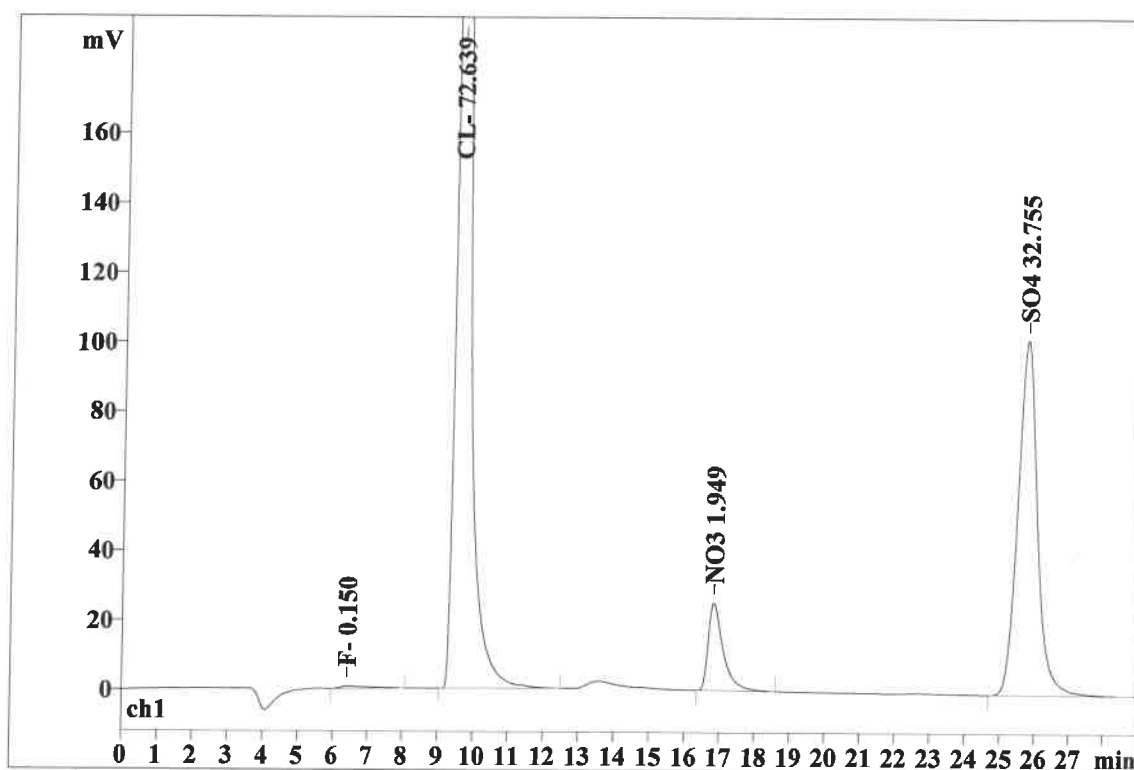

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.40	0.775	0.67	0.09	34.887	0.21
2	9.55	0.237	636.04	83.25	11491.715	70.52
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.82	0.424	25.23	3.30	751.719	4.61
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.70	0.579	102.04	13.36	4017.927	24.66
7	29.00	0.288	763.98	100.00	16296.246	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:19:03 AM
Printed by: wet


Ident: N4264-02DLX2
Analysis from: 8/22/2022 2:06:10 PM
File: _2022-08-22_

Last save: 8/22/2022 2:35:10 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31513

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

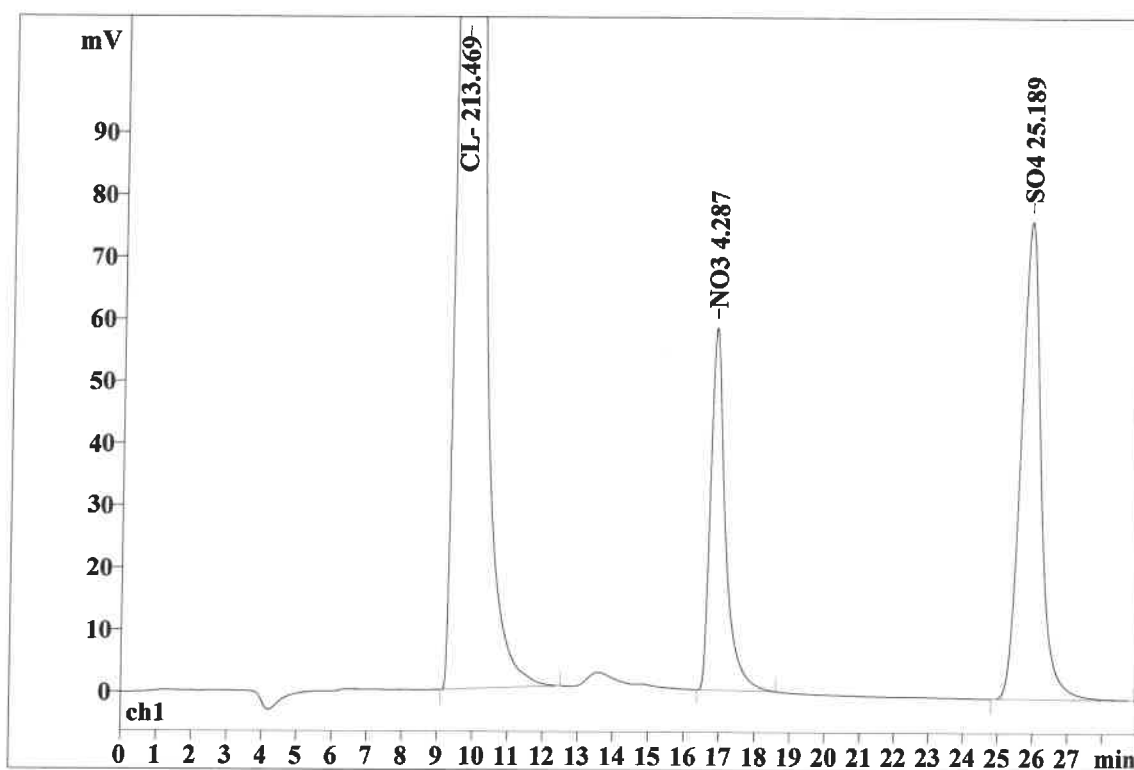

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.67	0.333	1414.07	91.28	33807.640	87.61
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.82	0.415	58.32	3.76	1712.278	4.44
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.82	0.587	76.79	4.96	3066.834	7.95
7	29.00	0.191	1549.18	100.00	38586.751	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:19:11 AM
Printed by: wet


Ident: N4262-01DLX100
Analysis from: 8/22/2022 2:37:48 PM
File: _2022-08-22_

Last save: 8/22/2022 3:06:48 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31514

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

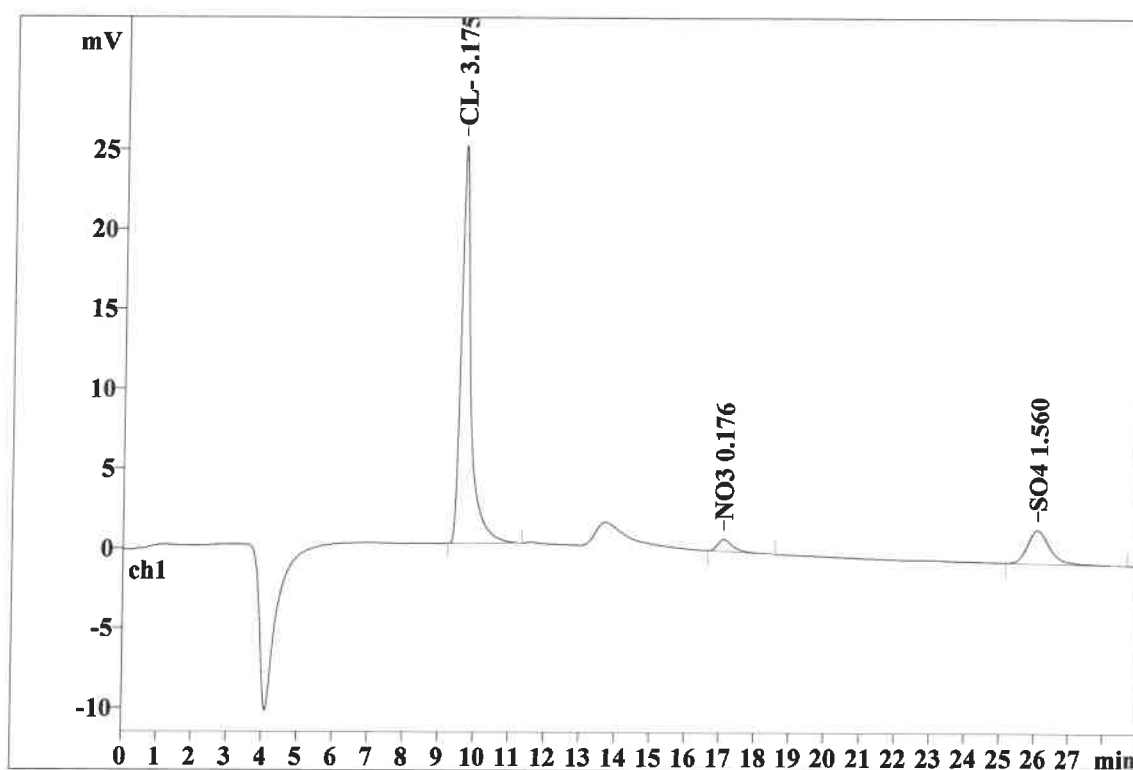

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.63	0.253	24.97	89.74	484.506	80.19
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.09	0.445	0.75	2.70	23.450	3.88
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.04	0.665	2.10	7.54	96.247	15.93
7	29.00	0.195	27.82	99.98	604.203	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:19:23 AM
Printed by: wet


Ident: N4262-02DLX2
Analysis from: 8/22/2022 3:09:26 PM
File: _2022-08-22_

Last save: 8/22/2022 3:38:26 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31515

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

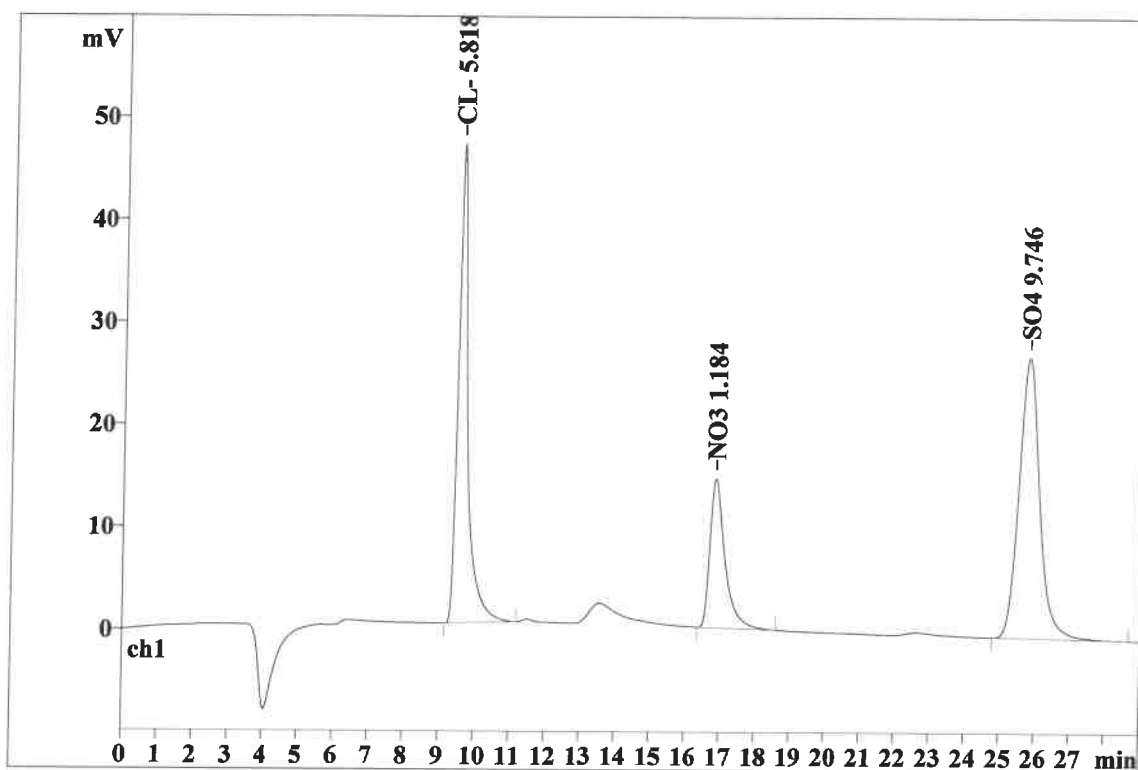

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.56	0.250	46.76	52.73	903.246	36.63
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.85	0.429	14.56	16.42	437.522	17.74
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.77	0.608	27.36	30.85	1125.346	45.63
7	29.00	0.184	88.67	100.00	2466.115	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:19:33 AM
Printed by: wet


Ident: N4262-03DLX50
Analysis from: 8/22/2022 3:41:03 PM
File: _2022-08-22_

Last save: 8/22/2022 4:10:03 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31516

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

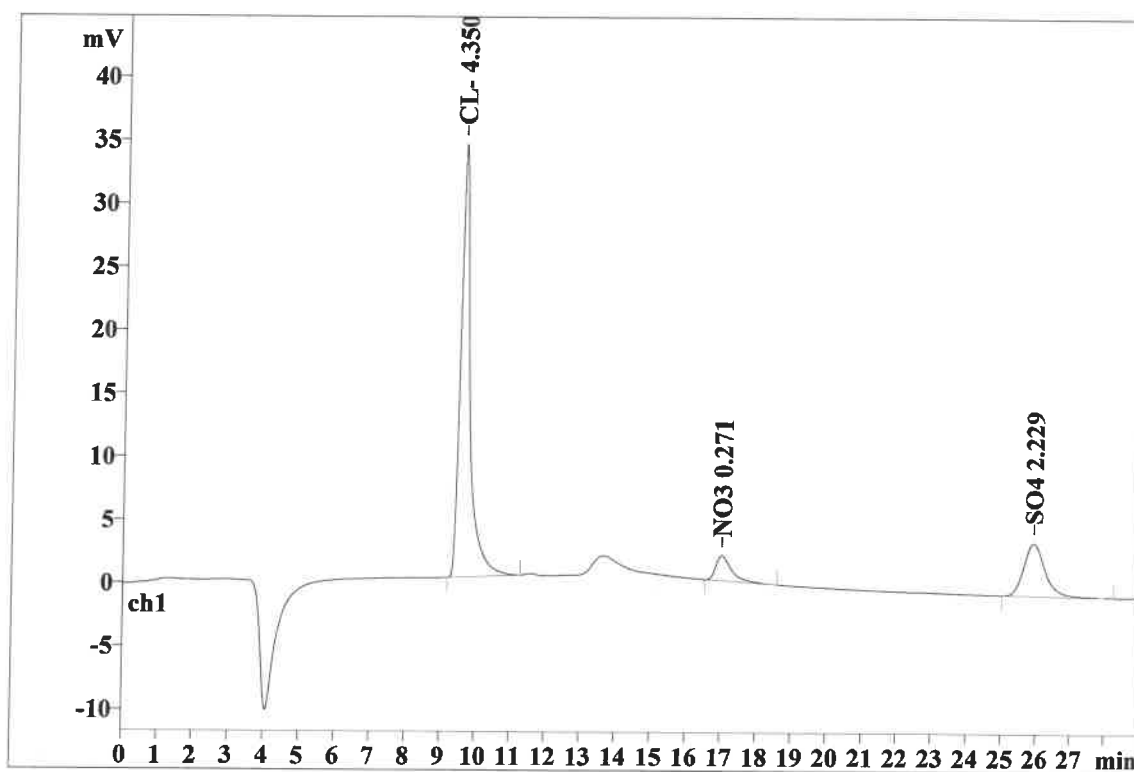

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.58	0.255	34.23	84.77	670.569	73.43
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.01	0.445	1.97	4.89	62.306	6.82
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.89	0.640	4.17	10.33	180.382	19.75
7	29.00	0.191	40.38	99.99	913.257	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:19:42 AM
Printed by: wet


Ident: N4262-04DLX50
Analysis from: 8/22/2022 4:12:46 PM
File: _2022-08-22_

Last save: 8/22/2022 4:41:46 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31517

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 24
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

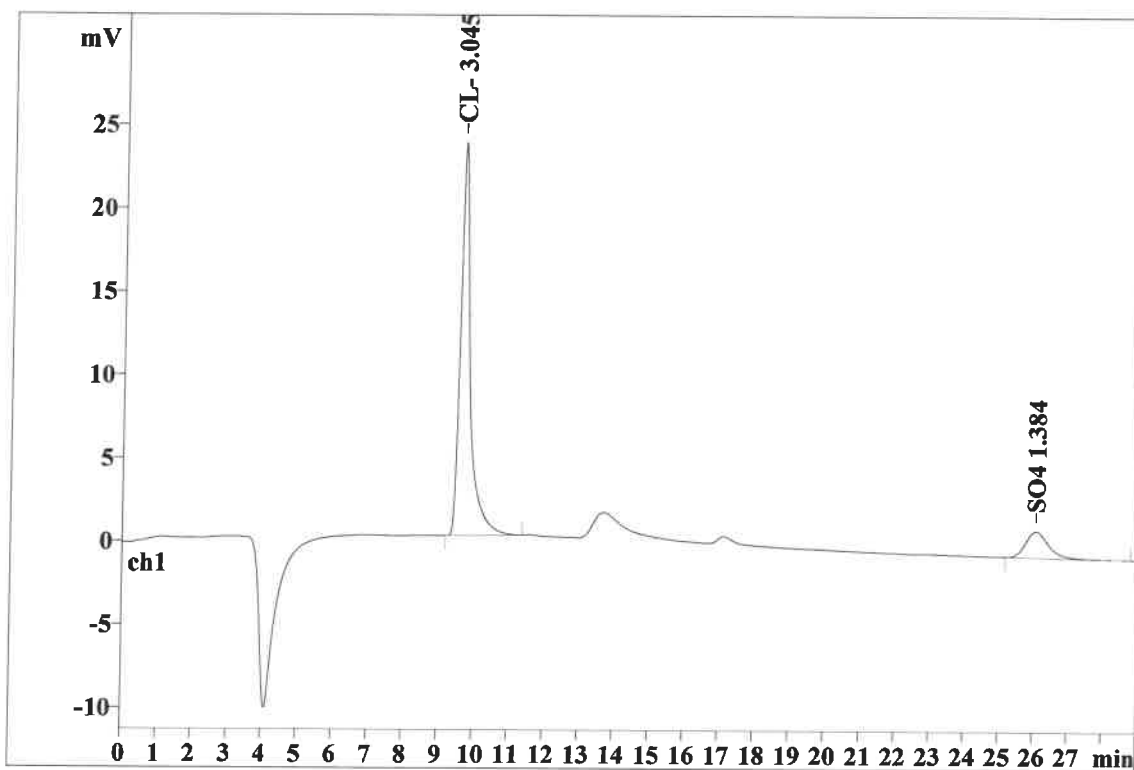

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.65	0.256	23.61	93.69	463.841	86.21
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.04	0.687	1.59	6.30	74.184	13.79
7	29.00	0.135	25.19	99.99	538.025	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:19:52 AM
Printed by: wet


Ident: N4262-05DLX100
Analysis from: 8/22/2022 4:44:23 PM
File: _2022-08-22_

Last save: 8/22/2022 5:13:24 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31518

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

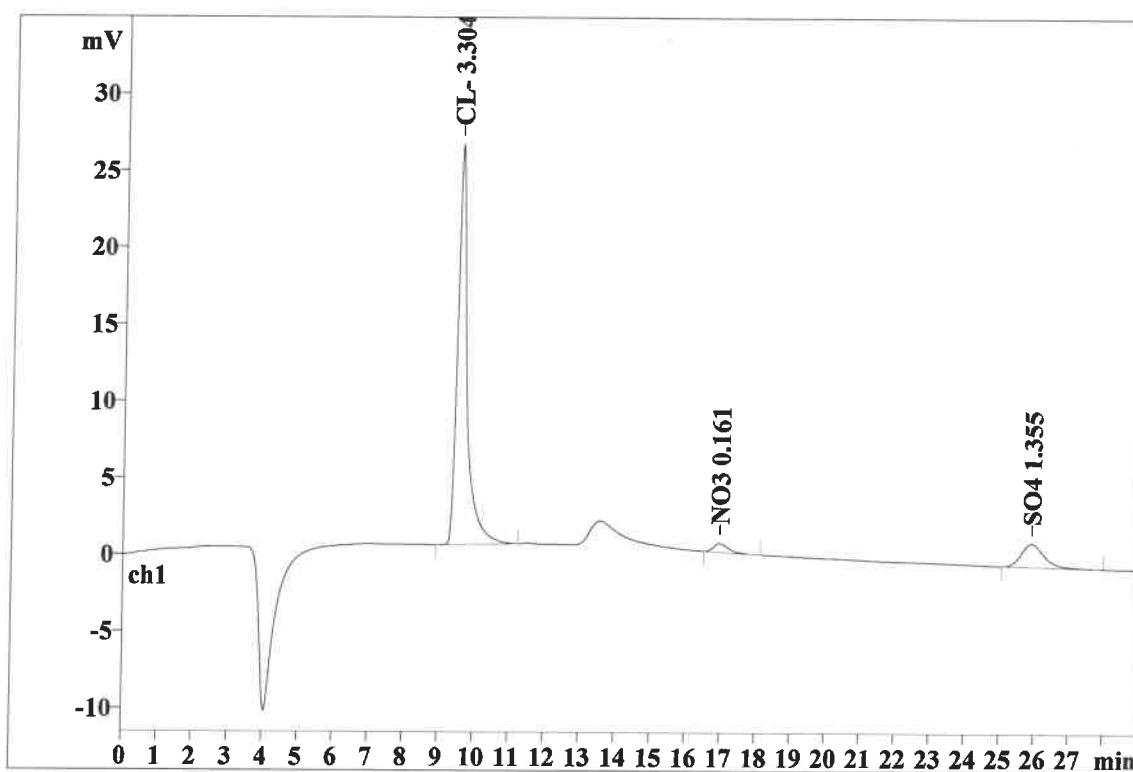

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.54	0.252	26.03	92.50	504.905	85.18
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.96	0.440	0.58	2.07	17.358	2.93
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.88	0.684	1.52	5.41	70.471	11.89
7	29.00	0.197	28.13	99.98	592.734	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:20:04 AM
Printed by: wet


Ident: CCV
Analysis from: 8/22/2022 5:16:07 PM
File: _2022-08-22_

Last save: 8/22/2022 5:45:07 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31519

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

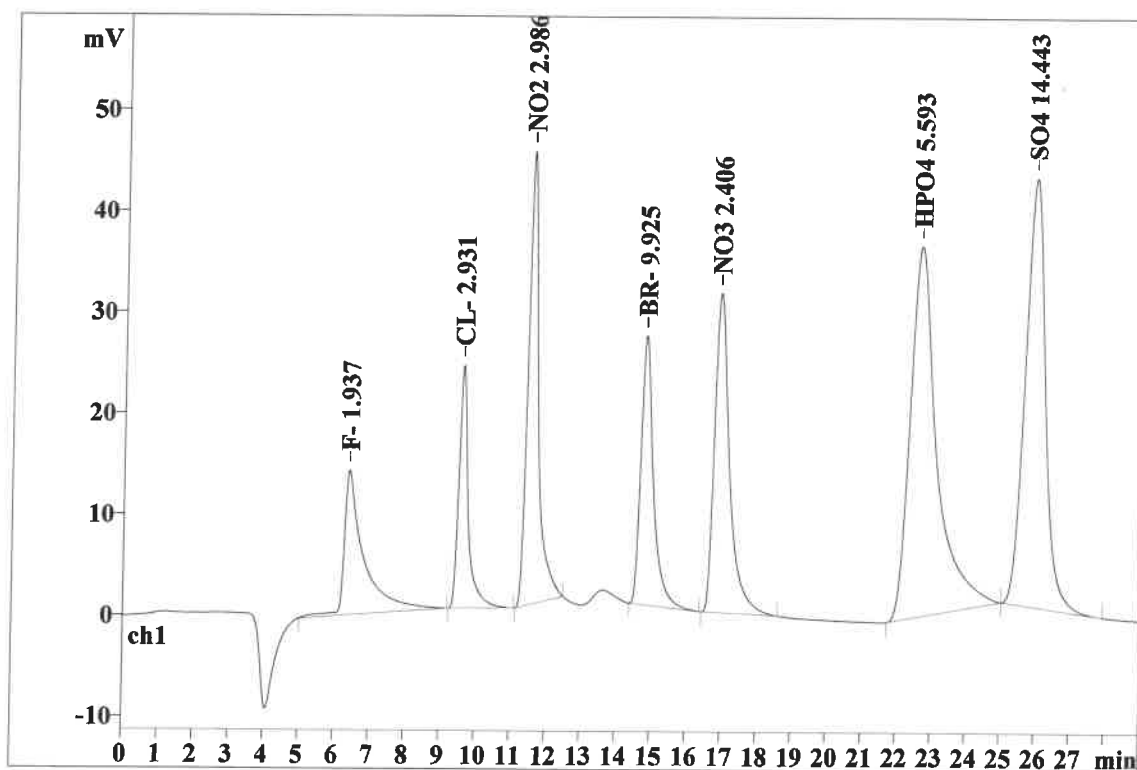

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.39	0.433	14.32	6.50	549.927	7.62
2	9.59	0.246	24.06	10.91	445.812	6.18
3	11.52	0.292	44.82	20.33	944.643	13.09
4	14.79	0.352	26.64	12.08	661.450	9.17
5	16.88	0.421	31.60	14.34	939.524	13.02
6	22.59	0.727	36.66	16.63	1959.297	27.15
7	25.88	0.608	42.33	19.20	1715.902	23.78
7	29.00	0.440	220.42	100.00	7216.555	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:20:13 AM
Printed by: wet


Ident: CCB
Analysis from: 8/22/2022 5:47:45 PM
File: _2022-08-22_

Last save: 8/22/2022 6:16:45 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31520

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

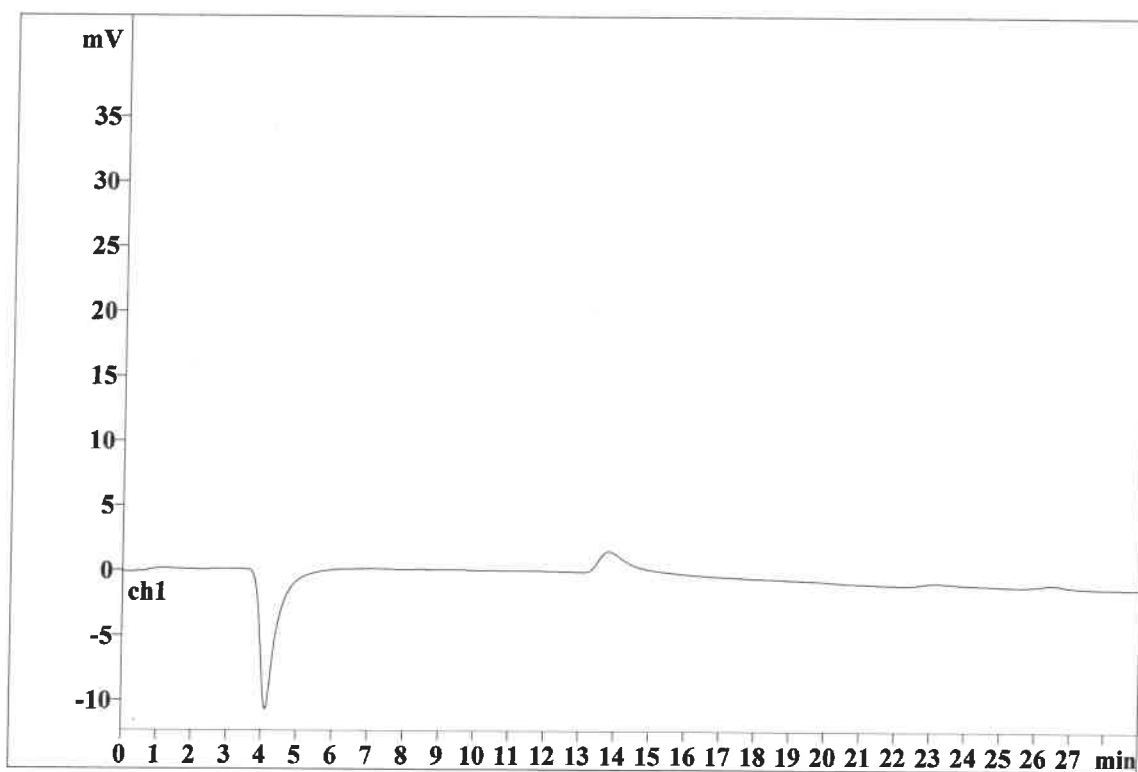

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:20:24 AM
Printed by: wet


Ident: N4262-06DLX100
Analysis from: 8/22/2022 6:19:28 PM
File: _2022-08-22_

Last save: 8/22/2022 6:48:28 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31521

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

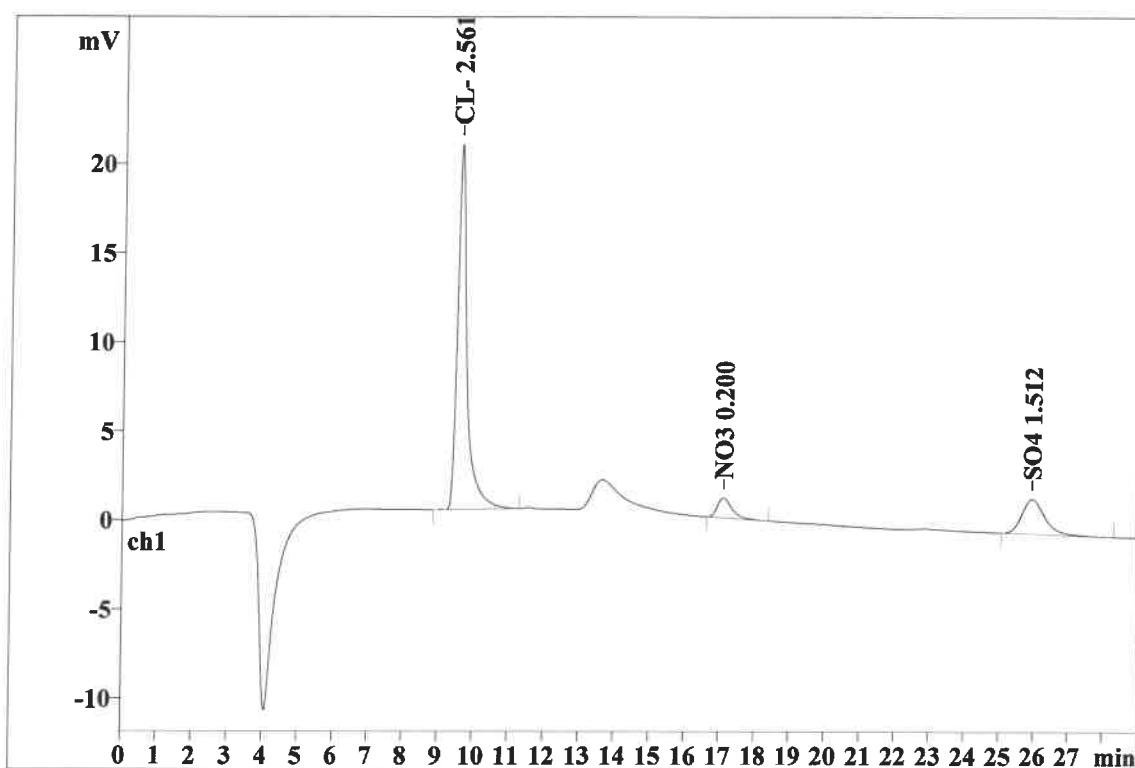

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.59	0.250	20.50	86.94	387.178	75.84
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.09	0.436	1.12	4.73	33.105	6.48
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.92	0.679	1.96	8.32	90.247	17.68
7	29.00	0.195	23.58	99.99	510.529	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:20:35 AM
Printed by: wet


Ident: N4262-07DLX100
Analysis from: 8/22/2022 6:51:05 PM
File: _2022-08-22_

Last save: 8/22/2022 7:20:06 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31522

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

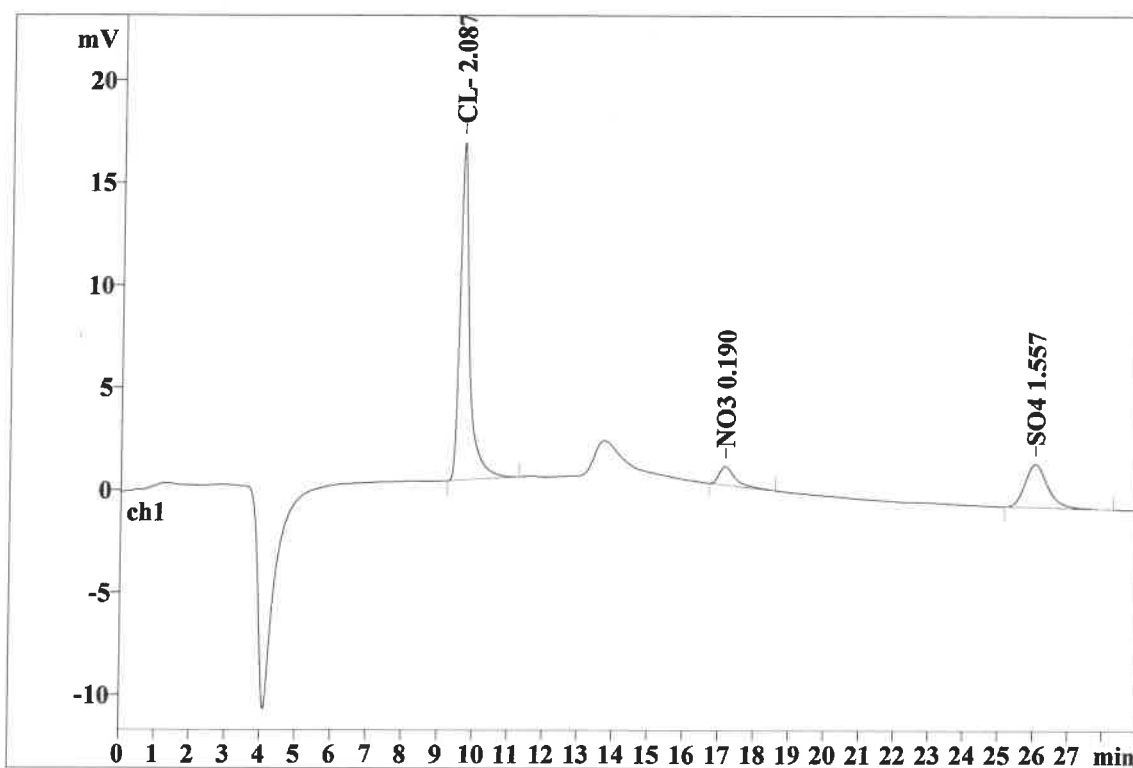

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.64	0.253	16.46	84.45	311.987	71.39
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.14	0.446	0.91	4.69	29.064	6.65
6	0.00	0.000	0.00	0.00	0.000	0.00
7	26.00	0.674	2.12	10.86	95.956	21.96
7	29.00	0.196	19.49	99.99	437.007	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:21:45 AM
Printed by: wet


Ident: CCV
Analysis from: 8/22/2022 7:54:27 PM
File: _2022-08-22_

Last save: 8/22/2022 8:23:27 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31524

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

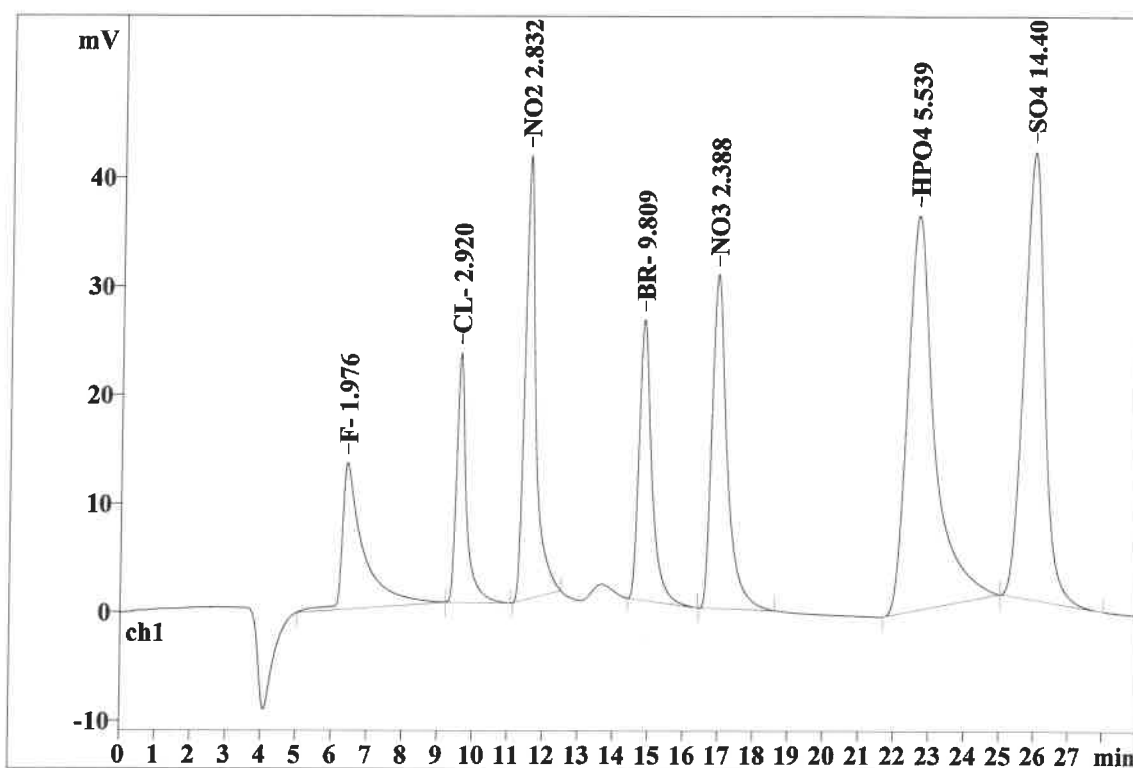

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.41	0.485	13.48	6.37	561.189	7.87
2	9.59	0.255	22.98	10.87	444.041	6.23
3	11.52	0.299	40.83	19.31	891.686	12.50
4	14.81	0.362	25.83	12.22	653.219	9.16
5	16.90	0.432	30.76	14.55	931.971	13.07
6	22.59	0.727	36.36	17.20	1940.407	27.20
7	25.88	0.623	41.18	19.48	1710.589	23.98
7	29.00	0.455	211.42	100.00	7133.102	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/23/2022 9:21:38 AM
Printed by: wet


Ident: CCB
Analysis from: 8/22/2022 8:26:04 PM
File: _2022-08-22_

Last save: 8/22/2022 8:55:04 PM

Method: AnionsIC2-081622.mtw
Run operator: wet
Analysis number: 31525

Last save: 8/22/2022 10:53

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

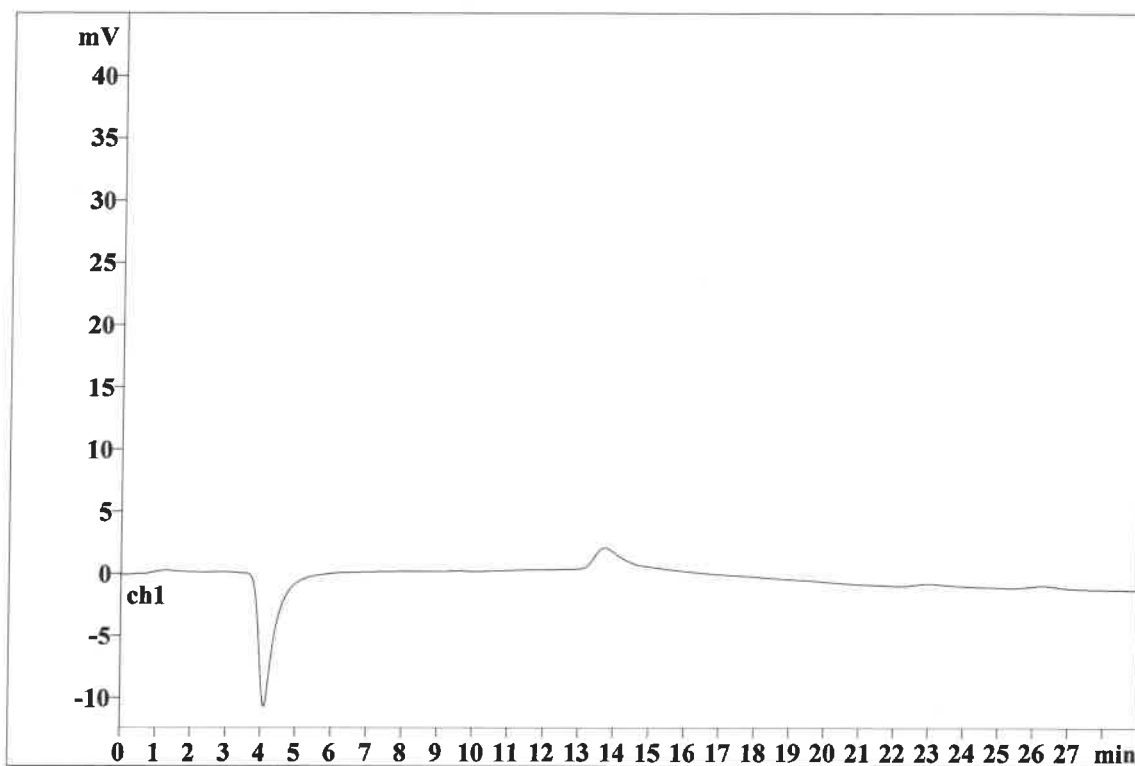

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD