


LB121646

7471B

INSTRUMENT ID: CV1

Linear

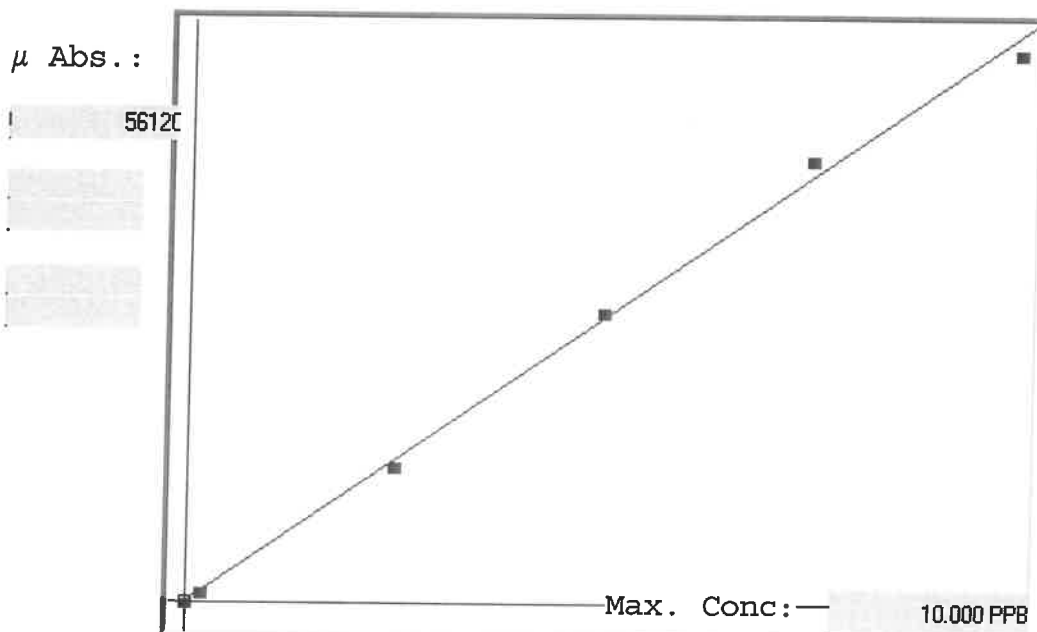

A= 0.0000e+000

B= 1.7298e-004

C= -9.2311e-003

Rho= 0.9986261

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.029	-0.029	-115	0.000	-115					7
0.2	0.200	0.186	-0.014	1131	0.0 %	1131					-7
2.5	2.500	2.388	-0.112	13860	0.0 %	13860					-4
5.0	5.000	5.139	0.139	29760	0.0 %	29760					3
7.5	7.500	7.817	0.317	45245	0.0 %	45245					4
10.0	10.000	9.698	-0.302	56120	0.0 %	56120					-3

LB121646 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Aug 2022 10:32:08

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-115	-	0.0000	7471B	PPB	23 Aug 2022 10:40:35	S	Std
0.2 - 1	512	1131	-	0.2000	7471B	PPB	23 Aug 2022 10:42:53	S	Std
2.5 - 1	525	13860	-	2.5000	7471B	PPB	23 Aug 2022 10:45:10	S	Std
5.0 - 1	55	29760	-	5.0000	7471B	PPB	23 Aug 2022 10:47:27	S	Std
7.5 - 1	575	45245	-	7.5000	7471B	PPB	23 Aug 2022 10:52:32	S	Std
10.0 - 1	50	56120	-	10.0000	7471B	PPB	23 Aug 2022 10:54:48	S	Std
ICV99 - 1	ICV99	22686	3.9150	-	7471B	PPB	23 Aug 2022 10:57:43	U	SMPL
ICB99 - 1	ICB99	-219	-0.0471	-	7471B	PPB	23 Aug 2022 10:59:58	U	SMPL
CCV88 - 1	CCV88	29946	5.1709	-	7471B	PPB	23 Aug 2022 11:02:14	U	SMPL
CCB88 - 1	CCB88	-238	-0.0504	-	7471B	PPB	23 Aug 2022 11:04:29	U	SMPL
CRA - 1	CRA	1208	0.1997	-	7471B	PPB	23 Aug 2022 11:06:47	U	SMPL
HighStd - 1	HighStd	58764	10.1558	-	7471B	PPB	23 Aug 2022 11:09:01	U	SMPL
ChkStd - 1	ChkStd	43871	7.5450	-	7471B	PPB	23 Aug 2022 11:16:38	U	SMPL
PB147205BL - 1	PBS	-118	-0.0296	-	7471B	PPB	23 Aug 2022 11:21:43	U	SMPL
PB147205BS - 1	LCSS	21494	3.7088	-	7471B	PPB	23 Aug 2022 11:26:29	U	SMPL
N3980-01 - 1	LOD-MDL-SOIL-01-QT3-2022	392	0.0586	-	7471B	PPB	23 Aug 2022 11:31:22	U	SMPL
N3980-01RE - 1	LOD-MDL-SOIL-01-QT3-2022	895	0.1456	-	7471B	PPB	23 Aug 2022 11:33:38	U	SMPL
N3980-03 - 1	MDL-SOIL-03-QT3-2022	348	0.0510	-	7471B	PPB	23 Aug 2022 11:38:32	U	SMPL
N4260-01 - 1	SASP2-T-4(0-5)	15325	2.6417	-	7471B	PPB	23 Aug 2022 11:45:40	U	SMPL
N4260-01DUP - 1	SASP2-T-4(0-5)DUP	15603	2.6898	-	7471B	PPB	23 Aug 2022 11:47:55	U	SMPL
CCV89 - 1	CCV89	29509	5.0953	-	7471B	PPB	23 Aug 2022 11:59:50	U	SMPL
CCB89 - 1	CCB89	-185	-0.0412	-	7471B	PPB	23 Aug 2022 12:02:05	U	SMPL
N4260-01MS - 1	SASP2-T-4(0-5)MS	38904	6.7204	-	7471B	PPB	23 Aug 2022 12:04:21	U	SMPL
N4260-01MSD - 1	SASP2-T-4(0-5)MSD	37796	6.5288	-	7471B	PPB	23 Aug 2022 12:06:36	U	SMPL
N4260-02 - 1	SASP2-T-4(5-10)	292	0.0413	-	7471B	PPB	23 Aug 2022 12:08:54	U	SMPL
N4260-03 - 1	SASP2-T-4(10-16)	949	0.1549	-	7471B	PPB	23 Aug 2022 12:11:12	U	SMPL
N4260-04 - 1	SASP2-T-4(16-22)	299	0.0425	-	7471B	PPB	23 Aug 2022 12:13:27	U	SMPL
N4270-01 - 1	SASP2-T-4(25-37)	8	-0.0078	-	7471B	PPB	23 Aug 2022 12:15:44	U	SMPL
N4272-01 - 1	PSC-124042	1329	0.2207	-	7471B	PPB	23 Aug 2022 12:18:01	U	SMPL
N4272-03 - 1	PSC-124055	1951	0.3283	-	7471B	PPB	23 Aug 2022 12:20:18	U	SMPL
N4272-05 - 1	PSC-124035	4033	0.6884	-	7471B	PPB	23 Aug 2022 12:22:35	U	SMPL
N4272-07 - 1	PSC-164717	3578	0.6097	-	7471B	PPB	23 Aug 2022 12:24:51	U	SMPL
CCV90 - 1	CCV90	28557	4.9306	-	7471B	PPB	23 Aug 2022 12:27:06	U	SMPL
CCB90 - 1	CCB90	-106	-0.0276	-	7471B	PPB	23 Aug 2022 12:29:22	U	SMPL
N4273-01 - 1	EO-1-081922	3629	0.6185	-	7471B	PPB	23 Aug 2022 12:31:39	U	SMPL
N4274-01 - 1	CL-1	1550	0.2589	-	7471B	PPB	23 Aug 2022 12:33:55	U	SMPL
N4275-01 - 1	OR-03-081922	2042	0.3440	-	7471B	PPB	23 Aug 2022 12:36:10	U	SMPL
N4277-01 - 1	B-2	5460	0.9352	-	7471B	PPB	23 Aug 2022 12:38:26	U	SMPL
N4283-01 - 1	337	689	0.1100	-	7471B	PPB	23 Aug 2022 12:40:42	U	SMPL
N4292-01 - 1	TR-04-082222	5784	0.9913	-	7471B	PPB	23 Aug 2022 12:42:58	U	SMPL
N4293-01 - 1	CON1-8-22-2022	890	0.1447	-	7471B	PPB	23 Aug 2022 12:45:15	U	SMPL
N4295-01 - 1	XRDS-RECYCLED-SAND-SP-A-COMP	9275	1.5952	-	7471B	PPB	23 Aug 2022 12:47:32	U	SMPL
N4260-01LX5 - 1		2913	0.4947	-	7471B	PPB	23 Aug 2022 12:49:50	U	SMPL
N4260-01A - 1		36094	6.2343	-	7471B	PPB	23 Aug 2022 12:54:43	U	SMPL
CCV91 - 1	CCV91	28522	4.9245	-	7471B	PPB	23 Aug 2022 12:59:35	U	SMPL
CCB91 - 1	CCB91	35	-0.0032	-	7471B	PPB	23 Aug 2022 13:04:23	U	SMPL