

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : R Instrument ID : Konelab

8/23/2022 14:39

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	0.977	0.0	0.107	
ICB1	0.001	0.0	0.008	
CCV1	0.978	0.0	0.107	
CCB1	0.007	0.0	0.009	
PB147214BL	0.005	0.0	0.009	
PB147214BS	0.979	0.0	0.107	
N4277-02	0.006	0.0	0.009	
N4277-02DUP	0.003	0.0	0.009	
N4277-02MS	1.078	0.0	0.117	
N4277-02MSD	1.071	0.0	0.117	
N4277-03	0.001	0.0	0.008	
N4291-01	-0.021	0.0	0.006	
CCV2	0.975	0.0	0.107	
CCB2	0.003	0.0	0.009	

N	14
Mean	0.433
SD	0.5192
CV%	119.88

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 23 13:28:52 2022

Tue Aug 23 14:34:34 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0038	mg/l	8/23/2022 13:28:52	
0.05PPM	A	Phenolics-	P	0.0529	mg/l	8/23/2022 13:28:53	
0.1PPM	A	Phenolics-	P	0.1094	mg/l	8/23/2022 13:28:54	
0.25PPM	A	Phenolics-	P	0.2557	mg/l	8/23/2022 13:28:55	
0.50PPM	A	Phenolics-	P	0.5019	mg/l	8/23/2022 13:28:56	
1.0PPM	A	Phenolics-	P	0.9563	mg/l	8/23/2022 13:28:57	
2.0PPM	A	Phenolics-	P	2.0201	mg/l	8/23/2022 13:28:58	
ICV1	S	Phenolics-	P	0.9768	mg/l	8/23/2022 14:27:42	
ICB1	S	Phenolics-	P	0.0008	mg/l	8/23/2022 14:27:44	
CCV1	S	Phenolics-	P	0.9777	mg/l	8/23/2022 14:27:46	
CCB1	S	Phenolics-	P	0.0065	mg/l	8/23/2022 14:27:48	
PB147214BL	S	Phenolics-	P	0.0053	mg/l	8/23/2022 14:27:50	
PB147214BS	S	Phenolics-	P	0.9786	mg/l	8/23/2022 14:27:52	
N4277-02	S	Phenolics-	P	0.0055	mg/l	8/23/2022 14:34:27	
N4277-02DUP	S	Phenolics-	P	0.0035	mg/l	8/23/2022 14:34:28	
N4277-02MS	S	Phenolics-	P	1.0784	mg/l	8/23/2022 14:34:29	
N4277-02MSD	S	Phenolics-	P	1.0713	mg/l	8/23/2022 14:34:30	
N4277-03	S	Phenolics-	P	0.001	mg/l	8/23/2022 14:34:31	
N4291-01	S	Phenolics-	P	-0.0206	mg/l	8/23/2022 14:34:32	
CCV2	S	Phenolics-	P	0.9749	mg/l	8/23/2022 14:34:33	
CCB2	S	Phenolics-	P	0.003	mg/l	8/23/2022 14:34:34	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/23/2022 13:30


Test Phenolics-

Accepted 8/23/2022 13:30

Factor 9.902
Bias 0.008

Coeff. of det. 0.999219

Errors

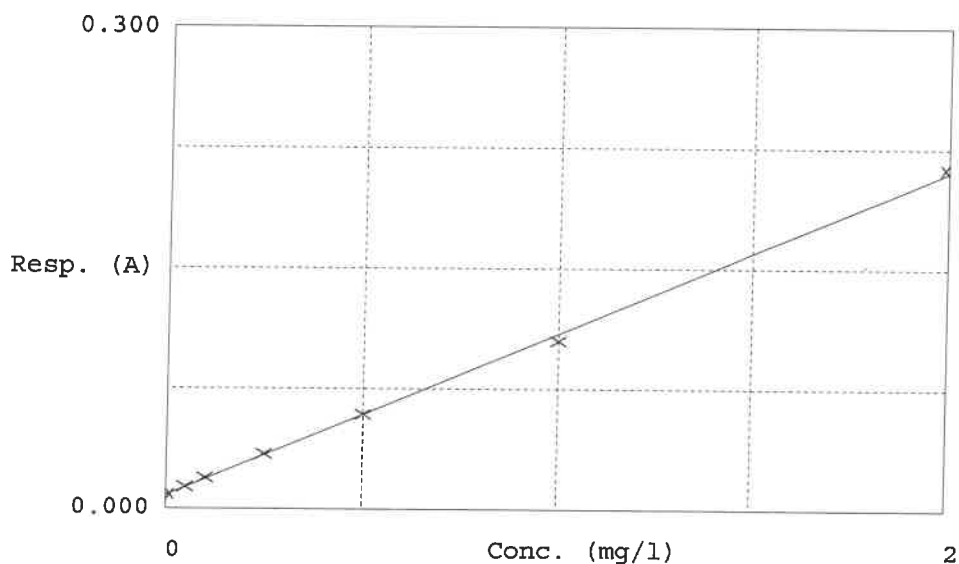

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.009	0.0038	0.0000	-
2	Phenol-2	0.014	0.0529	0.0500	5.8
3	Phenol-2	0.019	0.1094	0.1000	9.4
4	Phenol-2	0.034	0.2557	0.2500	2.3
5	Phenol-2	0.059	0.5019	0.5000	0.4
6	Phenol-2	0.105	0.9563	1.0000	-4.4
7	Phenol-2	0.212	2.0201	2.0000	1.0

12

8/23/22