

LB121657


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

46310

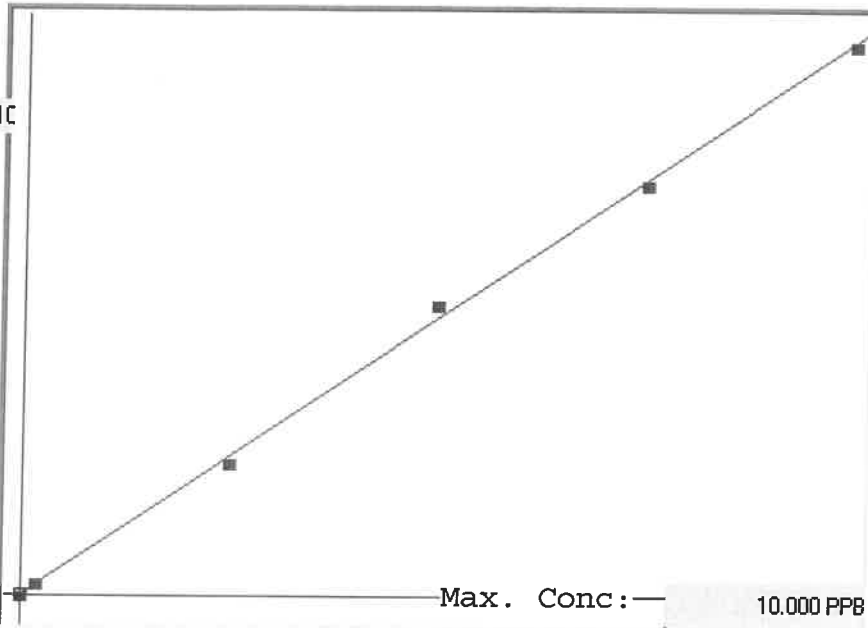

A= 0.0000e+000

B= 2.1509e-004

C= -1.0089e-002

Rho= 0.9994989

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.029	-0.029	-90	0.000	-90					
0.2	0.200	0.230	0.030	1114	0.0 %	1114					
2.5	2.500	2.373	-0.127	11079	0.0 %	11079					
5.0	5.000	5.240	0.240	24408	0.0 %	24408					
7.5	7.500	7.437	-0.063	34621	0.0 %	34621					
10.0	10.000	9.951	-0.049	46310	0.0 %	46310					

15510

LB121657 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 23 Aug 2022 15:01:29

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-90	-	0.0000	7470A	PPB	23 Aug 2022 15:31:15	S	Std
0.2 - 1	50.2	1114	-	0.2000	7470A	PPB	23 Aug 2022 15:33:31	S	Std
2.5 - 1	52.5	11079	-	2.5000	7470A	PPB	23 Aug 2022 15:40:42	S	Std
5.0 - 1	55	24408	-	5.0000	7470A	PPB	23 Aug 2022 15:42:59	S	Std
7.5 - 1	57.5	34621	-	7.5000	7470A	PPB	23 Aug 2022 15:45:15	S	Std
10.0 - 1	57.6	46310	-	10.0000	7470A	PPB	23 Aug 2022 15:52:42	S	Std
ICV01 - 1	ICV01	18578	3.9858	-7470A	PPB	23 Aug 2022 15:55:22	U	SMPL	
ICB01 - 1	ICB01	-186	-0.0501	-7470A	PPB	23 Aug 2022 15:57:37	U	SMPL	
CCV92 - 1	CCV92	24165	5.1875	-7470A	PPB	23 Aug 2022 15:59:52	U	SMPL	
CCB92 - 1	CCB92	-193	-0.0516	-7470A	PPB	23 Aug 2022 16:02:07	U	SMPL	
CRA - 1	CRA	1072	0.2205	-7470A	PPB	23 Aug 2022 16:04:23	U	SMPL	
HighStd - 1	HighStd	46426	9.9757	-7470A	PPB	23 Aug 2022 16:06:37	U	SMPL	
ChkStd - 1	ChkStd	32038	6.8809	-7470A	PPB	23 Aug 2022 16:08:53	U	SMPL	
PB147212BL - 1	PBW	-209	-0.0550	-7470A	PPB	23 Aug 2022 16:11:10	U	SMPL	
PB147212BS - 1	LCSW	19568	4.1988	-7470A	PPB	23 Aug 2022 16:13:27	U	SMPL	
N3980-07 - 1	LOD-MDL-WATER-01-QT3-2022	340	0.0630	-7470A	PPB	23 Aug 2022 16:20:48	U	SMPL	
N3980-07RE - 1	LOD-MDL-WATER-01-QT3-2022	598	0.1185	-7470A	PPB	23 Aug 2022 16:25:37	U	SMPL	
N3980-09 - 1	MDL-WATER-03-QT3-2022	314	0.0574	-7470A	PPB	23 Aug 2022 16:27:54	U	SMPL	
N4262-01 - 1	MW-102D	116	0.0149	-7470A	PPB	23 Aug 2022 16:30:11	U	SMPL	
N4262-02 - 1	MW-102S	-20	-0.0144	-7470A	PPB	23 Aug 2022 16:32:26	U	SMPL	
CCV93 - 1	CCV93	24003	5.1527	-7470A	PPB	23 Aug 2022 16:34:41	U	SMPL	
CCB93 - 1	CCB93	-183	-0.0495	-7470A	PPB	23 Aug 2022 16:36:56	U	SMPL	
N4262-03 - 1	MW-102I	-63	-0.0236	-7470A	PPB	23 Aug 2022 16:39:12	U	SMPL	
N4262-04 - 1	MW-101S	288	0.0519	-7470A	PPB	23 Aug 2022 16:41:28	U	SMPL	
N4262-05 - 1	MW-101I	23	-0.0051	-7470A	PPB	23 Aug 2022 16:43:43	U	SMPL	
N4262-06 - 1	MW-101D	-23	-0.0150	-7470A	PPB	23 Aug 2022 16:45:59	U	SMPL	
N4262-07 - 1	MW-107(42.5FT)	-26	-0.0157	-7470A	PPB	23 Aug 2022 16:48:15	U	SMPL	
N4262-07DUP - 1	MW-107(42.5FT)DUP	-8	-0.0118	-7470A	PPB	23 Aug 2022 16:50:31	U	SMPL	
N4262-07MS - 1	MW-107(42.5FT)MS	15707	3.3683	-7470A	PPB	23 Aug 2022 16:52:48	U	SMPL	
N4262-07MSD - 1	MW-107(42.5FT)MSD	15486	3.3208	-7470A	PPB	23 Aug 2022 16:55:06	U	SMPL	
N4262-07LX5 - 1		-167	-0.0460	-7470A	PPB	23 Aug 2022 16:57:23	U	SMPL	
N4262-07A - 1		18919	4.0592	-7470A	PPB	23 Aug 2022 16:59:38	U	SMPL	
CCV94 - 1	CCV94	23400	5.0230	-7470A	PPB	23 Aug 2022 17:01:54	U	SMPL	
CCB94 - 1	CCB94	-180	-0.0488	-7470A	PPB	23 Aug 2022 17:04:09	U	SMPL	