

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/23/2022 15:44

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.978	0.0	0.107	
ICB1	0.004	0.0	0.009	
CCV1	0.978	0.0	0.107	
CCB1	0.003	0.0	0.009	
PB147216BL	0.003	0.0	0.009	
PB147216BS	0.982	0.0	0.107	
PB147217BL	0.004	0.0	0.009	
PB147217BS	0.978	0.0	0.107	
N3980-03	0.030	0.0	0.011	
N3980-09	0.028	0.0	0.011	
CCV2	0.980	0.0	0.107	
CCB2	0.003	0.0	0.009	

N	12
Mean	0.414
SD	0.4988
CV%	120.41

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 23 15:01:31 2022

Tue Aug 23 15:32:24 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0038	mg/l	8/23/2022 13:28:52	
0.05PPM	A	Phenolics-	P	0.0529	mg/l	8/23/2022 13:28:53	
0.1PPM	A	Phenolics-	P	0.1094	mg/l	8/23/2022 13:28:54	
0.25PPM	A	Phenolics-	P	0.2557	mg/l	8/23/2022 13:28:55	
0.50PPM	A	Phenolics-	P	0.5019	mg/l	8/23/2022 13:28:56	
1.0PPM	A	Phenolics-	P	0.9563	mg/l	8/23/2022 13:28:57	
2.0PPM	A	Phenolics-	P	2.0201	mg/l	8/23/2022 13:28:58	
ICV1	S	Phenolics-	P	0.9778	mg/l	8/23/2022 15:01:32	
ICB1	S	Phenolics-	P	0.0036	mg/l	8/23/2022 15:01:34	
CCV1	S	Phenolics-	P	0.978	mg/l	8/23/2022 15:01:36	
CCB1	S	Phenolics-	P	0.0029	mg/l	8/23/2022 15:01:38	
PB147216BL	S	Phenolics-	P	0.0032	mg/l	8/23/2022 15:01:40	
PB147216BS	S	Phenolics-	P	0.9818	mg/l	8/23/2022 15:01:42	
PB147217BL	S	Phenolics-	P	0.0039	mg/l	8/23/2022 15:11:36	
PB147217BS	S	Phenolics-	P	0.9785	mg/l	8/23/2022 15:11:37	
N3980-03	S	Phenolics-	P	0.0303	mg/l	8/23/2022 15:32:20	
N3980-09	S	Phenolics-	P	0.0279	mg/l	8/23/2022 15:32:22	
CCV2	S	Phenolics-	P	0.9796	mg/l	8/23/2022 15:32:23	
CCB2	S	Phenolics-	P	0.003	mg/l	8/23/2022 15:32:24	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

8/23/2022 13:30


Test Phenolics-

Accepted 8/23/2022 13:30

Factor 9.902
Bias 0.008

Coeff. of det. 0.999219

Errors

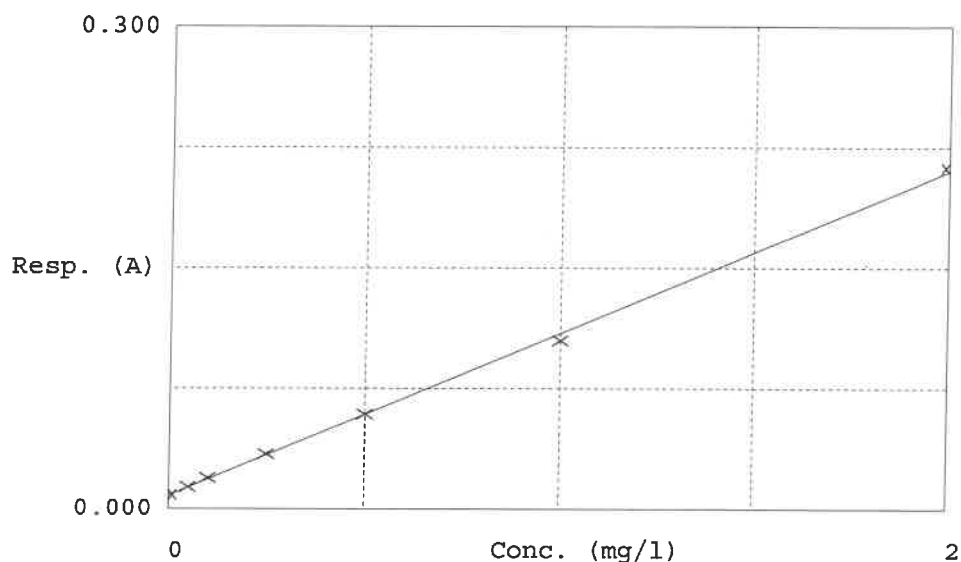

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.009	0.0038	0.0000	-
2	Phenol-2	0.014	0.0529	0.0500	5.8
3	Phenol-2	0.019	0.1094	0.1000	9.4
4	Phenol-2	0.034	0.2557	0.2500	2.3
5	Phenol-2	0.059	0.5019	0.5000	0.4
6	Phenol-2	0.105	0.9563	1.0000	-4.4
7	Phenol-2	0.212	2.0201	2.0000	1.0

12
8/23/22