


LB121832

7471B

INSTRUMENT ID: CV2

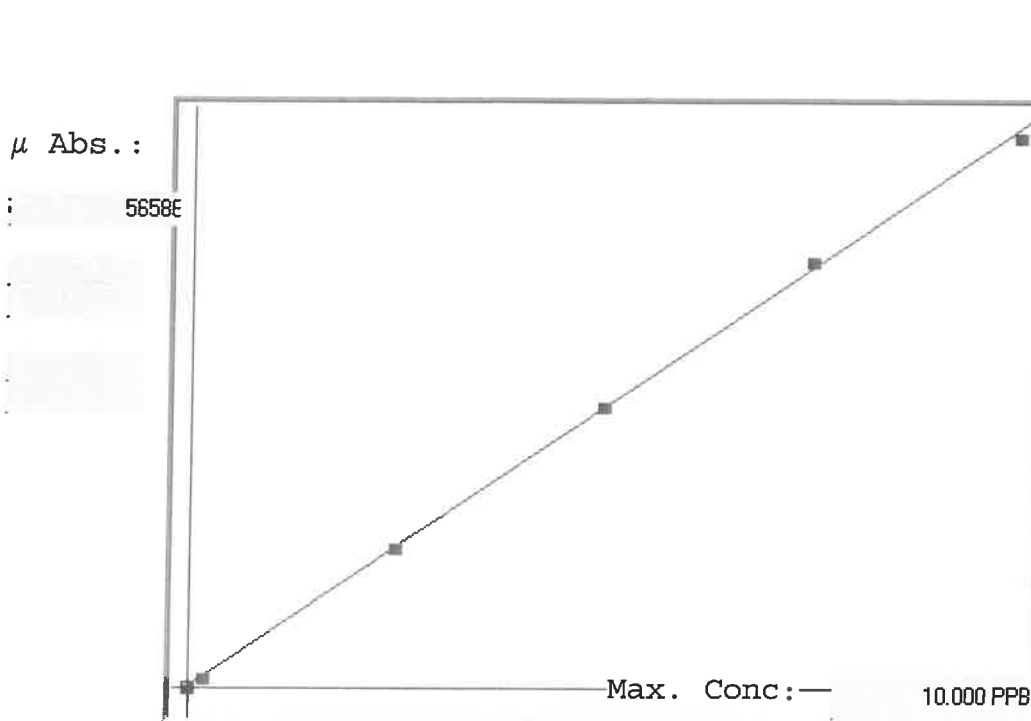

Linear

A= 0.0000e+000

B= 1.7473e-004

C= -1.4532e-002

Rho= 0.9997639

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1/00
0.0	0.000	-0.026	-0.026	-68	0.000	-68					
0.2	0.200	0.171	-0.029	1059	0.0 %	1059					-15
2.5	2.500	2.511	0.011	14452	0.0 %	14452					0
5.0	5.000	5.032	0.032	28883	0.0 %	28883					1
7.5	7.500	7.640	0.140	43809	0.0 %	43809					2
10.0	10.000	9.873	-0.127	56586	0.0 %	56586					-1

LB121832 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 01 Sep 2022 08:33:51

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	53	-88	-	0.0000	7471B	PPB	01 Sep 2022 09:09:40	S	Std
0.2 - 1	51.2	1059	-	0.2000	7471B	PPB	01 Sep 2022 09:11:58	S	Std
2.5 - 1	52.5	14452	-	2.5000	7471B	PPB	01 Sep 2022 09:14:15	S	Std
5.0 - 1	55	28883	-	5.0000	7471B	PPB	01 Sep 2022 09:16:32	S	Std
7.5 - 1	57.5	43809	-	7.5000	7471B	PPB	01 Sep 2022 09:18:49	S	Std
10.0 - 1	57.0	56586	-	10.0000	7471B	PPB	01 Sep 2022 09:23:40	S	Std
ICV14 - 1	ICV14	23036	4.0106	-	7471B	PPB	01 Sep 2022 09:26:32	U	SMPL
ICB14 - 1	ICB14	-115	-0.0346	-	7471B	PPB	01 Sep 2022 09:28:46	U	SMPL
CCV32 - 1	CCV32	28916	5.0380	-	7471B	PPB	01 Sep 2022 09:31:03	U	SMPL
CCB32 - 1	CCB32	-152	-0.0411	-	7471B	PPB	01 Sep 2022 09:33:18	U	SMPL
CRA - 1	CRA	1083	0.1747	-	7471B	PPB	01 Sep 2022 09:35:35	U	SMPL
HighStd - 1	HighStd	57134	9.9685	-	7471B	PPB	01 Sep 2022 09:37:50	U	SMPL
ChkStd - 1	ChkStd	41530	7.2420	-	7471B	PPB	01 Sep 2022 09:40:05	U	SMPL
PB147390BL - 1	PBS	-34	-0.0205	-	7471B	PPB	01 Sep 2022 09:45:14	U	SMPL
PB147390BS - 1	LCSS	21129	3.6774	-	7471B	PPB	01 Sep 2022 09:47:30	U	SMPL
N4421-01 - 1	WC-PALM-SP-01	99388	17.3516	-	7471B	PPB	01 Sep 2022 09:49:46	U	SMPL
N4421-06 - 1	WC-PALM-SP-02	94195	16.4442	-	7471B	PPB	01 Sep 2022 09:52:04	U	SMPL
N4421-11 - 1	WC-PALM-SP-03	66665	11.6339	-	7471B	PPB	01 Sep 2022 09:54:24	U	SMPL
N4423-01 - 1	WC-1	321	0.0416	-	7471B	PPB	01 Sep 2022 09:56:44	U	SMPL
N4423-04 - 1	WC-2	1417	0.2331	-	7471B	PPB	01 Sep 2022 09:59:02	U	SMPL
CCV33 - 1	CCV33	28620	4.9863	-	7471B	PPB	01 Sep 2022 10:01:17	U	SMPL
CCB33 - 1	CCB33	-144	-0.0397	-	7471B	PPB	01 Sep 2022 10:03:33	U	SMPL
N4424-01 - 1	VNJ-219	2838	0.4814	-	7471B	PPB	01 Sep 2022 10:05:50	U	SMPL
N4424-03 - 1	VNJ-241	4075	0.6975	-	7471B	PPB	01 Sep 2022 10:08:06	U	SMPL
N4426-01 - 1	ETGI-344	14148	2.4576	-	7471B	PPB	01 Sep 2022 10:10:21	U	SMPL
N4430-01 - 1	CRUSHED-MASONARY-PILE-3	4808	0.7906	-	7471B	PPB	01 Sep 2022 10:12:37	U	SMPL
N4431-01 - 1	CRUSHED-MASONARY-PILE-4	4728	0.8116	-	7471B	PPB	01 Sep 2022 10:14:54	U	SMPL
N4433-01 - 1	EP-1	510	0.0746	-	7471B	PPB	01 Sep 2022 10:17:10	U	SMPL
N4433-02 - 1	EP-2	2623	0.4438	-	7471B	PPB	01 Sep 2022 10:19:27	U	SMPL
N4433-03 - 1	EP-3	3551	0.6059	-	7471B	PPB	01 Sep 2022 10:21:44	U	SMPL
N4433-04 - 1	EP-BLIND-DUPLICATE	3691	0.6304	-	7471B	PPB	01 Sep 2022 10:24:02	U	SMPL
N4433-05 - 1	EP-4	1287	0.2103	-	7471B	PPB	01 Sep 2022 10:26:17	U	SMPL
CCV34 - 1	CCV34	27098	4.7203	-	7471B	PPB	01 Sep 2022 10:28:33	U	SMPL
CCB34 - 1	CCB34	-142	-0.0393	-	7471B	PPB	01 Sep 2022 10:30:49	U	SMPL
N4433-05DUP - 1	EP-4DUP	1319	0.2159	-	7471B	PPB	01 Sep 2022 10:36:21	U	SMPL
N4433-06 - 1	N4433-05MS	22964	3.9980	-	7471B	PPB	01 Sep 2022 10:38:37	U	SMPL
N4433-07 - 1	N4433-05MSD	22758	3.9622	-	7471B	PPB	01 Sep 2022 10:43:40	U	SMPL
PB147401BL - 1	PBS	-142	-0.0393	-	7471B	PPB	01 Sep 2022 10:45:55	U	SMPL
PB147401BS - 1	LCSS	21250	3.6985	-	7471B	PPB	01 Sep 2022 10:48:11	U	SMPL
N4439-01 - 1	KTS2-TR-03-0-05	16974	2.9513	-	7471B	PPB	01 Sep 2022 10:50:28	U	SMPL
N4439-02 - 1	KTS2-TR-01-0-5	23998	4.1787	-	7471B	PPB	01 Sep 2022 10:52:45	U	SMPL
N4439-03 - 1	KTS2-MH-02-0-20	39902	6.9576	-	7471B	PPB	01 Sep 2022 10:55:03	U	SMPL
N4439-04 - 1	KTS2-MH-01-0-20	119166	20.8074	-	7471B	PPB	01 Sep 2022 10:57:21	U	SMPL
N4439-05 - 1	KTS2-TR-02-0-12	24212	4.2160	-	7471B	PPB	01 Sep 2022 10:59:39	U	SMPL
CCV35 - 1	CCV35	27988	4.8758	-	7471B	PPB	01 Sep 2022 11:01:58	U	SMPL
CCB35 - 1	CCB35	-154	-0.0414	-	7471B	PPB	01 Sep 2022 11:04:15	U	SMPL
N4443-01 - 1	HD-01-083022	4274	0.7323	-	7471B	PPB	01 Sep 2022 11:06:32	U	SMPL
N4447-01 - 1	AUD-1656-OIL	-75	-0.0276	-	7471B	PPB	01 Sep 2022 11:08:48	U	SMPL
N4450-01 - 1	EO-03-083022	3579	0.6108	-	7471B	PPB	01 Sep 2022 11:11:04	U	SMPL
N4451-01 - 1	TP1	4542	0.7791	-	7471B	PPB	01 Sep 2022 11:13:19	U	SMPL
N4451-01DUP - 1	TP1DUP	3855	0.6591	-	7471B	PPB	01 Sep 2022 11:15:36	U	SMPL
N4451-01MS - 1	TP1MS	25542	4.4484	-	7471B	PPB	01 Sep 2022 11:17:52	U	SMPL
N4451-01MSD - 1	TP1MSD	25694	4.4750	-	7471B	PPB	01 Sep 2022 11:20:08	U	SMPL
N4453-01 - 1	SASP2-T-5-(0-5)	8460	1.4637	-	7471B	PPB	01 Sep 2022 11:22:27	U	SMPL
N4453-02 - 1	SASP2-T-5-(5-10)	2430	0.4101	-	7471B	PPB	01 Sep 2022 11:24:46	U	SMPL
N4464-01 - 1	WC-1	2770	0.4695	-	7471B	PPB	01 Sep 2022 11:27:02	U	SMPL
CCV36 - 1	CCV36	28933	5.0409	-	7471B	PPB	01 Sep 2022 11:29:18	U	SMPL
CCB36 - 1	CCB36	-156	-0.0418	-	7471B	PPB	01 Sep 2022 11:31:33	U	SMPL
N4464-03 - 1	WC-2	2346	0.3954	-	7471B	PPB	01 Sep 2022 11:33:51	U	SMPL
N4465-01 - 1	OK-1-083122	2952	0.5013	-	7471B	PPB	01 Sep 2022 11:36:06	U	SMPL
N4469-01 - 1	TR-06-083122	2728	0.4621	-	7471B	PPB	01 Sep 2022 11:38:23	U	SMPL
N4433-05LX5 - 1		-14	-0.0170	-	7471B	PPB	01 Sep 2022 11:40:38	U	SMPL
N4433-05A - 1		22739	3.9587	-	7471B	PPB	01 Sep 2022 11:42:54	U	SMPL
N4451-01LX5 - 1		636	0.0966	-	7471B	PPB	01 Sep 2022 11:45:10	U	SMPL
N4451-01A - 1		26692	4.6494	-	7471B	PPB	01 Sep 2022 11:47:28	U	SMPL
N4421-06DLX5 - 1		21043	3.6623	-	7471B	PPB	01 Sep 2022 11:49:45	U	SMPL
N4421-01DLX5 - 1		19824	3.4493	-	7471B	PPB	01 Sep 2022 11:52:04	U	SMPL
N4421-11DLX2 - 1		33487	5.8367	-	7471B	PPB	01 Sep 2022 11:54:21	U	SMPL
CCV37 - 1	CCV37	27609	4.8096	-	7471B	PPB	01 Sep 2022 11:56:38	U	SMPL
CCB37 - 1	CCB37	-150	-0.0407	-	7471B	PPB	01 Sep 2022 11:58:57	U	SMPL
N4439-04DLX5 - 1		24916	4.3391	-	7471B	PPB	01 Sep 2022 12:01:15	U	SMPL
CCV38 - 1	CCV38	31532	5.4951	-	7471B	PPB	01 Sep 2022 12:08:43	U	SMPL
CCB38 - 1	CCB38	-140	-0.0390	-	7471B	PPB	01 Sep 2022 12:11:00	U	SMPL