

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

9/6/2022 11:34

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.240	0.0	0.070	
ICB1	1.209	0.0	0.001	
CCV1	241.330	0.0	0.179	
CCB1	0.878	0.0	0.001	
PB147461BL	0.443	0.0	0.001	
N4478-01	0.847	0.0	0.001	
N4478-01DUP	0.722	0.0	0.001	
N4502-02	0.769	0.0	0.001	
PB147642BL	0.769	0.0	0.001	
N4485-06	0.835	0.0	0.001	
N4485-06DUP	0.801	0.0	0.001	
N4490-02	0.829	0.0	0.001	
N4490-07	0.772	0.0	0.001	
N4495-02	0.949	0.0	0.001	
CCV2	239.999	0.0	0.178	
CCB2	0.784	0.0	0.001	
N4500-02	0.332	0.0	0.001	
N4500-04	0.731	0.0	0.001	
N4500-06	0.808	0.0	0.001	
N4500-08	0.752	0.0	0.001	
N4500-10	0.747	0.0	0.001	
N4500-12	0.910	0.0	0.001	
N4500-14	0.892	0.0	0.001	
N4500-16	0.909	0.0	0.001	
N4500-18	0.766	0.0	0.001	
N4500-20	0.746	0.0	0.001	
CCV3	235.113	0.0	0.175	
CCB3	1.294	0.0	0.001	
PB147482BL	0.641	0.0	0.001	
N4501-02	0.541	0.0	0.001	
N4501-02DUP	0.907	0.0	0.001	
N4501-04	0.975	0.0	0.001	
N4501-06	0.883	0.0	0.001	
N4501-08	0.741	0.0	0.001	
N4501-12	0.479	0.0	0.001	
N4501-14	0.966	0.0	0.001	
N4501-16	1.155	0.0	0.001	
CCV4	245.436	0.0	0.182	
CCB4	1.112	0.0	0.001	
N4502-01	1.142	0.0	0.001	
N4501-10	0.991	0.0	0.001	
CCV5	247.451	0.0	0.184	
CCB5	1.076	0.0	0.001	

N 43
 Mean 31.039
 SD 78.6904
 CV% 253.52

L B1218P2

PB147482 BL
 12
 9/6/22

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 06 09:22:02 2022

Tue Sep 06 11:26:05 2022

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.4291	µg/l	9/6/2022 9:40:56	
5.0PPBCN	A	Total CN	P	4.9201	µg/l	9/6/2022 9:40:57	
10PPBCN	A	Total CN	P	9.4705	µg/l	9/6/2022 9:40:58	
50PPBCN	A	Total CN	P	51.218	µg/l	9/6/2022 9:40:59	
100PPBCN	A	Total CN	P	96.6046	µg/l	9/6/2022 9:41:00	
250PPBCN	A	Total CN	P	253.5781	µg/l	9/6/2022 9:41:01	
500PPBCN	A	Total CN	P	498.7796	µg/l	9/6/2022 9:41:02	
ICV1	S	Total CN	P	94.2399	µg/l	9/6/2022 10:56:37	
ICB1	S	Total CN	P	1.2087	µg/l	9/6/2022 10:56:38	
CCV1	S	Total CN	P	241.3302	µg/l	9/6/2022 10:56:41	
CCB1	S	Total CN	P	0.8778	µg/l	9/6/2022 10:56:43	
PB147461BL	S	Total CN	P	0.4425	µg/l	9/6/2022 10:56:44	
N4478-01	S	Total CN	P	0.847	µg/l	9/6/2022 10:56:46	
N4478-01DUP	S	Total CN	P	0.7222	µg/l	9/6/2022 11:04:11	
N4502-02	S	Total CN	P	0.7688	µg/l	9/6/2022 11:04:12	
PB147462BL	S	Total CN	P	0.7694	µg/l	9/6/2022 11:04:13	
N4485-06	S	Total CN	P	0.8349	µg/l	9/6/2022 11:04:15	
N4485-06DUP	S	Total CN	P	0.8008	µg/l	9/6/2022 11:04:16	
N4490-02	S	Total CN	P	0.8294	µg/l	9/6/2022 11:04:17	
N4490-07	S	Total CN	P	0.7715	µg/l	9/6/2022 11:04:18	
N4495-02	S	Total CN	P	0.949	µg/l	9/6/2022 11:04:19	
CCV2	S	Total CN	P	239.9995	µg/l	9/6/2022 11:04:21	
CCB2	S	Total CN	P	0.7843	µg/l	9/6/2022 11:11:46	
N4500-02	S	Total CN	P	0.3323	µg/l	9/6/2022 11:11:47	
N4500-04	S	Total CN	P	0.7309	µg/l	9/6/2022 11:11:48	
N4500-06	S	Total CN	P	0.8079	µg/l	9/6/2022 11:11:49	
N4500-08	S	Total CN	P	0.7525	µg/l	9/6/2022 11:11:50	
N4500-10	S	Total CN	P	0.7466	µg/l	9/6/2022 11:11:51	
N4500-12	S	Total CN	P	0.91	µg/l	9/6/2022 11:11:52	
N4500-14	S	Total CN	P	0.8918	µg/l	9/6/2022 11:11:53	
N4500-16	S	Total CN	P	0.9088	µg/l	9/6/2022 11:11:54	
N4500-18	S	Total CN	P	0.7659	µg/l	9/6/2022 11:11:55	
N4500-20	S	Total CN	P	0.7458	µg/l	9/6/2022 11:11:56	
CCV3	S	Total CN	P	235.1131	µg/l	9/6/2022 11:19:19	
CCB3	S	Total CN	P	1.2943	µg/l	9/6/2022 11:19:20	
PB147482BL	S	Total CN	P	0.6413	µg/l	9/6/2022 11:19:21	
N4501-02	S	Total CN	P	0.5406	µg/l	9/6/2022 11:19:22	
N4501-02DUP	S	Total CN	P	0.9065	µg/l	9/6/2022 11:19:23	
N4501-04	S	Total CN	P	0.9749	µg/l	9/6/2022 11:19:24	
N4501-06	S	Total CN	P	0.8831	µg/l	9/6/2022 11:19:25	
N4501-08	S	Total CN	P	0.7408	µg/l	9/6/2022 11:19:26	
N4501-12	S	Total CN	P	0.4787	µg/l	9/6/2022 11:19:28	

N4501-14	S	Total CN	P	0.9655 µg/l	9/6/2022 11:25:57
N4501-16	S	Total CN	P	1.1552 µg/l	9/6/2022 11:25:58
CCV4	S	Total CN	P	245.4361 µg/l	9/6/2022 11:25:59
CCB4	S	Total CN	P	1.1122 µg/l	9/6/2022 11:26:00
N4502-01	S	Total CN	P	1.1418 µg/l	9/6/2022 11:26:01
N4501-10	S	Total CN	P	0.9911 µg/l	9/6/2022 11:26:02
CCV5	S	Total CN	P	247.4509 µg/l	9/6/2022 11:26:04
CCB5	S	Total CN	P	1.0756 µg/l	9/6/2022 11:26:05

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

9/6/2022 9:50


Test Total CN

Accepted 9/6/2022 9:50

Factor 1349
Bias 0

Coeff. of det. 0.999865

Errors

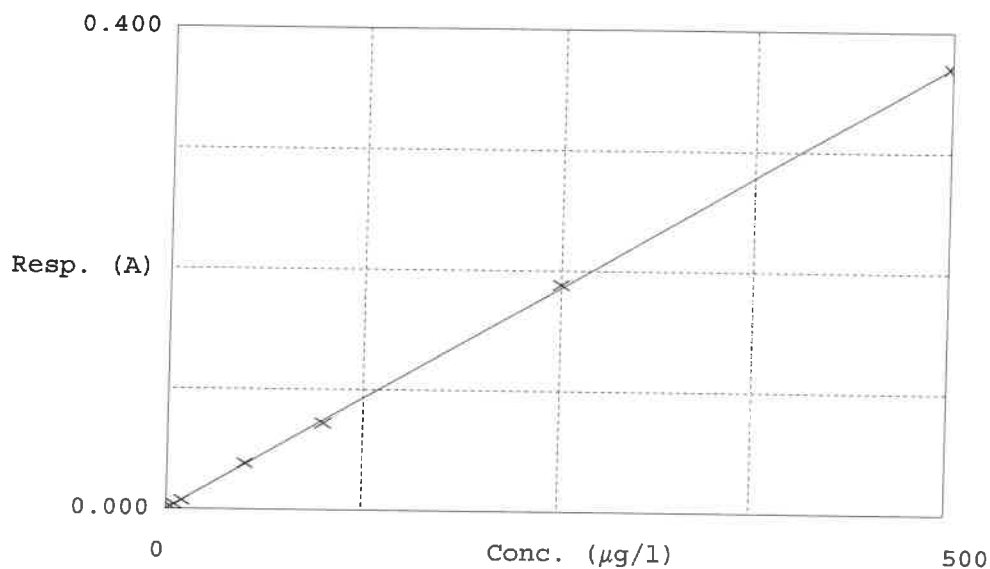

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.4291	0.0000	-
2	5.0PPBCN	0.004	4.9201	5.0000	-1.6
3	10PPBCN	0.007	9.4705	10.0000	-5.3
4	50PPBCN	0.038	51.2180	50.0000	2.4
5	100PPBCN	0.072	96.6046	100.0000	-3.4
6	250PPBCN	0.188	253.5781	250.0000	1.4
7	500PPBCN	0.370	498.7796	500.0000	-0.2

12
9/6/22