

LB121948

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : IL

Instrument ID : Konelab

9/9/2022 12:31

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.000	0.0	0.113	
ICB1	0.003	0.0	0.008	
CCV1	0.980	0.0	0.111	
CCB1	0.002	0.0	0.008	
PB147567BL	0.005	0.0	0.008	
PB147567BS	1.001	0.0	0.113	
N4437-01	-0.004	0.0	0.007	
N4437-01DUP	-0.011	0.0	0.006	
N4437-01MS	1.046	0.0	0.118	
N4437-01MSD	1.035	0.0	0.116	
N4437-02	-0.002	0.0	0.007	
N4452-01	-0.001	0.0	0.007	
CCV2	0.982	0.0	0.111	
CCB2	0.001	0.0	0.007	

N	14
Mean	0.431
SD	0.5180
CV%	120.13

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 09 11:01:54 2022

Fri Sep 09 12:22:27 2022

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0019	mg/l	9/9/2022 11:19:17	
0.05PPM	A	Phenolics-	P	0.0532	mg/l	9/9/2022 11:19:18	
0.1PPM	A	Phenolics-	P	0.1055	mg/l	9/9/2022 11:19:19	
0.25PPM	A	Phenolics-	P	0.2527	mg/l	9/9/2022 11:19:20	
0.50PPM	A	Phenolics-	P	0.4957	mg/l	9/9/2022 11:19:21	
1.0PPM	A	Phenolics-	P	0.989	mg/l	9/9/2022 11:19:22	
2.0PPM	A	Phenolics-	P	2.0059	mg/l	9/9/2022 11:19:23	
ICV1	S	Phenolics-	P	1	mg/l	9/9/2022 12:14:36	
ICB1	S	Phenolics-	P	0.0026	mg/l	9/9/2022 12:14:38	
CCV1	S	Phenolics-	P	0.9797	mg/l	9/9/2022 12:14:40	
CCB1	S	Phenolics-	P	0.0022	mg/l	9/9/2022 12:14:43	
PB147567BL	S	Phenolics-	P	0.0051	mg/l	9/9/2022 12:14:44	
PB147567BS	S	Phenolics-	P	1.0005	mg/l	9/9/2022 12:14:46	
N4437-01	S	Phenolics-	P	-0.0037	mg/l	9/9/2022 12:22:18	
N4437-01DUP	S	Phenolics-	P	-0.0114	mg/l	9/9/2022 12:22:19	
N4437-01MS	S	Phenolics-	P	1.0462	mg/l	9/9/2022 12:22:20	
N4437-01MSD	S	Phenolics-	P	1.035	mg/l	9/9/2022 12:22:21	
N4437-02	S	Phenolics-	P	-0.0018	mg/l	9/9/2022 12:22:22	
N4452-01	S	Phenolics-	P	-0.0008	mg/l	9/9/2022 12:22:23	
CCV2	S	Phenolics-	P	0.9822	mg/l	9/9/2022 12:22:25	
CCB2	S	Phenolics-	P	0.0012	mg/l	9/9/2022 12:22:27	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

9/9/2022 11:19


Test Phenolics-

Accepted 9/9/2022 11:19

Factor 9.491
Bias 0.007

Coeff. of det. 0.999928

Errors

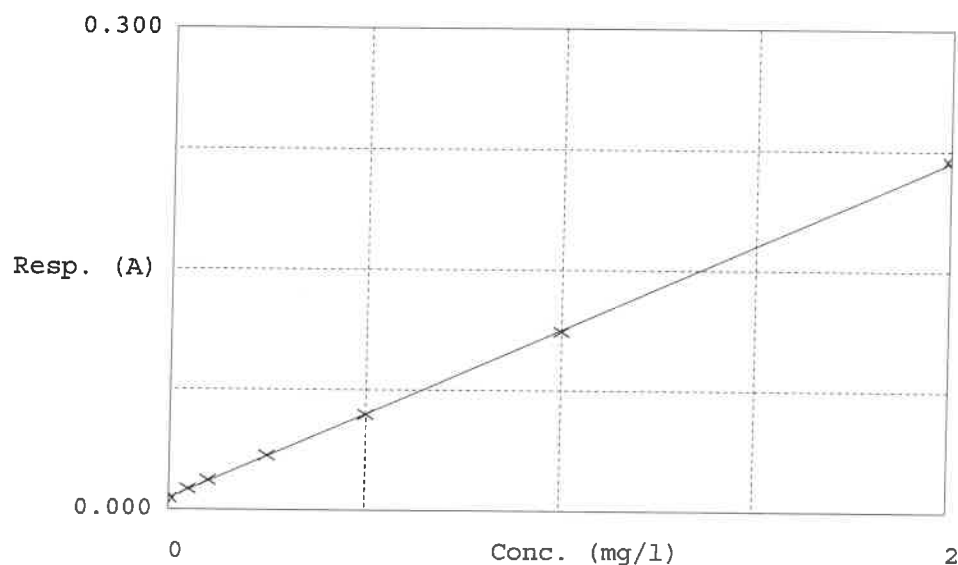

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.007	-0.0019	0.0000	-
2	Phenol-2	0.013	0.0532	0.0500	6.4
3	Phenol-2	0.018	0.1055	0.1000	5.5
4	Phenol-2	0.034	0.2527	0.2500	1.1
5	Phenol-2	0.060	0.4957	0.5000	-0.9
6	Phenol-2	0.112	0.9890	1.0000	-1.1
7	Phenol-2	0.219	2.0059	2.0000	0.3

12
9/9/22