

LB 121963


245.1

INSTRUMENT ID: CV2

Linear

 μ Abs.:

26847

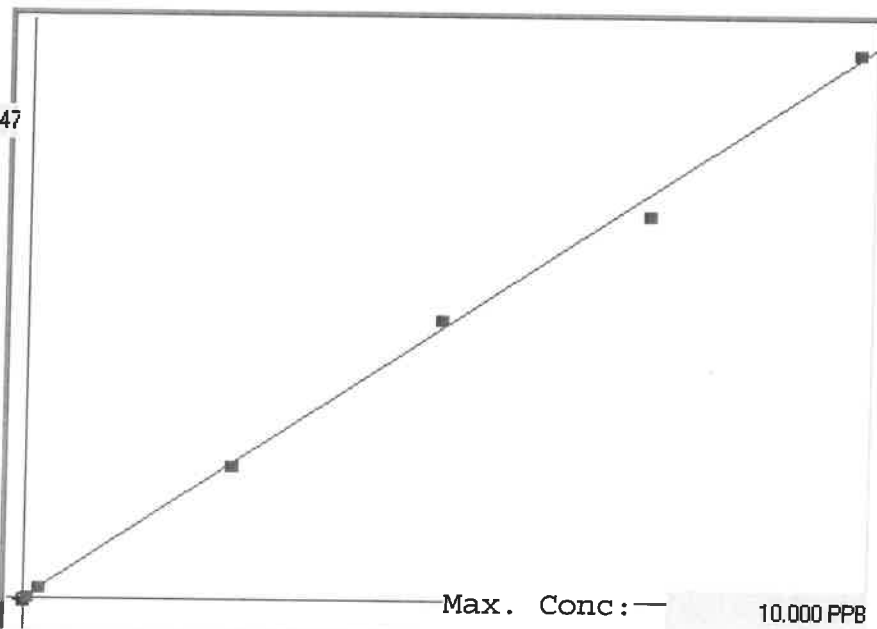

A= 0.0000e+000

B= 3.7736e-004

C= 5.5505e-003

Rho= 0.9989717

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.049	-0.049	-144	0.000	-144				
0.05	0.050	0.065	0.015	158	0.0 %	158	0			
0.2	0.200	0.230	0.030	594	0.0 %	594				
2.5	2.500	2.505	0.005	6624	0.0 %	6624				
5.0	5.000	5.220	0.220	13818	0.0 %	13818				
7.5	7.500	7.142	-0.358	18913	0.0 %	18913				
10.0	10.000	10.136	0.136	26847	0.0 %	26847				

MB
9/12/14

LB121963 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 12 Sep 2022 09:46:35

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-144	-	0.0000	245.1	PPB	12 Sep 2022 09:50:09	S	Std
0.05 - 1	50.05	158	-	0.0500	245.1	PPB	12 Sep 2022 09:55:07	S	Std
0.2 - 1	50.2	594	-	0.2000	245.1	PPB	12 Sep 2022 09:57:24	S	Std
2.5 - 1	52.5	6824	-	2.5000	245.1	PPB	12 Sep 2022 09:59:41	S	Std
5.0 - 1	55	13818	-	5.0000	245.1	PPB	12 Sep 2022 10:01:57	S	Std
7.5 - 1	57.5	18913	-	7.5000	245.1	PPB	12 Sep 2022 10:17:22	S	Std
10.0 - 1	570	26847	-	10.0000	245.1	PPB	12 Sep 2022 10:35:57	S	Std
ICV25 - 1	ICV25	10375	3.9206	-245.1		PPB	12 Sep 2022 11:01:05	U	SMPL
ICB25 - 1	ICB25	-194	-0.0677	-245.1		PPB	12 Sep 2022 11:03:20	U	SMPL
CCV79 - 1	CCV79	13700	5.1753	-245.1		PPB	12 Sep 2022 11:10:39	U	SMPL
CCB79 - 1	CCB79	-183	-0.0635	-245.1		PPB	12 Sep 2022 11:12:54	U	SMPL
CRA - 1	CRA	111	0.0474	-245.1		PPB	12 Sep 2022 11:17:42	U	SMPL
HighStd - 1	HighStd	25526	9.6379	-245.1		PPB	12 Sep 2022 11:22:31	U	SMPL
ChkStd - 1	ChkStd	18958	7.1596	-245.1		PPB	12 Sep 2022 11:27:22	U	SMPL
PB147572BL - 1	PBW	-183	-0.0635	-245.1		PPB	12 Sep 2022 11:29:38	U	SMPL
PB147572BS - 1	LCSW	9445	3.5697	-245.1		PPB	12 Sep 2022 11:41:21	U	SMPL
N4393-01 - 1	20220737-DI-WATER	-223	-0.0786	-245.1		PPB	12 Sep 2022 11:43:37	U	SMPL
N4395-01 - 1	20220738-MANASQUAN-WATER	-96	-0.0307	-245.1		PPB	12 Sep 2022 11:45:53	U	SMPL
N4437-01 - 1	MW-2-(17)	172	0.0705	-245.1		PPB	12 Sep 2022 11:48:10	U	SMPL
N4437-02 - 1	BASMENT-STAND-PIPE	-152	-0.0518	-245.1		PPB	12 Sep 2022 11:50:27	U	SMPL
N4452-01 - 1	MW-2-(22)	386	0.1512	-245.1		PPB	12 Sep 2022 11:52:43	U	SMPL
CCV80 - 1	CCV80	12167	4.5968	-245.1		PPB	12 Sep 2022 11:57:31	U	SMPL
CCB80 - 1	CCB80	-208	-0.0729	-245.1		PPB	12 Sep 2022 11:59:45	U	SMPL
N4452-01DUP - 1	MW-2-(22)DUP	423	0.1652	-245.1		PPB	12 Sep 2022 12:02:01	U	SMPL
N4452-01MS - 1	MW-2-(22)MS	12521	4.7304	-245.1		PPB	12 Sep 2022 12:06:37	U	SMPL
N4452-01MSD - 1	MW-2-(22)MSD	10873	4.1085	-245.1		PPB	12 Sep 2022 12:13:50	U	SMPL
N4452-01LX5 - 1		-118	-0.0390	-245.1		PPB	12 Sep 2022 12:16:05	U	SMPL
N4452-01A - 1		10878	4.1104	-245.1		PPB	12 Sep 2022 12:18:21	U	SMPL
CCV81 - 1	CCV81	13132	4.9610	-245.1		PPB	12 Sep 2022 12:20:37	U	SMPL
CCB81 - 1	CCB81	-166	-0.0571	-245.1		PPB	12 Sep 2022 12:22:54	U	SMPL