


LB122247

7470A

INSTRUMENT ID: CV4

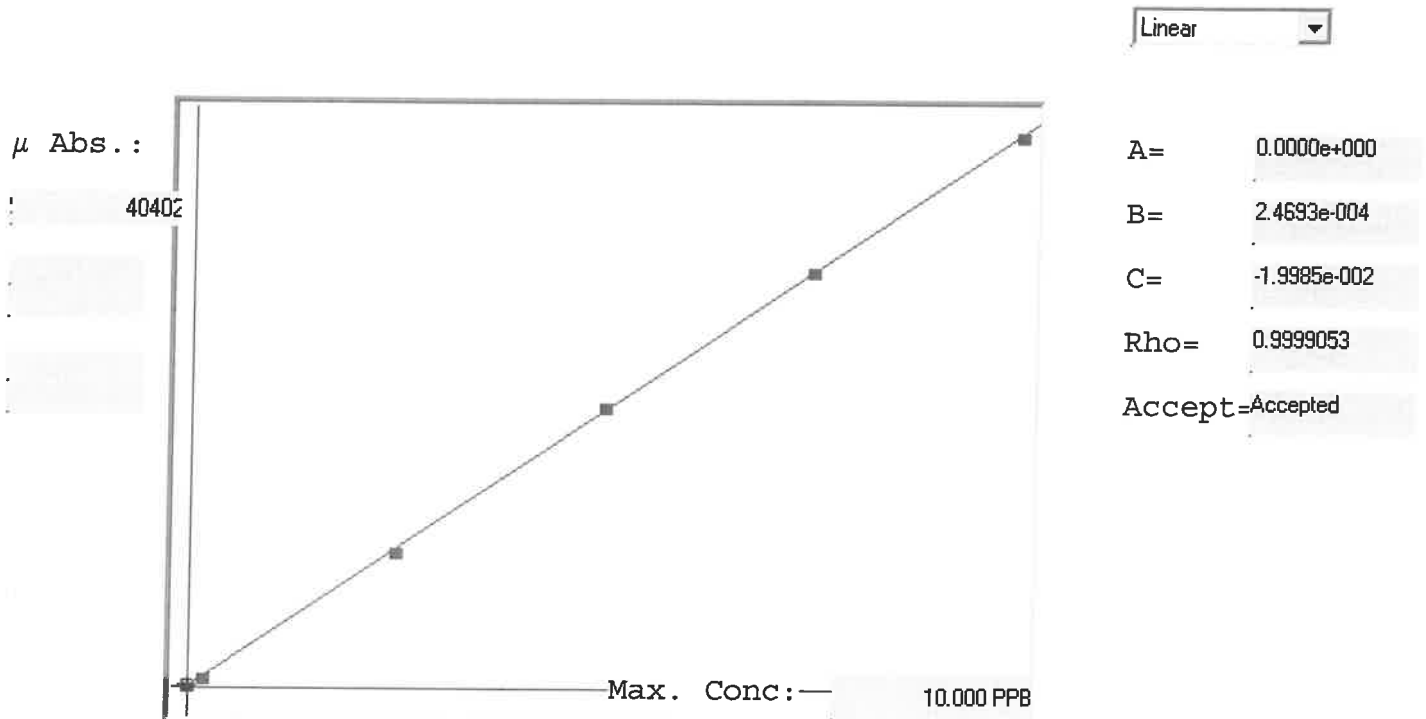

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%1)
0.0	0.000	0.036	0.036	227	0.000	227					
0.2	0.200	0.162	-0.038	736	0.0 %	736					-19
2.5	2.500	2.441	-0.059	9968	0.0 %	9968					12
5.0	5.000	5.083	0.083	20667	0.0 %	20667					1
7.5	7.500	7.521	0.021	30539	0.0 %	30539					0
10.0	10.000	9.956	-0.044	40402	0.0 %	40402					0

LB122247 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Sep 2022 16:23:42

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	227	-	0.0000	7470A	PPB	28 Sep 2022 16:24:32	S	Std
0.2 - 1	50.2	736	-	0.2000	7470A	PPB	28 Sep 2022 16:26:49	S	Std
2.5 - 1	52.5	9968	-	2.5000	7470A	PPB	28 Sep 2022 16:29:07	S	Std
5.0 - 1	55	20667	-	5.0000	7470A	PPB	28 Sep 2022 16:31:24	S	Std
7.5 - 1	57.5	30539	-	7.5000	7470A	PPB	28 Sep 2022 16:33:42	S	Std
10.0 - 1	511	40402	-	10.0000	7470A	PPB	28 Sep 2022 16:35:59	S	Std
ICV50 - 1	ICV50	16367	4.0215	-	7470A	PPB	28 Sep 2022 16:39:28	U	SMPL
ICB50 - 1	ICB50	8	-0.0180	-	7470A	PPB	28 Sep 2022 16:44:21	U	SMPL
CCV84 - 1	CCV84	20916	5.1448	-	7470A	PPB	28 Sep 2022 16:46:36	U	SMPL
CCB84 - 1	CCB84	-81	-0.0400	-	7470A	PPB	28 Sep 2022 16:48:51	U	SMPL
CRA - 1	CRA	805	0.1788	-	7470A	PPB	28 Sep 2022 16:51:07	U	SMPL
HighStd - 1	HighStd	39977	9.8515	-	7470A	PPB	28 Sep 2022 16:53:22	U	SMPL
ChkStd - 1	ChkStd	29979	7.3827	-	7470A	PPB	28 Sep 2022 16:55:37	U	SMPL
PB147980BL - 1	PBW	-104	-0.0457	-	7470A	PPB	28 Sep 2022 17:00:38	U	SMPL
PB147980BS - 1	LCSW	16848	4.1403	-	7470A	PPB	28 Sep 2022 17:02:54	U	SMPL
N4850-02 - 1	WC-14B-SP-2	163	0.0203	-	7470A	PPB	28 Sep 2022 17:07:52	U	SMPL
N4850-02DUP - 1	WC-14B-SP-2DUP	105	0.0059	-	7470A	PPB	28 Sep 2022 17:10:08	U	SMPL
N4850-02MS - 1	WC-14B-SP-2MS	17722	4.3561	-	7470A	PPB	28 Sep 2022 17:12:26	U	SMPL
N4850-02MSD - 1	WC-14B-SP-2MSD	15881	3.9015	-	7470A	PPB	28 Sep 2022 17:14:44	U	SMPL
PB147943TB - 1	PB147943TB	144	0.0156	-	7470A	PPB	28 Sep 2022 17:19:22	U	SMPL
CCV85 - 1	CCV85	21291	5.2374	-	7470A	PPB	28 Sep 2022 17:21:39	U	SMPL
CCB85 - 1	CCB85	49	-0.0079	-	7470A	PPB	28 Sep 2022 17:26:40	U	SMPL
N4850-02LX5 - 1		-72	-0.0378	-	7470A	PPB	28 Sep 2022 17:28:55	U	SMPL
N4850-02A - 1		17043	4.1884	-	7470A	PPB	28 Sep 2022 17:31:11	U	SMPL
CCV86 - 1	CCV86	21478	5.2836	-	7470A	PPB	28 Sep 2022 17:35:01	U	SMPL
CCB86 - 1	CCB86	-61	-0.0350	-	7470A	PPB	28 Sep 2022 17:37:16	U	SMPL