


7470A

LB122316 INSTRUMENT ID: CV1

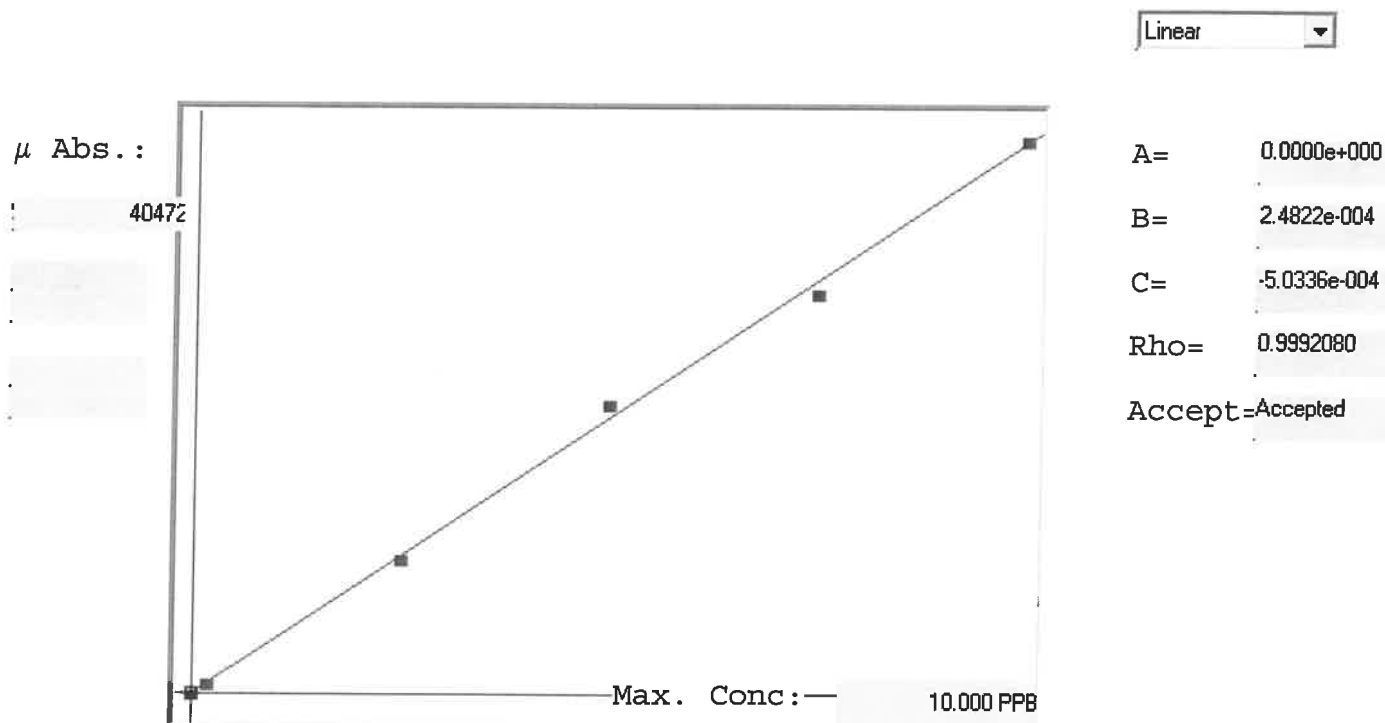

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	23	0.000	23				
0.2	0.200	0.179	-0.021	722	0.0 %	722				
2.5	2.500	2.441	-0.059	9834	0.0 %	9834				
5.0	5.000	5.263	0.263	21204	0.0 %	21204				
7.5	7.500	7.267	-0.233	29279	0.0 %	29279				
10.0	10.000	10.046	0.046	40472	0.0 %	40472				

LB122316 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Oct 2022 12:46:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	23	-	0.0000	7470A	PPB	03 Oct 2022 12:54:45	S	Std
0.2 - 1	8.2	722	-	0.2000	7470A	PPB	03 Oct 2022 12:57:02	S	Std
2.5 - 1	52.5	9834	-	2.5000	7470A	PPB	03 Oct 2022 12:59:19	S	Std
5.0 - 1	55.0	21204	-	5.0000	7470A	PPB	03 Oct 2022 13:01:36	S	Std
7.5 - 1	57.5	29279	-	7.5000	7470A	PPB	03 Oct 2022 13:03:53	S	Std
10.0 - 1	59.0	40472	-	10.0000	7470A	PPB	03 Oct 2022 13:06:10	S	Std
ICV57 - 1	ICV57	14915	3.7017	-	7470A	PPB	03 Oct 2022 13:18:50	U	SMPL
ICB57 - 1	ICB57	-67	-0.0171	-	7470A	PPB	03 Oct 2022 13:21:05	U	SMPL
CCV10 - 1	CCV10	20353	5.0516	-	7470A	PPB	03 Oct 2022 13:23:21	U	SMPL
CCB10 - 1	CCB10	-70	-0.0179	-	7470A	PPB	03 Oct 2022 13:25:36	U	SMPL
CRA - 1	CRA	674	0.1668	-	7470A	PPB	03 Oct 2022 13:27:53	U	SMPL
HighStd - 1	HighStd	39754	9.8673	-	7470A	PPB	03 Oct 2022 13:30:08	U	SMPL
ChkStd - 1	ChkStd	27497	6.8249	-	7470A	PPB	03 Oct 2022 13:32:23	U	SMPL
PB148076BL - 1	PBW	-86	-0.0219	-	7470A	PPB	03 Oct 2022 13:34:41	U	SMPL
PB148076BS - 1	LCSW	15530	3.8544	-	7470A	PPB	03 Oct 2022 13:36:58	U	SMPL
N4862-04 - 1	A2720	152	0.0372	-	7470A	PPB	03 Oct 2022 13:39:15	U	SMPL
N4862-04DUP - 1	A2720DUP	247	0.0608	-	7470A	PPB	03 Oct 2022 13:41:32	U	SMPL
N4862-04MS - 1	A2720MS	16604	4.1210	-	7470A	PPB	03 Oct 2022 13:43:49	U	SMPL
N4862-04MSD - 1	A2720MSD	16902	4.1950	-	7470A	PPB	03 Oct 2022 13:46:06	U	SMPL
N4915-01 - 1	257155-3	46	0.0109	-	7470A	PPB	03 Oct 2022 13:48:22	U	SMPL
CCV11 - 1	CCV11	20575	5.1067	-	7470A	PPB	03 Oct 2022 13:50:38	U	SMPL
CCB11 - 1	CCB11	-67	-0.0171	-	7470A	PPB	03 Oct 2022 13:52:54	U	SMPL
N4917-01 - 1	265393-5	61	0.0146	-	7470A	PPB	03 Oct 2022 13:55:10	U	SMPL
N4919-01 - 1	265393-6	143	0.0350	-	7470A	PPB	03 Oct 2022 13:57:25	U	SMPL
N4930-01 - 1	TOTES-0930	427	0.1055	-	7470A	PPB	03 Oct 2022 13:59:41	U	SMPL
N4862-04LX5 - 1	A2720L	11	0.0022	-	7470A	PPB	03 Oct 2022 14:01:59	U	SMPL
N4862-04A - 1	A2720A	16790	4.1672	-	7470A	PPB	03 Oct 2022 14:04:16	U	SMPL
CCV12 - 1	CCV12	20508	5.0900	-	7470A	PPB	03 Oct 2022 14:06:32	U	SMPL
CCB12 - 1	CCB12	-64	-0.0164	-	7470A	PPB	03 Oct 2022 14:08:50	U	SMPL