


7471B LB122410, INSTRUMENT ID:CV1, ANALYSIS DATE:10/08/2022

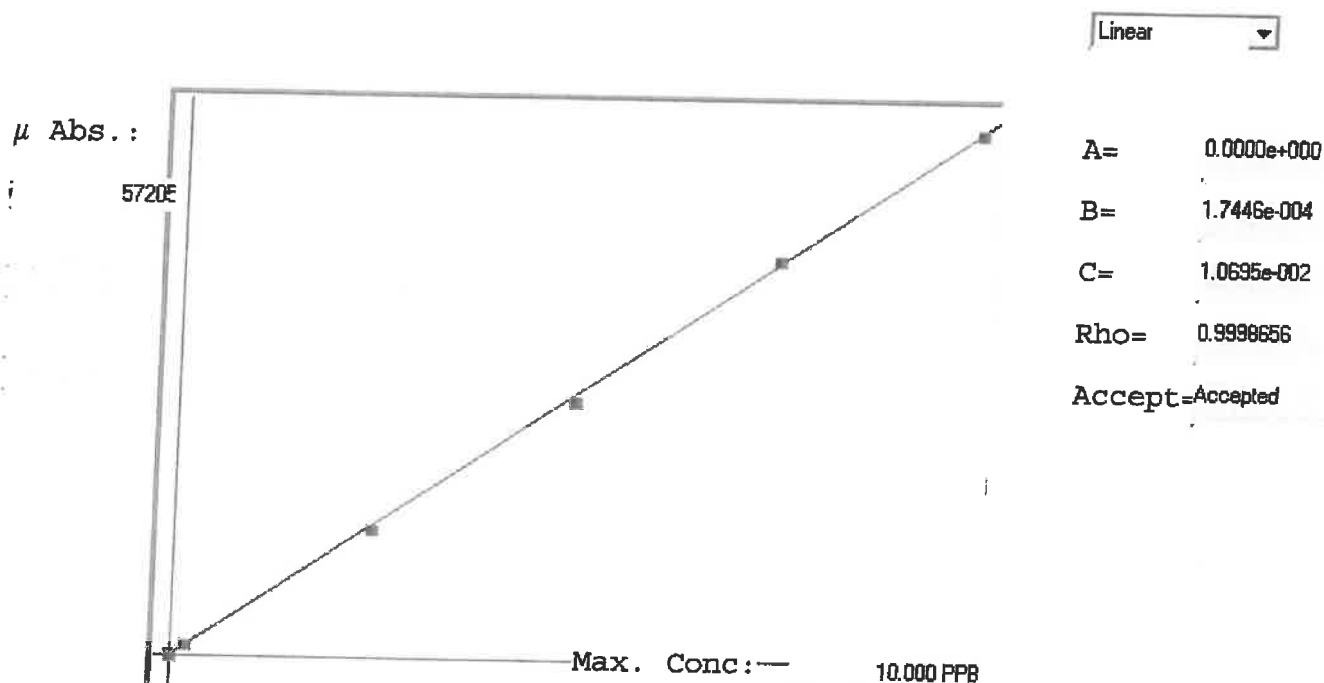

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.029	0.029	106	0.000	106					1.0
0.2	0.200	0.235	0.035	1285	0.0 %	1285					18
2.5	2.500	2.455	-0.045	14008	0.0 %	14008					-2
5.0	5.000	4.901	-0.099	28031	0.0 %	28031					-2
7.5	7.500	7.589	0.089	43439	0.0 %	43439					1
10.0	10.000	9.991	-0.009	57205	0.0 %	57205					0

LB122410 INSTRUMENT ID: CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Oct 2022 14:45:37

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1		106	-	0.0000	7471B	PPB	08 Oct 2022 14:45:48	S	Std
0.2 - 1		1285	-	0.2000	7471B	PPB	08 Oct 2022 14:48:05	S	Std
2.5 - 1		14008	-	2.5000	7471B	PPB	08 Oct 2022 14:50:22	S	Std
5.0 - 1		28031	-	5.0000	7471B	PPB	08 Oct 2022 14:52:39	S	Std
7.5 - 1		43439	-	7.5000	7471B	PPB	08 Oct 2022 14:54:57	S	Std
10.0 - 1		57205	-	10.0000	7471B	PPB	08 Oct 2022 14:57:15	S	Std
ICV65 - 1	ICV65	21347	3.7350	-	7471B	PPB	08 Oct 2022 15:00:07	U	SMPL
ICB65 - 1	ICB65	297	0.0625	-	7471B	PPB	08 Oct 2022 15:02:21	U	SMPL
CCV40 - 1	CCV40	27958	4.8884	-	7471B	PPB	08 Oct 2022 15:04:39	U	SMPL
CCB40 - 1	CCB40	228	0.0505	-	7471B	PPB	08 Oct 2022 15:06:54	U	SMPL
CRA - 1	CRA	1146	0.2106	-	7471B	PPB	08 Oct 2022 15:09:11	U	SMPL
HighStd - 1	HighStd	56478	9.8641	-	7471B	PPB	08 Oct 2022 15:12:11	U	SMPL
ChkStd - 1	ChkStd	39505	6.9029	-	7471B	PPB	08 Oct 2022 15:14:27	U	SMPL
PB148202BL - 1	PBS202	178	0.0418	-	7471B	PPB	08 Oct 2022 15:16:44	U	SMPL
PB148202BS - 1	LCS202	21371	3.7392	-	7471B	PPB	08 Oct 2022 15:19:02	U	SMPL
N5012-01 - 1	OE-3-100522	37477	6.5491	-	7471B	PPB	08 Oct 2022 15:21:19	U	SMPL
N5014-01 - 1	SB-04-0-2.0	1860	0.3352	-	7471B	PPB	08 Oct 2022 15:23:37	U	SMPL
N5014-02 - 1	SB-05-0-2.0	2887	0.5144	-	7471B	PPB	08 Oct 2022 15:25:56	U	SMPL
N5014-03 - 1	SB-05-2.0-3.0	1551	0.2813	-	7471B	PPB	08 Oct 2022 15:28:13	U	SMPL
N5014-03DUP - 1	SB-05-2.0-3.0DUP	1722	0.3111	-	7471B	PPB	08 Oct 2022 15:30:28	U	SMPL
CCV41 - 1	CCV41	26163	4.5752	-	7471B	PPB	08 Oct 2022 15:32:43	U	SMPL
CCB41 - 1	CCB41	262	0.0564	-	7471B	PPB	08 Oct 2022 15:34:58	U	SMPL
N5014-03MS - 1	SB-05-2.0-3.0MS	10620	1.8635	-	7471B	PPB	08 Oct 2022 15:37:16	U	SMPL
N5014-03MSD - 1	SB-05-2.0-3.0MSD	10396	1.8244	-	7471B	PPB	08 Oct 2022 15:40:12	U	SMPL
N5014-04 - 1	SB-06-0-2.0	2298	0.4116	-	7471B	PPB	08 Oct 2022 15:42:28	U	SMPL
N5014-05 - 1	SB-06-2.0-4.0	1043	0.1927	-	7471B	PPB	08 Oct 2022 15:44:45	U	SMPL
N5014-06 - 1	SB-07-0-2.0	1293	0.2363	-	7471B	PPB	08 Oct 2022 15:47:00	U	SMPL
N5014-07 - 1	SB-08-0-2.0	1199	0.2199	-	7471B	PPB	08 Oct 2022 15:49:17	U	SMPL
N5014-08 - 1	SB-09-0-2.0	1381	0.2516	-	7471B	PPB	08 Oct 2022 15:51:33	U	SMPL
N5014-09 - 1	SB-09-2.0-3.0	626	0.1199	-	7471B	PPB	08 Oct 2022 15:53:50	U	SMPL
N5014-10 - 1	SB-10-0-2.0	1768	0.3191	-	7471B	PPB	08 Oct 2022 15:56:07	U	SMPL
N5014-11 - 1	SB-10-0-2.0-DUP	2005	0.3605	-	7471B	PPB	08 Oct 2022 15:58:22	U	SMPL
CCV42 - 1	CCV42	25919	4.5326	-	7471B	PPB	08 Oct 2022 16:00:38	U	SMPL
CCB42 - 1	CCB42	263	0.0566	-	7471B	PPB	08 Oct 2022 16:02:53	U	SMPL
N5014-12 - 1	SB-10-2.0-3.5	782	0.1471	-	7471B	PPB	08 Oct 2022 16:05:10	U	SMPL
N5014-13 - 1	SB-01-0-2.0	1943	0.3497	-	7471B	PPB	08 Oct 2022 16:07:26	U	SMPL
N5014-14 - 1	SB-02-0-2.0	943	0.1752	-	7471B	PPB	08 Oct 2022 16:09:42	U	SMPL
N5014-15 - 1	SB-03-0-2.0	6169	1.0870	-	7471B	PPB	08 Oct 2022 16:11:57	U	SMPL
N5020-01 - 1	TR-5-100522	1345	0.2454	-	7471B	PPB	08 Oct 2022 16:14:13	U	SMPL
PB148203BL - 1	PBS203	318	0.0662	-	7471B	PPB	08 Oct 2022 16:16:30	U	SMPL
PB148203BS - 1	LCS203	20036	3.5063	-	7471B	PPB	08 Oct 2022 16:18:47	U	SMPL
N5018-01DUP - 1	SASP2-T-3-(0-6)DUP	12144	2.1294	-	7471B	PPB	08 Oct 2022 16:21:03	U	SMPL
N5018-01MS - 1	SASP2-T-3-(0-6)MS	31216	5.4568	-	7471B	PPB	08 Oct 2022 16:23:23	U	SMPL
CCV43 - 1	CCV43	26663	4.6624	-	7471B	PPB	08 Oct 2022 16:25:43	U	SMPL
CCB43 - 1	CCB43	-235	-0.0303	-	7471B	PPB	08 Oct 2022 16:28:01	U	SMPL
N5018-01MSD - 1	SASP2-T-3-(0-6)MSD	31519	5.5096	-	7471B	PPB	08 Oct 2022 16:30:19	U	SMPL
N5018-02 - 1	SASP2-T-3-(5-10)	1299	0.2373	-	7471B	PPB	08 Oct 2022 16:32:37	U	SMPL
N5018-03 - 1	SASP2-T-3-(10-14)	429	0.0855	-	7471B	PPB	08 Oct 2022 16:34:53	U	SMPL
N5018-04 - 1	SASP2-T-3-(14-16)	287	0.0608	-	7471B	PPB	08 Oct 2022 16:37:11	U	SMPL
N5042-01 - 1	EOR-0655	62	0.0215	-	7471B	PPB	08 Oct 2022 16:39:26	U	SMPL
N5046-01 - 1	R-1	5277	0.9313	-	7471B	PPB	08 Oct 2022 16:41:42	U	SMPL
N5046-02 - 1	R-2	1532	0.2780	-	7471B	PPB	08 Oct 2022 16:43:59	U	SMPL
N5046-03 - 1	R-3	2123	0.3811	-	7471B	PPB	08 Oct 2022 16:46:15	U	SMPL
N5046-04 - 1	R-4	1152	0.2117	-	7471B	PPB	08 Oct 2022 16:48:32	U	SMPL
N5046-05 - 1	R-5	584	0.1126	-	7471B	PPB	08 Oct 2022 16:50:49	U	SMPL
CCV44 - 1	CCV44	27960	4.8887	-	7471B	PPB	08 Oct 2022 16:53:05	U	SMPL
CCB44 - 1	CCB44	213	0.0479	-	7471B	PPB	08 Oct 2022 16:55:21	U	SMPL
N5046-06 - 1	R-6	1319	0.2408	-	7471B	PPB	08 Oct 2022 16:57:37	U	SMPL
N5046-07 - 1	R-7	672	0.1279	-	7471B	PPB	08 Oct 2022 16:59:55	U	SMPL
N5046-08 - 1	R-8	1680	0.3038	-	7471B	PPB	08 Oct 2022 17:02:11	U	SMPL
N5046-09 - 1	R-9	821	0.1539	-	7471B	PPB	08 Oct 2022 17:04:26	U	SMPL
N5046-10 - 1	R-10	718	0.1360	-	7471B	PPB	08 Oct 2022 17:06:42	U	SMPL
N5046-11 - 1	R-11	604	0.1161	-	7471B	PPB	08 Oct 2022 17:08:58	U	SMPL
N5046-12 - 1	R-12	1286	0.2351	-	7471B	PPB	08 Oct 2022 17:11:14	U	SMPL
N5046-13 - 1	R-13	774	0.1457	-	7471B	PPB	08 Oct 2022 17:13:30	U	SMPL
N5047-01 - 1	OR-3-100622	818	0.1534	-	7471B	PPB	08 Oct 2022 17:15:48	U	SMPL
CCV45 - 1	CCV45	27537	4.8149	-	7471B	PPB	08 Oct 2022 17:18:05	U	SMPL
CCB45 - 1	CCB45	242	0.0529	-	7471B	PPB	08 Oct 2022 17:20:21	U	SMPL
N5014-03LX5 - 1	SB-05-2.0-3.0L	495	0.0971	-	7471B	PPB	08 Oct 2022 17:22:37	U	SMPL
N5014-03A - 1	SB-05-2.0-3.0A	25336	4.4309	-	7471B	PPB	08 Oct 2022 17:24:55	U	SMPL
N5018-01DUP - 1	SASP2-T-3-(0-6)DUP	11584	2.0317	-	7471B	PPB	08 Oct 2022 17:27:12	U	SMPL
N5018-01LX5 - 1	SASP2-T-3-(0-6)LX5	2730	0.4870	-	7471B	PPB	08 Oct 2022 17:29:28	U	SMPL
N5018-01A - 1	SASP2-T-3-(0-6)A	30141	5.2692	-	7471B	PPB	08 Oct 2022 17:31:47	U	SMPL
CCV46 - 1	CCV46	28635	5.0065	-	7471B	PPB	08 Oct 2022 17:34:04	U	SMPL
CCB46 - 1	CCB46	184	0.0428	-	7471B	PPB	08 Oct 2022 17:36:20	U	SMPL
				-	7471B	PPB	08 Oct 2022 17:38:39	U	SMPL