


7470A LB122441, INSTRUMENT ID:CV1, ANALYSIS DATE: 10/12/2022

OPERATOR: JASWAL

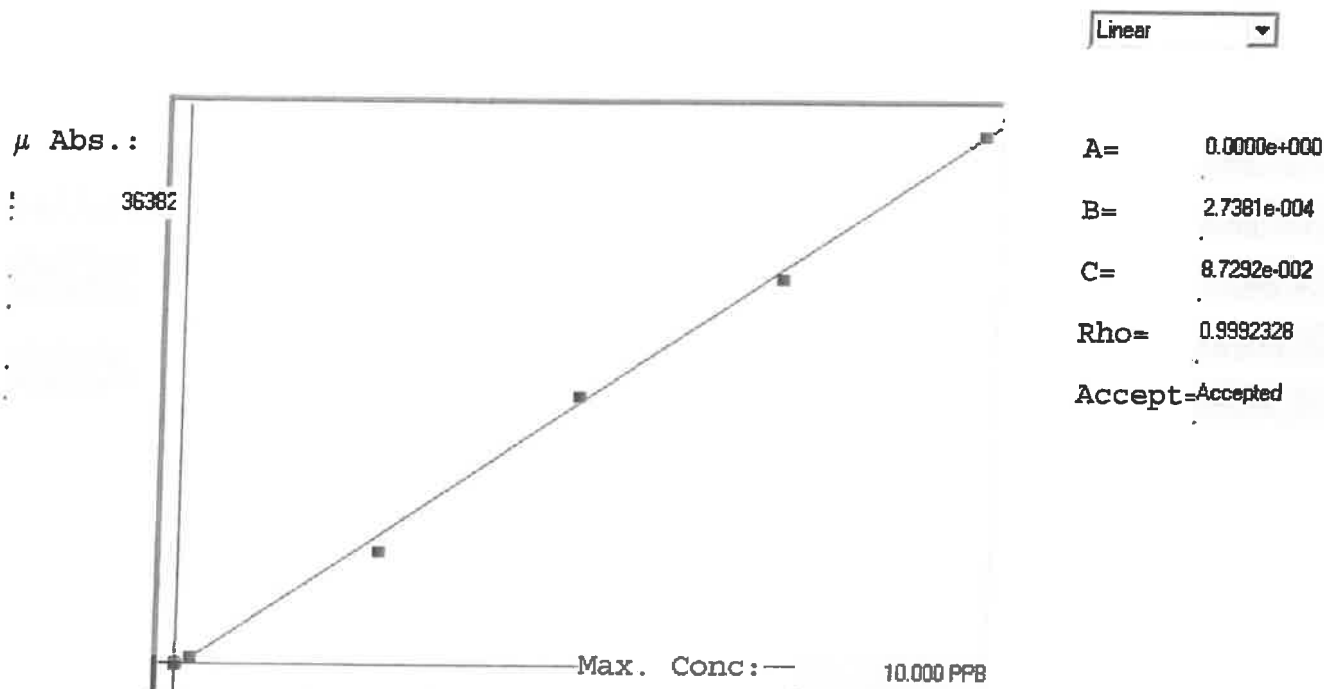

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	y.D
0.0	0.000	0.096	0.096	31	0.000	31					
0.2	0.200	0.252	0.052	600	0.0 %	600					26
2.5	2.500	2.242	-0.258	7870	0.0 %	7870					-10
5.0	5.000	5.177	0.177	18588	0.0 %	18588					4
7.5	7.500	7.385	-0.115	26651	0.0 %	26651					-2
10.0	10.000	10.049	0.049	36382	0.0 %	36382					-3

LB122441, INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Oct 2022 12:33:44

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30.0	31	-	0.000	7470A	PPB	12 Oct 2022 12:43:17	S	Std
0.2 - 1	30.2	600	-	0.200	7470A	PPB	12 Oct 2022 12:45:34	S	Std
2.5 - 1	52.5	7870	-	2.500	7470A	PPB	12 Oct 2022 12:47:51	S	Std
5.0 - 1	55.0	18588	-	5.000	7470A	PPB	12 Oct 2022 12:50:08	S	Std
7.5 - 1	57.5	26651	-	7.500	7470A	PPB	12 Oct 2022 12:52:24	S	Std
10.0 - 1	510.0	36382	-	10.000	7470A	PPB	12 Oct 2022 12:54:42	S	Std
ICV74 - 1	ICV74	13453	3.7708	-	7470A	PPB	12 Oct 2022 13:14:48	U	SMPL
ICB74 - 1	ICB74	-50	0.0736	-	7470A	PPB	12 Oct 2022 13:17:03	U	SMPL
CCV41 - 1	CCV41	19422	5.4052	-	7470A	PPB	12 Oct 2022 13:19:19	U	SMPL
CCB41 - 1	CCB41	-57	0.0717	-	7470A	PPB	12 Oct 2022 13:21:34	U	SMPL
CRA - 1	CRA	615	0.2557	-	7470A	PPB	12 Oct 2022 13:23:51	U	SMPL
HighStd - 1	HighStd	36661	10.1254	-	7470A	PPB	12 Oct 2022 13:26:06	U	SMPL
ChkStd - 1	ChkStd	25218	6.9922	-	7470A	PPB	12 Oct 2022 13:28:22	U	SMPL
PB148272BL - 1	PBW	-123	0.0536	-	7470A	PPB	12 Oct 2022 13:30:40	U	SMPL
PB148272BS - 1	LCSW	13107	3.6761	-	7470A	PPB	12 Oct 2022 13:35:54	U	SMPL
N5066-11 - 1	C11(10-11)	-96	0.0610	-	7470A	PPB	12 Oct 2022 13:38:10	U	SMPL
N5066-13 - 1	C12(11-12)	45	0.0996	-	7470A	PPB	12 Oct 2022 13:40:27	U	SMPL
N5066-14 - 1	C13(12-13)	40	0.0982	-	7470A	PPB	12 Oct 2022 13:42:45	U	SMPL
N5066-15 - 1	C14(13-14)	93	0.1128	-	7470A	PPB	12 Oct 2022 13:45:02	U	SMPL
N5066-17 - 1	C6(5-6)	121	0.1204	-	7470A	PPB	12 Oct 2022 13:47:18	U	SMPL
CCV42 - 1	CCV42	16409	4.5802	-	7470A	PPB	12 Oct 2022 13:49:34	U	SMPL
CCB42 - 1	CCB42	-56	0.0720	-	7470A	PPB	12 Oct 2022 13:51:49	U	SMPL
N5066-19 - 1	C20(19-20)	215	0.1462	-	7470A	PPB	12 Oct 2022 13:54:06	U	SMPL
N5066-20 - 1	C21(20-21)	42	0.0988	-	7470A	PPB	12 Oct 2022 13:56:21	U	SMPL
N5067-12 - 1	C22(21-22)	182	0.1371	-	7470A	PPB	12 Oct 2022 13:58:37	U	SMPL
N5067-13 - 1	C23(22-23)	137	0.1248	-	7470A	PPB	12 Oct 2022 14:00:53	U	SMPL
N5067-14 - 1	C24(23-24)	118	0.1196	-	7470A	PPB	12 Oct 2022 14:03:09	U	SMPL
N5067-15 - 1	C25(24-25)	74	0.1076	-	7470A	PPB	12 Oct 2022 14:05:26	U	SMPL
N5067-17 - 1	COMP-B-3-VERT	111	0.1177	-	7470A	PPB	12 Oct 2022 14:07:43	U	SMPL
N5067-19 - 1	COMP-B-2-VERT	58	0.1032	-	7470A	PPB	12 Oct 2022 14:10:00	U	SMPL
N5067-21 - 1	COMP-B-6-VERT	192	0.1399	-	7470A	PPB	12 Oct 2022 14:12:18	U	SMPL
N5078-02 - 1	ETGI-358	84	0.1103	-	7470A	PPB	12 Oct 2022 14:14:34	U	SMPL
CCV43 - 1	CCV43	16854	4.7021	-	7470A	PPB	12 Oct 2022 14:20:10	U	SMPL
CCB43 - 1	CCB43	-126	0.0528	-	7470A	PPB	12 Oct 2022 14:22:26	U	SMPL
N5078-02DUP - 1	ETGI-358DUP	54	0.1021	-	7470A	PPB	12 Oct 2022 14:24:43	U	SMPL
N5078-02MS - 1	ETGI-358MS	15845	4.4269	-	7470A	PPB	12 Oct 2022 14:26:59	U	SMPL
N5078-02MSD - 1	ETGI-358MSD	15889	4.4378	-	7470A	PPB	12 Oct 2022 14:29:15	U	SMPL
PB148301BL - 1	PBW	-93	0.0618	-	7470A	PPB	12 Oct 2022 14:31:33	U	SMPL
PB148301BS - 1	LCSW	15465	4.3218	-	7470A	PPB	12 Oct 2022 14:33:50	U	SMPL
N5082-02 - 1	FLORENCE-COMP-1-FLORENCE-VOC-1	-96	0.0610	-	7470A	PPB	12 Oct 2022 14:36:06	U	SMPL
N5082-04 - 1	FLORENCE-COMP-2-FLORENCE-VOC-2	-36	0.0774	-	7470A	PPB	12 Oct 2022 14:38:24	U	SMPL
N5083-02 - 1	MOUNT-LAUREL-COMP-1-MOUNT-LAUREL-VOC-1	2	0.0878	-	7470A	PPB	12 Oct 2022 14:40:41	U	SMPL
N5083-04 - 1	MOUNT-LAUREL-COMP-2-MOUNT-LAUREL-VOC-2	-43	0.0755	-	7470A	PPB	12 Oct 2022 14:42:59	U	SMPL
N5083-06 - 1	MOUNT-LAUREL-COMP-3-MOUNT-LAUREL-VOC-3	17	0.0919	-	7470A	PPB	12 Oct 2022 14:45:15	U	SMPL
CCV44 - 1	CCV44	19412	5.4025	-	7470A	PPB	12 Oct 2022 14:47:31	U	SMPL
CCB44 - 1	CCB44	-125	0.0531	-	7470A	PPB	12 Oct 2022 14:49:47	U	SMPL
N5083-08 - 1	MOUNT-LAUREL-COMP-4-MOUNT-LAUREL-VOC-4	-54	0.0725	-	7470A	PPB	12 Oct 2022 14:52:04	U	SMPL
N5093-01 - 1	D2732	-30	0.0791	-	7470A	PPB	12 Oct 2022 14:54:20	U	SMPL
N5093-02 - 1	COMP(D2736-D2734)	-20	0.0818	-	7470A	PPB	12 Oct 2022 14:56:37	U	SMPL
N5096-03 - 1	COMP(2690-2688)	-17	0.0826	-	7470A	PPB	12 Oct 2022 14:58:53	U	SMPL
N5096-04 - 1	2699	-23	0.0810	-	7470A	PPB	12 Oct 2022 15:01:10	U	SMPL
N5105-11 - 1	WC-7	4	0.0884	-	7470A	PPB	12 Oct 2022 15:03:27	U	SMPL
N5105-12 - 1	WC-6	9	0.0898	-	7470A	PPB	12 Oct 2022 15:05:44	U	SMPL
N5105-13 - 1	WC-5	76	0.1081	-	7470A	PPB	12 Oct 2022 15:08:01	U	SMPL
N5105-14 - 1	WC-4	20	0.0928	-	7470A	PPB	12 Oct 2022 15:10:18	U	SMPL
N5105-15 - 1	WC-2	45	0.1007	-	7470A	PPB	12 Oct 2022 15:12:35	U	SMPL
CCV45 - 1	CCV45	17262	4.8136	-	7470A	PPB	12 Oct 2022 15:14:51	U	SMPL
CCB45 - 1	CCB45	-142	0.0484	-	7470A	PPB	12 Oct 2022 15:17:06	U	SMPL
N5105-15DUP - 1	WC-2DUP	45	0.0996	-	7470A	PPB	12 Oct 2022 15:19:24	U	SMPL
N5105-15MS - 1	WC-2MS	15774	4.4064	-	7470A	PPB	12 Oct 2022 15:21:40	U	SMPL
N5105-15MSD - 1	WC-2MSD	15444	4.3160	-	7470A	PPB	12 Oct 2022 15:23:56	U	SMPL
PB148302BL - 1	PBW	-83	0.0646	-	7470A	PPB	12 Oct 2022 15:26:12	U	SMPL
PB148302BS - 1	LCSW	15083	4.2188	-	7470A	PPB	12 Oct 2022 15:28:29	U	SMPL
N5093-03 - 1	D2735	-54	0.0725	-	7470A	PPB	12 Oct 2022 15:30:47	U	SMPL
N5093-03DUP - 1	D2735DUP	-1	0.0870	-	7470A	PPB	12 Oct 2022 15:33:05	U	SMPL
N5093-03MS - 1	D2735MS	14721	4.1180	-	7470A	PPB	12 Oct 2022 15:35:22	U	SMPL
N5093-03MSD - 1	D2735MSD	14463	4.0474	-	7470A	PPB	12 Oct 2022 15:37:40	U	SMPL
N5093-04 - 1	COMP(D2724-D2723-D2722)	-55	0.0722	-	7470A	PPB	12 Oct 2022 15:39:57	U	SMPL
CCV46 - 1	CCV46	16168	4.5137	-	7470A	PPB	12 Oct 2022 15:42:15	U	SMPL
CCB46 - 1	CCB46	-78	0.0659	-	7470A	PPB	12 Oct 2022 15:44:32	U	SMPL
N5096-05 - 1	COMP(2692-2691)	2	0.0875	-	7470A	PPB	12 Oct 2022 15:46:50	U	SMPL
N5096-06 - 1	2673	0	0.0873	-	7470A	PPB	12 Oct 2022 15:49:06	U	SMPL
N5096-07 - 1	2693	180	0.1366	-	7470A	PPB	12 Oct 2022 15:51:23	U	SMPL
N5078-02LX5 - 1	ETGI-358L	-8	0.0851	-	7470A	PPB	12 Oct 2022 15:53:38	U	SMPL
N5078-02A - 1	ETGI-358A	15588	4.3554	-	7470A	PPB	12 Oct 2022 15:55:56	U	SMPL
PB148254TB - 1	LEB254	-73	0.0668	-	7470A	PPB	12 Oct 2022 15:58:13	U	SMPL
N5105-15LX5 - 1	WC-2L	-23	0.0810	-	7470A	PPB	12 Oct 2022 16:00:31	U	SMPL
N5105-15A - 1	WC-2A	15126	4.2289	-	7470A	PPB	12 Oct 2022 16:02:49	U	SMPL
PB148273TB - 1	LEB273	-61	0.0706	-	7470A	PPB	12 Oct 2022 16:05:07	U	SMPL
N5093-03LX5 - 1	D2736L	-28	0.0796	-	7470A	PPB	12 Oct 2022 16:07:26	U	SMPL
CCV47 - 1	CCV47	17019	4.7473	-	7470A	PPB	12 Oct 2022 16:09:42	U	SMPL
CCB47 - 1	CCB47	-77	0.0662	-	7470A	PPB	12 Oct 2022 16:11:59	U	SMPL
N5093-03A - 1	D2735A	14068	3.9392	-	7470A	PPB	12 Oct 2022 16:14:18	U	SMPL
PB148274TB - 1	LEB274	-56	0.0720	-	7470A	PPB	12 Oct 2022 16:16:35	U	SMPL
CCV48 - 1	CCV48	17287	4.8206	-	7470A	PPB	12 Oct 2022 16:23:53	U	SMPL
CCB48 - 1	CCB48	-116	0.0555	-	7470A	PPB	12 Oct 2022 16:26:09	U	SMPL