


7471B LB122449, INSTRUMENT ID: CV1, ANALYSIS DATE : 10/12/2022

OPERATOR: JASWAL

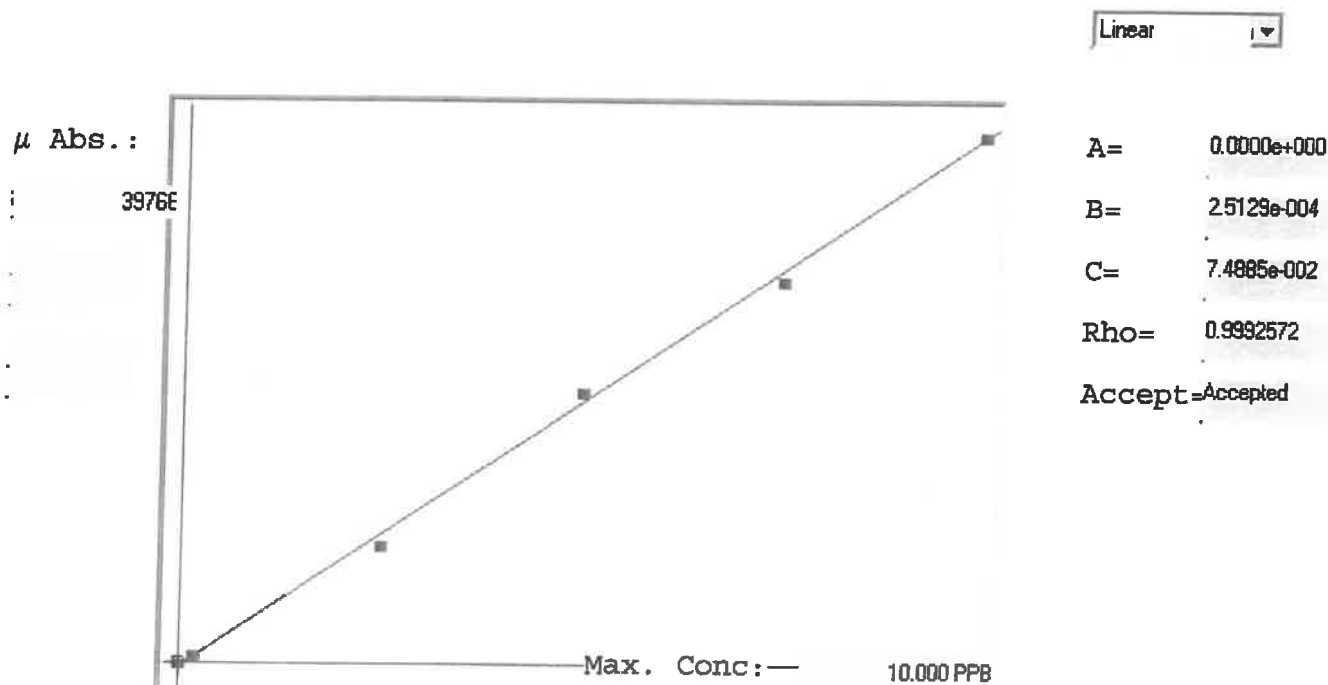

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.070	0.070	-18	0.000	-18					
0.2	0.200	0.223	0.023	588	0.0 %	588					12
2.5	2.500	2.315	-0.185	8916	0.0 %	8916					-7
5.0	5.000	5.208	0.208	20428	0.0 %	20428					4
7.5	7.500	7.316	-0.184	28816	0.0 %	28816					-2
10.0	10.000	10.068	0.068	39766	0.0 %	39766					7

LB122449, INSTRUMENT ID: CV1

Method: 7471B

Operator: Admin

Date of Analysis: 12 Oct 2022 18:29:57

Sample ID	Extended ID	μ Abs	Conc	Strd Conc	Method	Units	Date	Type	Type
0.0 - 1	5.0	-18	-	0.000	7471B	PPB	12 Oct 2022 18:30:19	S	Std
0.2 - 1	5.2	588	-	0.200	7471B	PPB	12 Oct 2022 18:32:37	S	Std
2.5 - 1	5.2.5	8916	-	2.500	7471B	PPB	12 Oct 2022 18:34:54	S	Std
5.0 - 1	5.5	20428	-	5.000	7471B	PPB	12 Oct 2022 18:37:11	S	Std
7.5 - 1	5.7.5	28816	-	7.500	7471B	PPB	12 Oct 2022 18:39:28	S	Std
10.0 - 1	5.10.0	39766	-	10.000	7471B	PPB	12 Oct 2022 18:41:45	S	Std
ICV75 - 1	ICV75	15245	3.9057	-	7471B	PPB	12 Oct 2022 18:44:38	U	SMPL
ICB75 - 1	ICB75	-102	0.0483	-	7471B	PPB	12 Oct 2022 18:46:53	U	SMPL
CCV49 - 1	CCV49	19244	4.9106	-	7471B	PPB	12 Oct 2022 18:52:39	U	SMPL
CCB49 - 1	CCB49	-126	0.0432	-	7471B	PPB	12 Oct 2022 18:54:54	U	SMPL
CRA - 1	CRA	642	0.2362	-	7471B	PPB	12 Oct 2022 18:57:10	U	SMPL
HighStd - 1	HighStd	40668	10.2942	-	7471B	PPB	12 Oct 2022 18:59:26	U	SMPL
ChkStd - 1	ChkStd	29158	7.4019	-	7471B	PPB	12 Oct 2022 19:01:41	U	SMPL
PB148303BL - 1	PB148303BL	149	0.1123	-	7471B	PPB	12 Oct 2022 19:03:59	U	SMPL
PB148303BS - 1	PB148303BS	15094	3.8678	-	7471B	PPB	12 Oct 2022 19:06:17	U	SMPL
N5067-16 - 1	COMP-B-3-VERT	23179	5.8994	-	7471B	PPB	12 Oct 2022 19:08:34	U	SMPL
N5067-18 - 1	COMP-B-2-VERT	54094	13.6680	-	7471B	PPB	12 Oct 2022 19:10:51	U	SMPL
N5067-20 - 1	COMP-B-6-VERT	135604	34.1503	-	7471B	PPB	12 Oct 2022 19:13:11	U	SMPL
N5080-01 - 1	TR-6-101022	549	0.2128	-	7471B	PPB	12 Oct 2022 19:15:31	U	SMPL
N5082-01 - 1	FLORENCE-COMP-1-FLORENCE-VOC-1	1026	0.3327	-	7471B	PPB	12 Oct 2022 19:23:43	U	SMPL
CCV50 - 1	CCV50	19014	4.8528	-	7471B	PPB	12 Oct 2022 19:25:58	U	SMPL
CCB50 - 1	CCB50	-95	0.0510	-	7471B	PPB	12 Oct 2022 19:28:13	U	SMPL
N5082-03 - 1	FLORENCE-COMP-2-FLORENCE-VOC-2	1011	0.3289	-	7471B	PPB	12 Oct 2022 19:30:30	U	SMPL
N5083-01 - 1	MOUNT-LAUREL-COMP-1-MOUNT-LAUREL-VOC-1	695	0.2495	-	7471B	PPB	12 Oct 2022 19:32:46	U	SMPL
N5083-03 - 1	MOUNT-LAUREL-COMP-2-MOUNT-LAUREL-VOC-2	2844	0.7895	-	7471B	PPB	12 Oct 2022 19:35:02	U	SMPL
N5083-05 - 1	MOUNT-LAUREL-COMP-3-MOUNT-LAUREL-VOC-3	1362	0.4171	-	7471B	PPB	12 Oct 2022 19:37:18	U	SMPL
N5083-07 - 1	MOUNT-LAUREL-COMP-4-MOUNT-LAUREL-VOC-4	1041	0.3365	-	7471B	PPB	12 Oct 2022 19:39:34	U	SMPL
N5087-01 - 1	5922	557	0.2149	-	7471B	PPB	12 Oct 2022 19:41:51	U	SMPL
N5096-01 - 1	VNJ-217	1251	0.3892	-	7471B	PPB	12 Oct 2022 19:44:07	U	SMPL
N5101-01 - 1	OK-2-101122	19783	5.0461	-	7471B	PPB	12 Oct 2022 19:46:24	U	SMPL
N5102-01 - 1	CL-1-101122	3142	0.8644	-	7471B	PPB	12 Oct 2022 19:48:41	U	SMPL
N5104-01 - 1	PL-01-101122	2778	0.7730	-	7471B	PPB	12 Oct 2022 19:50:58	U	SMPL
CCV51 - 1	CCV51	19455	4.9637	-	7471B	PPB	12 Oct 2022 19:53:14	U	SMPL
CCB51 - 1	CCB51	-79	0.0550	-	7471B	PPB	12 Oct 2022 19:55:29	U	SMPL
N5104-01DUP - 1	PL-01-101122DUP	2671	0.7461	-	7471B	PPB	12 Oct 2022 19:57:46	U	SMPL
N5104-01MS - 1	PL-01-101122MS	15523	3.9756	-	7471B	PPB	12 Oct 2022 20:00:05	U	SMPL
N5104-01MSD - 1	PL-01-101122MSD	15572	3.9879	-	7471B	PPB	12 Oct 2022 20:02:21	U	SMPL
N5105-01 - 1	WC-7	375	0.1691	-	7471B	PPB	12 Oct 2022 20:04:39	U	SMPL
N5105-03 - 1	WC-6	1318	0.4081	-	7471B	PPB	12 Oct 2022 20:06:56	U	SMPL
N5105-05 - 1	WC-5	679	0.2455	-	7471B	PPB	12 Oct 2022 20:09:13	U	SMPL
N5105-07 - 1	WC-4	215	0.1289	-	7471B	PPB	12 Oct 2022 20:11:29	U	SMPL
N5105-09 - 1	WC-2	1460	0.4418	-	7471B	PPB	12 Oct 2022 20:13:46	U	SMPL
N5104-01LX5 - 1	PL-01-101122LX5	448	0.1875	-	7471B	PPB	12 Oct 2022 20:16:03	U	SMPL
N5104-01A - 1	PL-01-101122A	16364	4.1869	-	7471B	PPB	12 Oct 2022 20:18:19	U	SMPL
CCV52 - 1	CCV52	18489	4.7209	-	7471B	PPB	12 Oct 2022 20:23:19	U	SMPL
CCB52 - 1	CCB52	-134	0.0412	-	7471B	PPB	12 Oct 2022 20:25:35	U	SMPL
N5067-18DLX5 - 1		10369	2.6803	-	7471B	PPB	12 Oct 2022 20:27:53	U	SMPL
N5067-20DLX10 - 1		16298	4.1703	-	7471B	PPB	12 Oct 2022 20:30:09	U	SMPL
CCV53 - 1	CCV53	18752	4.7870	-	7471B	PPB	12 Oct 2022 20:32:26	U	SMPL
CCB53 - 1	CCB53	-140	0.0397	-	7471B	PPB	12 Oct 2022 20:34:44	U	SMPL