


7471B LB122471, INSTRUMENT ID:CV1, ANALYSIS DATE: 10/13/2022

OPERATOR : JASWAL

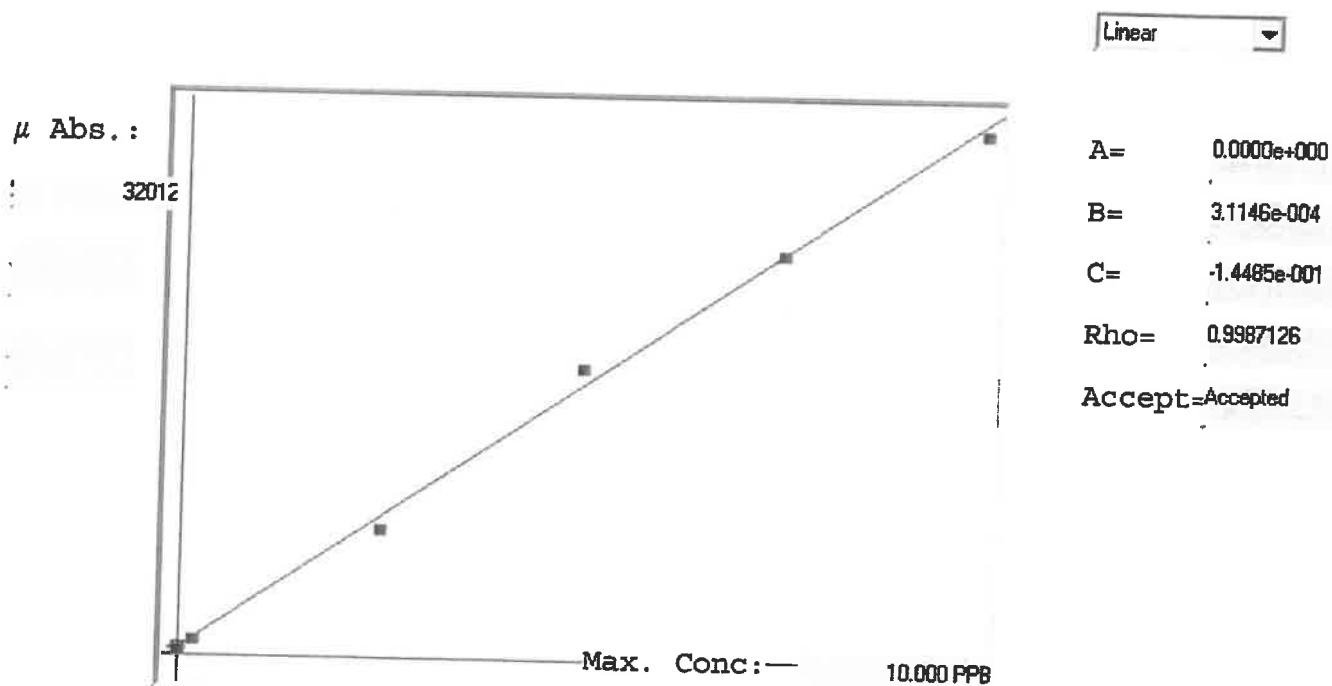

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Σ
0.0	0.000	0.004	0.004	478	0.000	478					478
0.2	0.200	0.185	-0.015	1059	0.0 %	1059					-8
2.5	2.500	2.288	-0.212	7811	0.0 %	7811					-8
5.0	5.000	5.365	0.365	17692	0.0 %	17692					7
7.5	7.500	7.532	0.032	24648	0.0 %	24648					4
10.0	10.000	9.826	-0.174	32012	0.0 %	32012					-2

LB122471, INSTRUMENT ID: CV1

Method: 7471B

Operator: Admin

Date of Analysis: 13 Oct 2022 19:28:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30.0	478	-	0.0000	7471B	PPB	13 Oct 2022 19:28:27	S	Std
0.2 - 1	30.2	1059	-	0.2000	7471B	PPB	13 Oct 2022 19:30:45	S	Std
2.5 - 1	32.5	7811	-	2.5000	7471B	PPB	13 Oct 2022 19:33:02	S	Std
5.0 - 1	35.0	17692	-	5.0000	7471B	PPB	13 Oct 2022 19:35:19	S	Std
7.5 - 1	37.5	24648	-	7.5000	7471B	PPB	13 Oct 2022 19:37:38	S	Std
10.0 - 1	310.0	32012	-	10.0000	7471B	PPB	13 Oct 2022 19:39:56	S	Std
ICV77 - 1	ICV77	12908	3.8755	-	7471B	PPB	13 Oct 2022 19:44:26	U	SMPL
ICB77 - 1	ICB77	507	0.0131	-	7471B	PPB	13 Oct 2022 19:46:41	U	SMPL
CCV59 - 1	CCV59	17192	5.2097	-	7471B	PPB	13 Oct 2022 19:48:59	U	SMPL
CCB59 - 1	CCB59	317	-0.0461	-	7471B	PPB	13 Oct 2022 19:51:13	U	SMPL
CRA - 1	CRA	1030	0.1760	-	7471B	PPB	13 Oct 2022 19:53:31	U	SMPL
HighStd - 1	HighStd	31573	9.6888	-	7471B	PPB	13 Oct 2022 19:55:46	U	SMPL
ChkStd - 1	ChkStd	23717	7.2420	-	7471B	PPB	13 Oct 2022 19:58:01	U	SMPL
PB148320BL - 1	PBS	79	-0.1202	-	7471B	PPB	13 Oct 2022 20:00:26	U	SMPL
PB148320BS - 1	LCSS	12534	3.7590	-	7471B	PPB	13 Oct 2022 20:02:44	U	SMPL
N5066-12 - 1	C11(10-11)	23249	7.0963	-	7471B	PPB	13 Oct 2022 20:05:01	U	SMPL
N5108-01 - 1	OR-2-101222	849	0.1196	-	7471B	PPB	13 Oct 2022 20:07:19	U	SMPL
N5111-01 - 1	WC-3	1011	0.1700	-	7471B	PPB	13 Oct 2022 20:09:49	U	SMPL
N5111-01DUP - 1	WC-3DUP	757	0.0909	-	7471B	PPB	13 Oct 2022 20:12:07	U	SMPL
N5111-01MS - 1	WC-3MS	6921	2.0108	-	7471B	PPB	13 Oct 2022 20:14:22	U	SMPL
CCV60 - 1	CCV60	17996	5.4602	-	7471B	PPB	13 Oct 2022 20:22:10	U	SMPL
CCB60 - 1	CCB60	169	-0.0922	-	7471B	PPB	13 Oct 2022 20:24:26	U	SMPL
N5111-01MSD - 1	WC-3MSD	6878	1.9974	-	7471B	PPB	13 Oct 2022 20:26:44	U	SMPL
N5114-01 - 1	31266	334	-0.0408	-	7471B	PPB	13 Oct 2022 20:28:59	U	SMPL
N5114-02 - 1	FMC-0083	871	0.1264	-	7471B	PPB	13 Oct 2022 20:31:19	U	SMPL
N5114-03 - 1	FMC-0080	913	0.1395	-	7471B	PPB	13 Oct 2022 20:33:35	U	SMPL
N5114-04 - 1	FMC-0095	795	0.1028	-	7471B	PPB	13 Oct 2022 20:35:51	U	SMPL
N5116-01 - 1	SWRN-30977	1553	0.3388	-	7471B	PPB	13 Oct 2022 20:38:07	U	SMPL
N5118-01 - 1	SU-2-101222	2017	0.4834	-	7471B	PPB	13 Oct 2022 20:40:23	U	SMPL
N5118-03 - 1	SU-4-101222	1784	0.4108	-	7471B	PPB	13 Oct 2022 20:42:40	U	SMPL
N5123-01 - 1	HR-2-101222	2569	0.6553	-	7471B	PPB	13 Oct 2022 20:44:59	U	SMPL
CCV61 - 1	CCV61	15460	4.6703	-	7471B	PPB	13 Oct 2022 21:01:27	U	SMPL
CCB61 - 1	CCB61	355	-0.0343	-	7471B	PPB	13 Oct 2022 21:03:42	U	SMPL
N5111-01LX5 - 1	WC-3L	588	0.0383	-	7471B	PPB	13 Oct 2022 21:06:01	U	SMPL
N5111-01A - 1	WC-3A	11891	3.5587	-	7471B	PPB	13 Oct 2022 21:08:16	U	SMPL
CCV62 - 1	CCV62	16990	5.1468	-	7471B	PPB	13 Oct 2022 21:17:15	U	SMPL
CCB62 - 1	CCB62	208	-0.0801	-	7471B	PPB	13 Oct 2022 21:19:30	U	SMPL