


SFAM01.1 LB122492, INSTRUMENT ID:CV1, DATE OF ANALYSIS:10/16/2022

OPERATOR : JASWAL

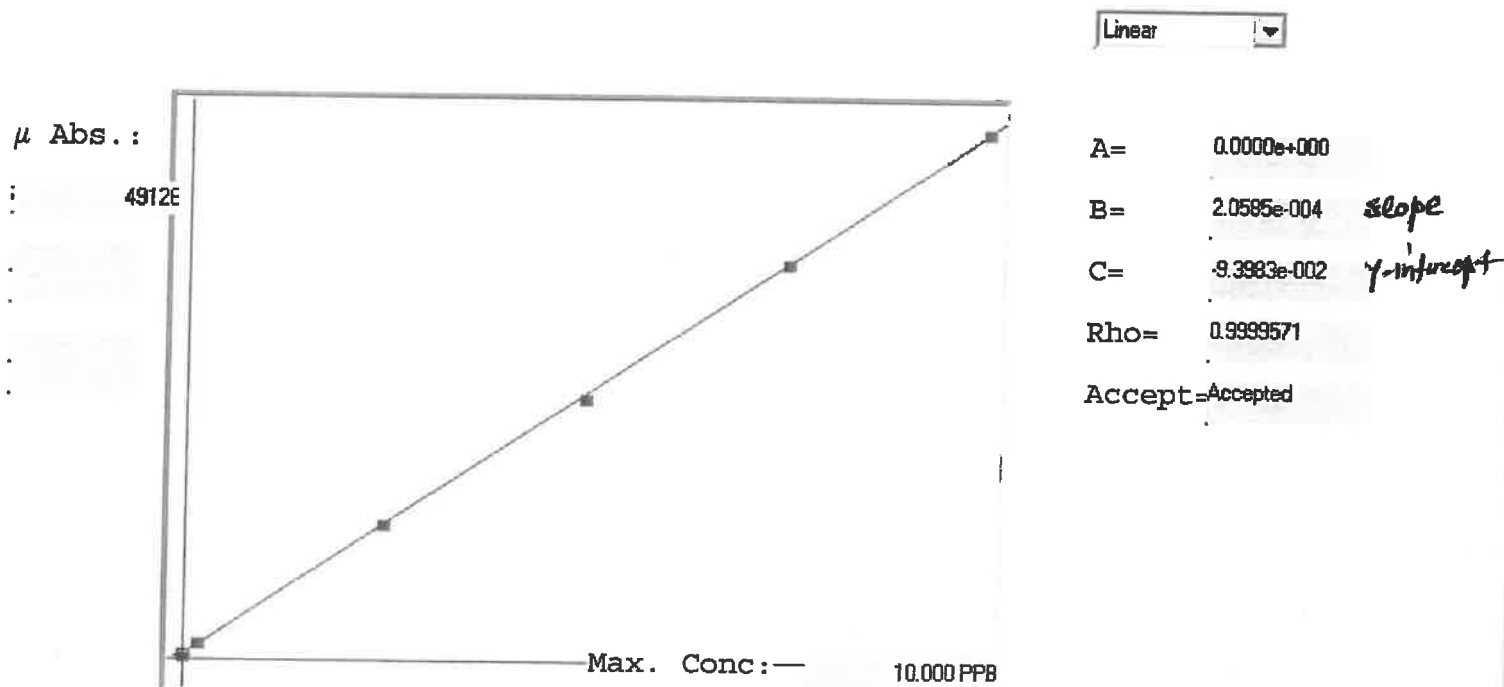

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.006	0.006	487	0.000	487					
0.05	0.050					185					
0.20	0.200	0.226	0.026	1556	0.0 %	1556	0				
2.50	2.500	2.500	-0.000	12600	0.0 %	12600					13
5.00	5.000	4.926	-0.074	24388	0.0 %	24388					0
7.50	7.500	7.523	0.023	37000	0.0 %	37000					-2
10.0	10.000	10.019	0.019	49126	0.0 %	49126					0

Sample ID	Extended μ	Abs. Conc.	Std Conc	Method	Units	Date	Type
0.00 - 1		487 -		0 SFAM01.1	PPB	10/16/2022 21:15	Std
0.20 - 1		1556 -		0.2 SFAM01.1	PPB	10/16/2022 21:18	Std
2.50 - 1		12600 -		2.5 SFAM01.1	PPB	10/16/2022 21:20	Std
5.00 - 1		24388 -		5 SFAM01.1	PPB	10/16/2022 21:22	Std
7.50 - 1		37000 -		7.5 SFAM01.1	PPB	10/16/2022 21:24	Std
10.0 - 1		49126 -		10 SFAM01.1	PPB	10/16/2022 21:27	Std
ICV80 - 1	ICV80	20315 4.0879 -		SFAM01.1	PPB	10/16/2022 21:34	SMPL
ICB80 - 1	ICB80	448 -0.0018 -		SFAM01.1	PPB	10/16/2022 21:37	SMPL
CCV004 - 1	CCV004	24200 4.8877 -		SFAM01.1	PPB	10/16/2022 21:39	SMPL
CCB004 - 1	CCB004	369 -0.018 -		SFAM01.1	PPB	10/16/2022 21:41	SMPL
PB148374BL - 1	PBW374	482 0.0052 -		SFAM01.1	PPB	10/16/2022 21:43	SMPL
N5084-01 - 1	EYB33	462 0.0011 -		SFAM01.1	PPB	10/16/2022 21:46	SMPL
N5084-02 - 1	EYB35	1341 0.1821 -		SFAM01.1	PPB	10/16/2022 21:48	SMPL
N5084-03 - 1	EYB36	550 0.0192 -		SFAM01.1	PPB	10/16/2022 21:50	SMPL
N5084-04 - 1	EYB39	545 0.0182 -		SFAM01.1	PPB	10/16/2022 21:52	SMPL
N5084-05 - 1	EYBC4	764 0.0633 -		SFAM01.1	PPB	10/16/2022 21:55	SMPL
N5084-06 - 1	EYBC8	453 -0.0007 -		SFAM01.1	PPB	10/16/2022 21:57	SMPL
N5084-07 - 1	EYBF2	456 -0.0001 -		SFAM01.1	PPB	10/16/2022 21:59	SMPL
N5084-08 - 1	EYBF3	495 0.0079 -		SFAM01.1	PPB	10/16/2022 22:02	SMPL
N5084-09 - 1	EYBC8D	489 0.0067 -		SFAM01.1	PPB	10/16/2022 22:04	SMPL
N5084-10 - 1	EYBC8S	5957 1.1323 -		SFAM01.1	PPB	10/16/2022 22:06	SMPL
N5085-01 - 1	EYB41	454 -0.0005 -		SFAM01.1	PPB	10/16/2022 22:08	SMPL
N5085-02 - 1	EYB45	456 -0.0001 -		SFAM01.1	PPB	10/16/2022 22:11	SMPL
N5085-03 - 1	EYB451	493 0.0075 -		SFAM01.1	PPB	10/16/2022 22:13	SMPL
N5085-04 - 1	EYB48	381 -0.0156 -		SFAM01.1	PPB	10/16/2022 22:15	SMPL
N5085-05 - 1	EYBC5	405 -0.0106 -		SFAM01.1	PPB	10/16/2022 22:17	SMPL
N5085-06 - 1	EYBC9	419 -0.0077 -		SFAM01.1	PPB	10/16/2022 22:20	SMPL
N5085-07 - 1	EYBF5	440 -0.0034 -		SFAM01.1	PPB	10/16/2022 22:22	SMPL
N5085-08 - 1	EYBF6	421 -0.0073 -		SFAM01.1	PPB	10/16/2022 22:24	SMPL
N5085-09 - 1	EYBC9D	421 -0.0073 -		SFAM01.1	PPB	10/16/2022 22:26	SMPL
CCV005 - 1	CCV005	24363 4.9212 -		SFAM01.1	PPB	10/16/2022 22:29	SMPL
CCB005 - 1	CCB005	395 -0.0127 -		SFAM01.1	PPB	10/16/2022 22:31	SMPL
N5085-10 - 1	EYBC9S	5796 1.0991 -		SFAM01.1	PPB	10/16/2022 22:33	SMPL
CCV006 - 1	CCV006	24287 4.9056 -		SFAM01.1	PPB	10/16/2022 22:36	SMPL
CCB006 - 1	CCB006	405 -0.0106 -		SFAM01.1	PPB	10/16/2022 22:38	SMPL