

Clear table

Instrument ID: IC-2										Analyst : IZ		Method: 300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2022-10-17_	10/17/22 11:14		IZ/MA		
STD2	0.4600	0.6690	0.6790	2.2670	0.5710	0.8860	3.5320	_2022-10-17_	10/17/22 11:45		IZ/MA		
STD3	0.7820	1.2190	1.2070	4.0270	1.0100	1.9680	6.0830	_2022-10-17_	10/17/22 12:15		IZ/MA		
STD4	0.9840	1.4910	1.4960	5.0330	1.2510	2.5410	7.5010	_2022-10-17_	10/17/22 12:46		IZ/MA		
STD5	1.9760	2.9130	2.9080	9.6540	2.4100	5.1530	14.3160	_2022-10-17_	10/17/22 12:46		IZ/MA		
STD6	3.9490	5.9190	5.9200	19.6570	4.9220	10.0590	29.4430	_2022-10-17_	10/17/22 13:16		IZ/MA		
STD7	5.0500	7.5890	7.5900	25.3630	6.3370	12.3930	38.1240	_2022-10-17_	10/17/22 13:47		IZ/MA		
ICV	1.9220	2.9820	3.0440	9.9700	2.4890	4.7350	14.7470	_2022-10-17_	10/17/22 14:18		IZ/MA		
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2022-10-17_	10/17/22 15:53		IZ/MA		
CCV	1.8910	3.0100	2.9700	10.0530	2.4960	4.5040	14.9390	_2022-10-31_	10/17/22 16:24		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2022-10-31_	10/31/22 11:33		IZ/MA		
LB122709BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2022-10-31_	10/31/22 12:04		IZ/MA		
LB122709BSW	1.9310	3.0030	2.9360	10.0290	2.4910	4.5300	14.9580	_2022-10-31_	10/31/22 12:34		IZ/MA		
N5394-01	0.0000	0.0000	0.0000	0.0000	0.2880	0.0000	0.0000	_2022-10-31_	10/31/22 13:05		IZ/MA		
N5394-01MS	1.9000	2.8540	2.7920	9.4410	2.5050	4.4130	14.0610	_2022-10-31_	10/31/22 14:57		IZ/MA		
N5394-01MSD	1.8680	3.0430	2.9410	9.8290	2.6070	4.4610	14.6070	_2022-10-31_	10/31/22 15:28		IZ/MA		
CCV	1.9270	3.0300	3.0030	10.1170	2.5120	4.5110	14.9280	_2022-10-31_	10/31/22 15:59		IZ/MA		
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2022-10-31_	10/31/22 16:29		IZ/MA		
								2022-10-31	10/31/22 17:00		IZ/MA		

Report date: 11/1/2022 1:07:27 PM

Printed by: wet

Ident: CCV

Analysis from: 10/31/2022 11:33:27 AM

File: _2022-10-31_

Last save: 10/31/2022 12:01:27 PM

Method: AnionsIC2-101722.mtw

Last save: 10/27/2022 9:16

Run operator: wet

Analysis number: 32390

SAMPLE:


: IZ/MA

Vial number: 32

Volume: 20.0 µL

Dilution: 1.00

Amount: 1.0000

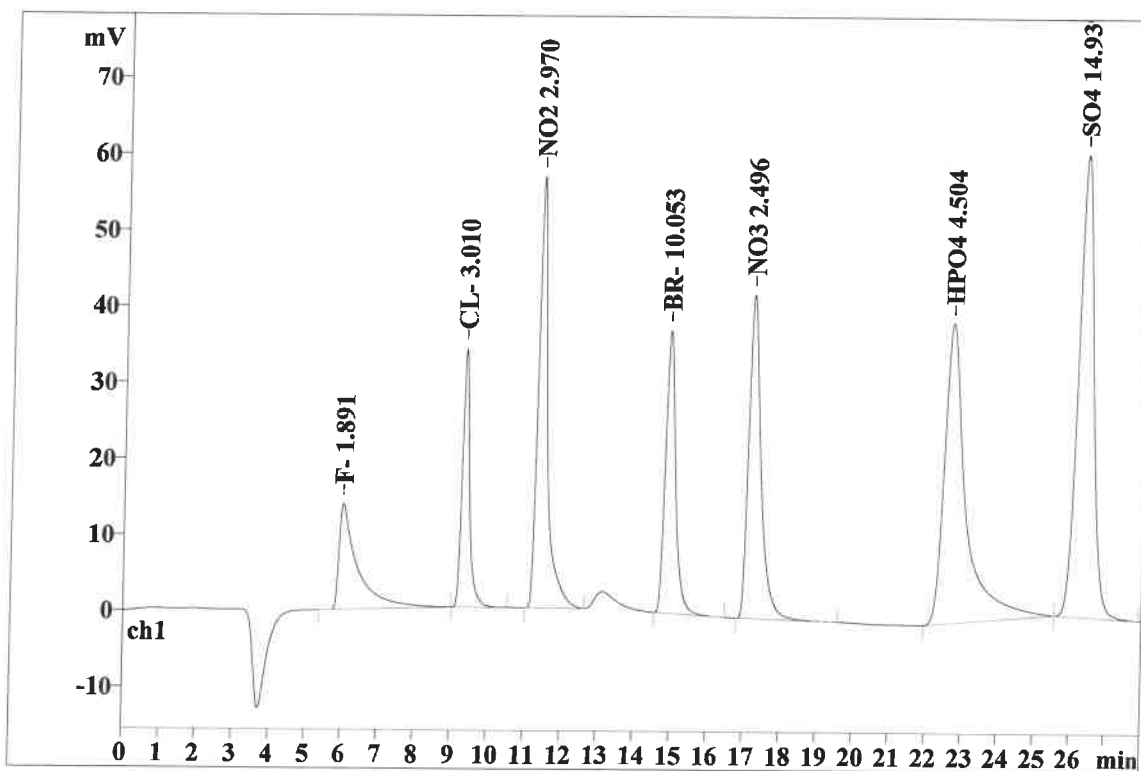

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.01	0.423	13.94	4.90	495.623	6.87
2	9.34	0.200	33.97	11.94	476.462	6.61
3	11.38	0.249	56.67	19.93	1043.064	14.47
4	14.91	0.281	37.14	13.06	710.319	9.85
5	17.18	0.341	42.50	14.95	1002.515	13.90
6	22.66	0.527	39.41	13.86	1642.920	22.79
7	26.33	0.461	60.74	21.36	1839.070	25.51
7	28.00	0.355	284.37	100.00	7209.972	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:07:34 PM
Printed by: wet


Ident: CCB
Analysis from: 10/31/2022 12:04:23 PM
File: _2022-10-31_

Last save: 10/31/2022 12:32:23 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32391

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

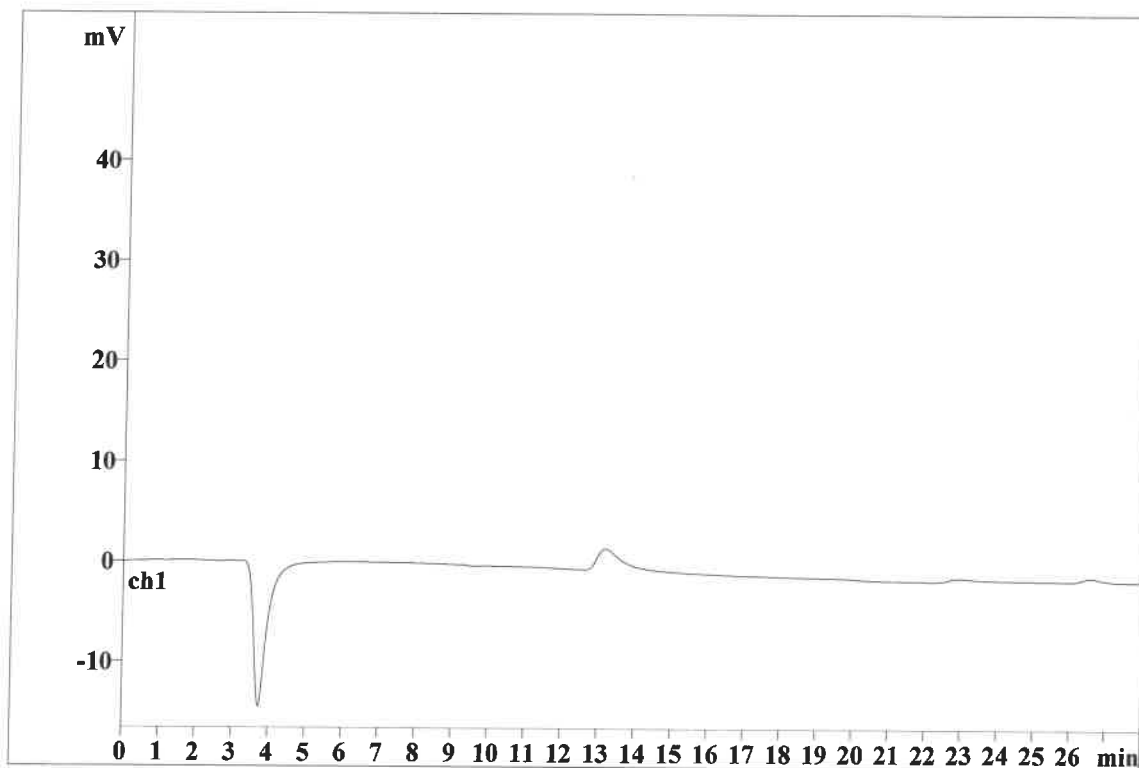

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:07:45 PM
Printed by: wet


Ident: LB122709BLW
Analysis from: 10/31/2022 12:34:58 PM
File: _2022-10-31_

Last save: 11/1/2022 12:25:02 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32392

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

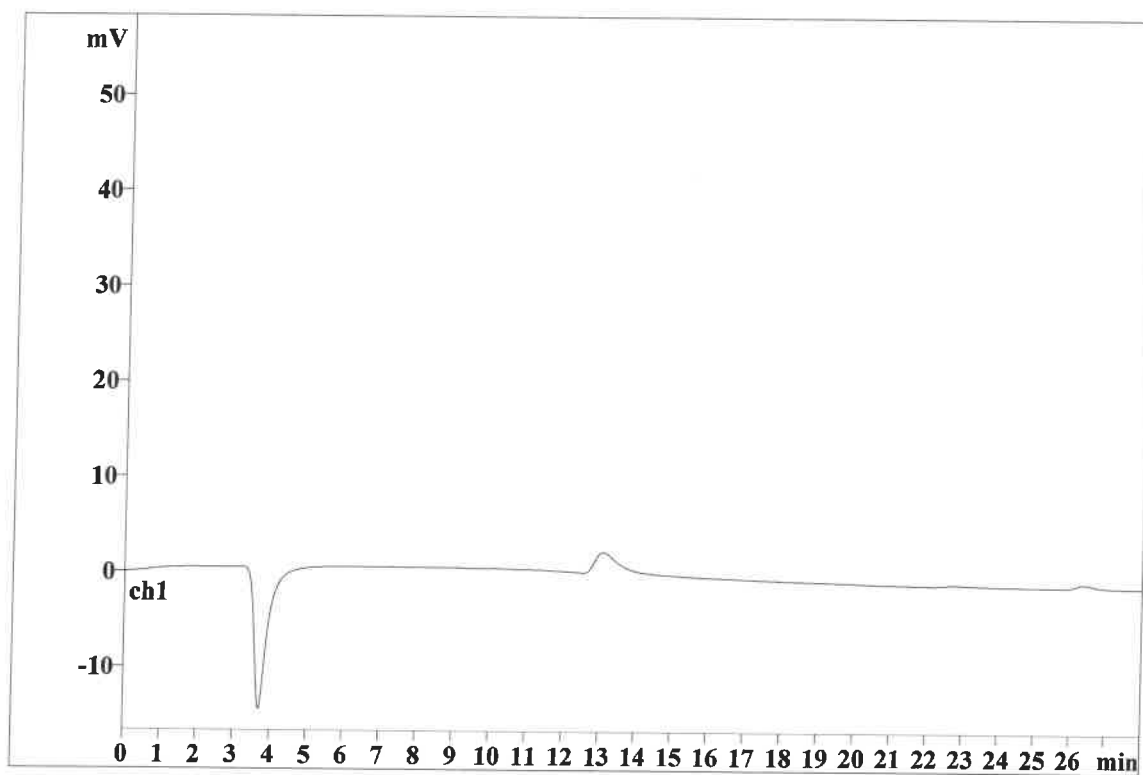

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:07:51 PM
Printed by: wet


Ident: LB122709BSW
Analysis from: 10/31/2022 1:05:43 PM
File: _2022-10-31_

Last save: 11/1/2022 12:25:02 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32393

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

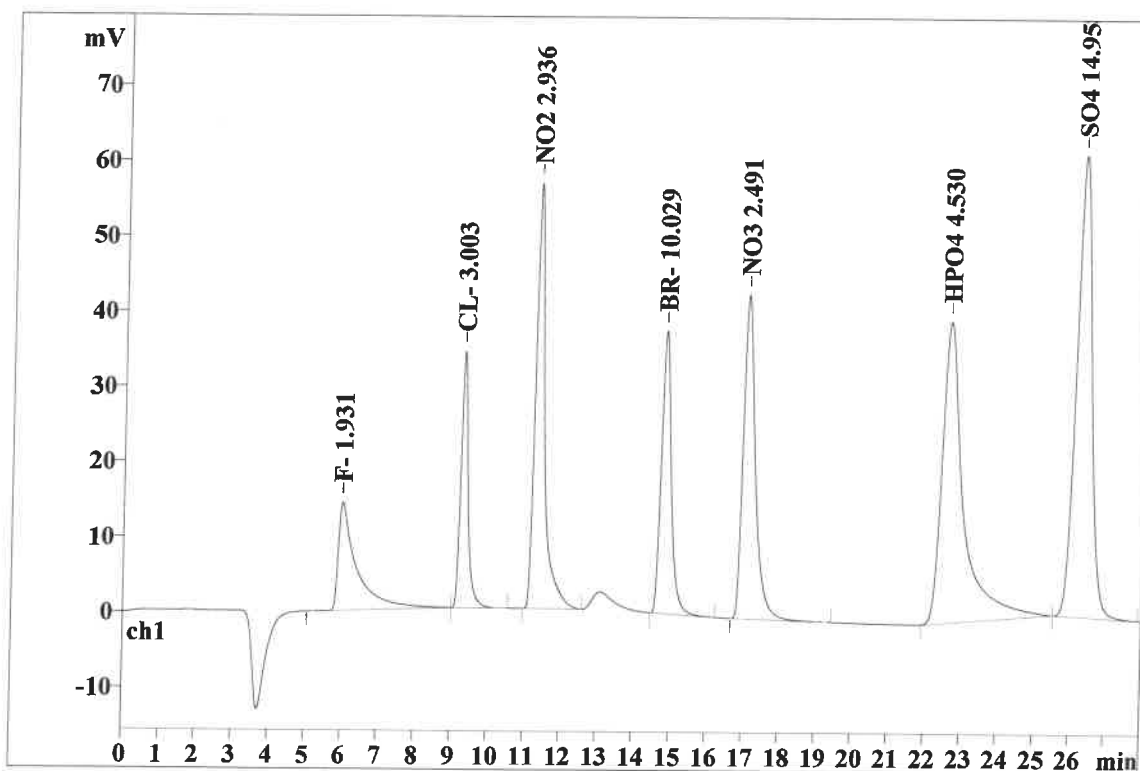

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.00	0.417	14.37	5.00	507.537	7.03
2	9.30	0.198	34.11	11.88	475.130	6.59
3	11.32	0.246	56.58	19.70	1030.349	14.28
4	14.81	0.277	37.61	13.10	708.497	9.82
5	17.06	0.335	43.10	15.01	1000.056	13.86
6	22.63	0.521	40.02	13.94	1651.847	22.89
7	26.29	0.458	61.39	21.38	1841.594	25.52
7	28.00	0.350	287.17	100.00	7215.010	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:08:18 PM
Printed by: wet


Ident: N5394-01
Analysis from: 10/31/2022 2:57:51 PM
File: _2022-10-31_

Last save: 10/31/2022 3:25:50 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32396

Last save: 10/27/2022 9:16

SAMPLE:
:
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

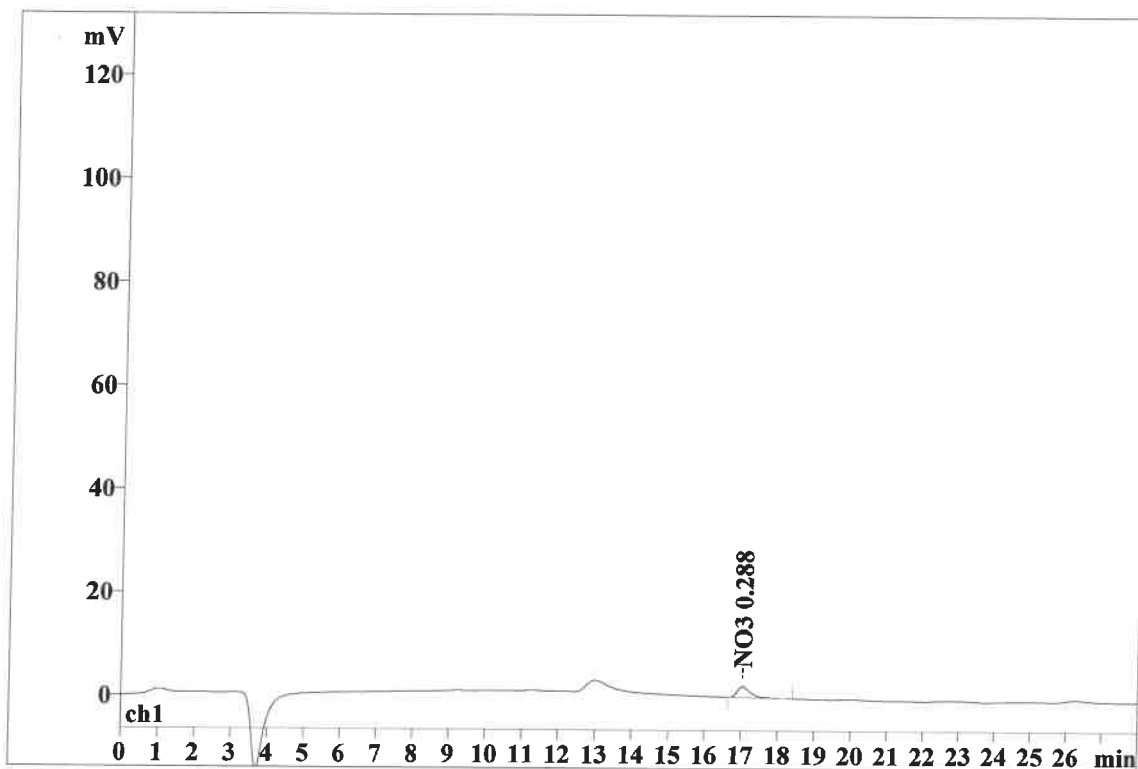

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.04	0.372	2.11	99.96	53.005	100.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.053	2.11	99.96	53.005	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:08:29 PM
Printed by: wet


Ident: N5394-01MS
Analysis from: 10/31/2022 3:28:26 PM
File: _2022-10-31_

Last save: 11/1/2022 12:25:22 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32397

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

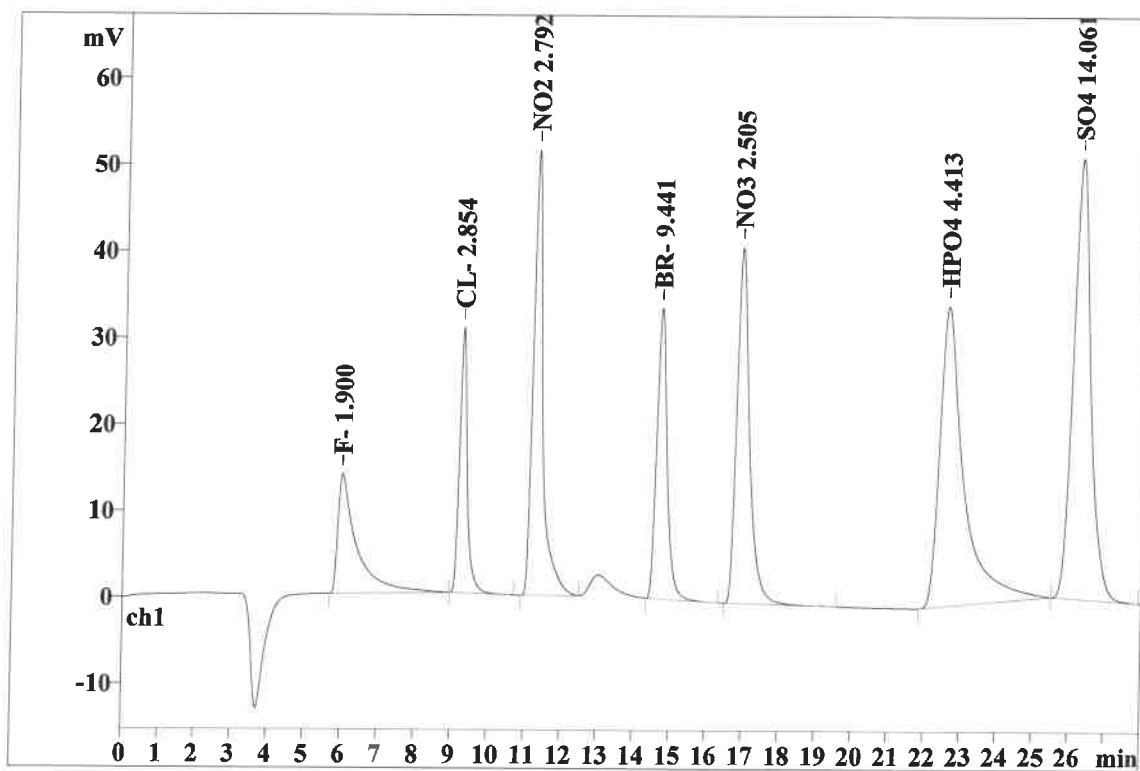

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	6.00	0.436	13.83	5.40	498.345	7.19
2	9.25	0.209	30.68	11.97	450.317	6.50
3	11.24	0.257	51.42	20.06	976.083	14.09
4	14.69	0.292	33.63	13.12	664.058	9.58
5	16.89	0.357	41.11	16.04	1006.020	14.52
6	22.58	0.605	34.67	13.53	1611.025	23.25
7	26.24	0.502	50.93	19.87	1722.482	24.86
7	28.00	0.380	256.28	99.99	6928.331	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:08:37 PM
Printed by: wet


Ident: N5394-01MSD
Analysis from: 10/31/2022 3:59:01 PM
File: _2022-10-31_

Last save: 11/1/2022 12:25:22 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32398

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

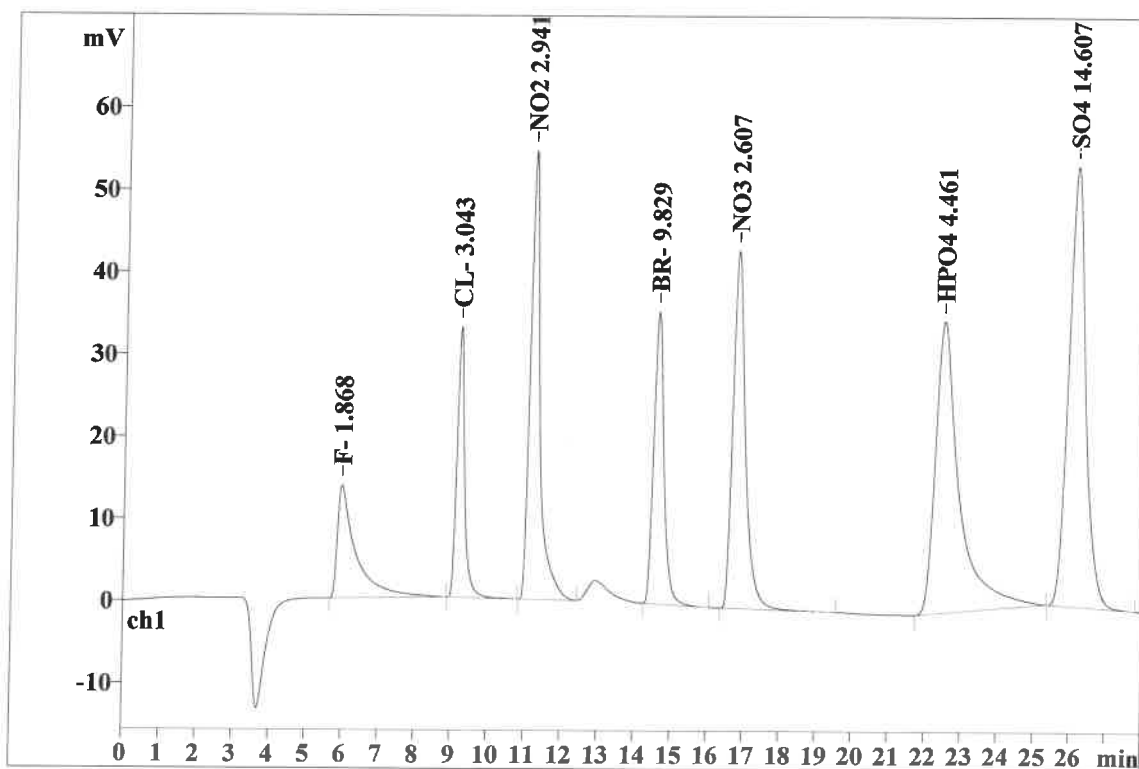

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.96	0.427	13.72	5.10	489.040	6.82
2	9.18	0.208	32.90	12.22	481.957	6.72
3	11.16	0.256	54.55	20.27	1032.272	14.40
4	14.57	0.289	35.56	13.21	693.424	9.67
5	16.75	0.353	43.45	16.14	1050.170	14.65
6	22.44	0.598	35.47	13.18	1627.868	22.70
7	26.08	0.499	53.50	19.88	1794.971	25.04
7	28.00	0.376	269.14	100.00	7169.703	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:08:45 PM
Printed by: wet


Ident: CCV
Analysis from: 10/31/2022 4:29:41 PM
File: _2022-10-31_

Last save: 10/31/2022 4:57:41 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32399

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 32
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

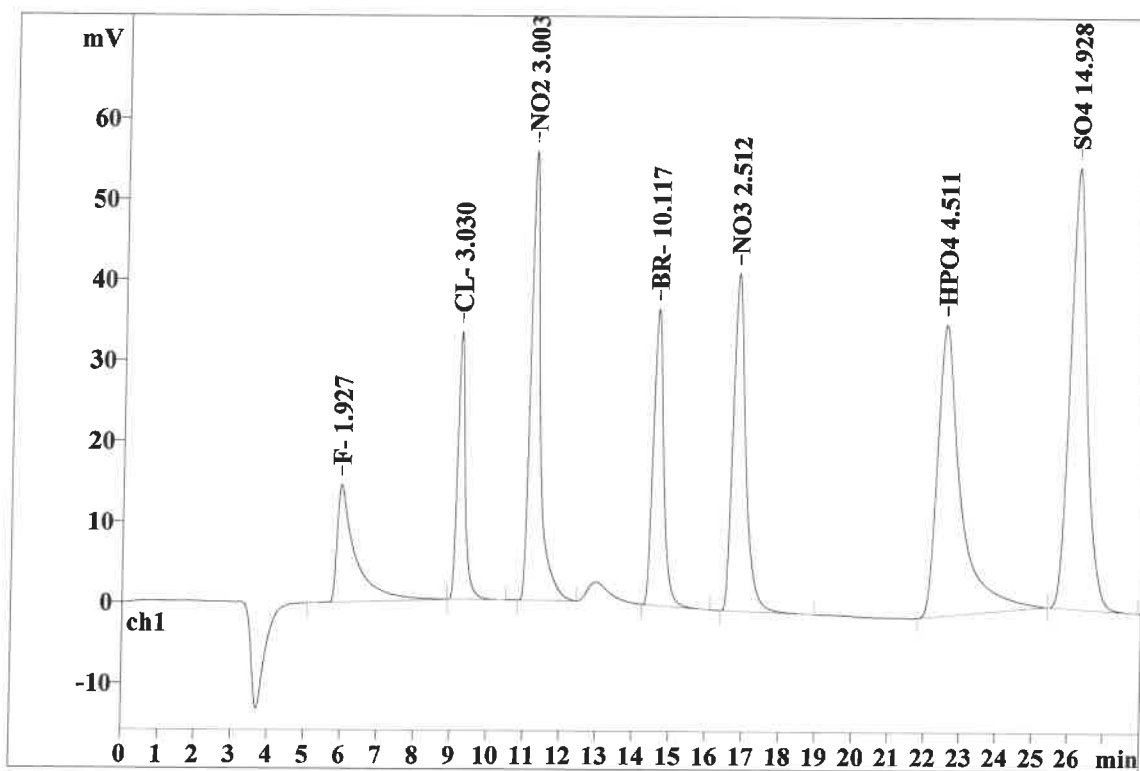

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.96	0.415	14.56	5.34	506.327	6.99
2	9.20	0.208	33.21	12.17	479.769	6.62
3	11.18	0.260	55.67	20.41	1055.486	14.56
4	14.59	0.289	36.73	13.46	715.137	9.87
5	16.77	0.353	41.85	15.34	1009.130	13.92
6	22.50	0.595	36.10	13.23	1645.189	22.70
7	26.15	0.501	54.69	20.05	1837.569	25.35
7	28.00	0.374	272.81	100.00	7248.607	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/1/2022 1:08:56 PM
Printed by: wet


Ident: CCB
Analysis from: 10/31/2022 5:00:24 PM
File: _2022-10-31_

Last save: 10/31/2022 5:28:24 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32400

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

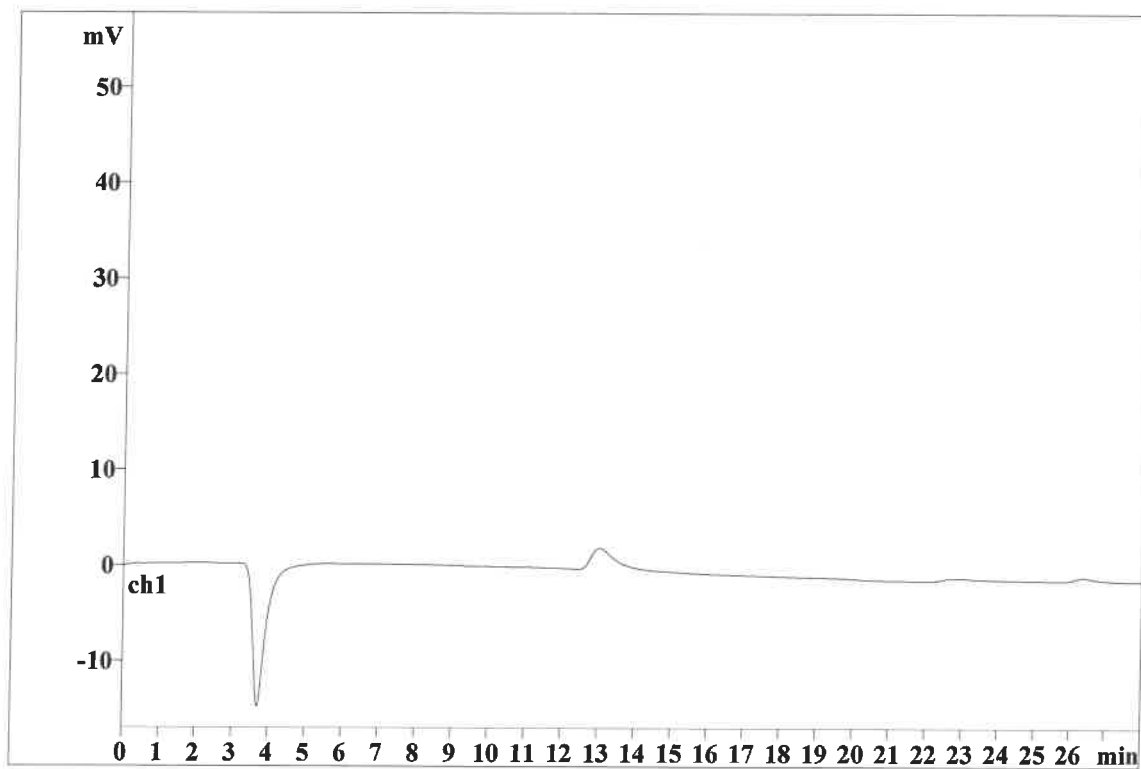

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD