

Clear table

Instrument ID: IC-2											Analyst :	IZ	Method:	300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-10-17_	10/17/22 11:14		IZ/MA				
STD2	0.4600	0.6690	0.6790	2.2670	0.5710	0.8860	3.5320	2022-10-17_	10/17/22 11:45		IZ/MA				
STD3	0.7820	1.2190	1.2070	4.0270	1.0100	1.9680	6.0830	2022-10-17_	10/17/22 12:15		IZ/MA				
STD4	0.9840	1.4910	1.4960	5.0330	1.2510	2.5410	7.5010	2022-10-17_	10/17/22 12:46		IZ/MA				
STD5	1.9760	2.9130	2.9080	9.6540	2.4100	5.1530	14.3160	2022-10-17_	10/17/22 13:16		IZ/MA				
STD6	3.9490	5.9190	5.9200	19.6570	4.9220	10.0590	29.4430	2022-10-17_	10/17/22 13:47		IZ/MA				
STD7	5.0500	7.5890	7.5900	25.3630	6.3370	12.3930	38.1240	2022-10-17_	10/17/22 14:18		IZ/MA				
ICV	1.9220	2.9820	3.0440	9.9700	2.4890	4.7350	14.7470	2022-10-17_	10/17/22 15:53		IZ/MA				
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-10-17_	10/17/22 16:24		IZ/MA				
CCV	2.0240	3.0480	3.0050	10.0260	2.4980	4.7770	14.8380	2022-11-02_	11/2/22 10:45		IZ/MA				
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-11-02_	11/2/22 12:00		IZ/MA				
LB122743BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-11-02_	11/2/22 12:08		IZ/MA				
LB122743BSW	2.0070	3.0790	3.0190	10.1610	2.5460	4.8990	14.9760	2022-11-02_	11/2/22 13:15		IZ/MA				
N5420-02	0.0000	9.9630	0.0000	0.0000	0.2280	-0.0910	8.3280	2022-11-02_	11/2/22 13:56		IZ/MA				
N5420-03	0.0000	9.5950	0.0000	0.0000	0.0000	0.0000	6.4500	2022-11-02_	11/2/22 14:27		IZ/MA				
N5420-04	0.0000	10.1030	0.0000	0.0000	0.2270	0.0000	8.2720	2022-11-02_	11/2/22 14:57		IZ/MA				
N5420-05	0.0000	9.7220	0.0000	0.0000	0.0000	0.0000	6.8570	2022-11-02_	11/2/22 15:28		IZ/MA				
N5420-05MS	2.4800	12.7180	2.9500	9.8810	2.5030	6.4420	20.1260	2022-11-02_	11/2/22 15:58		IZ/MA				
N5420-05MSD	2.2290	12.6890	2.8840	9.6110	2.4410	6.3860	19.6640	2022-11-02_	11/2/22 16:29		IZ/MA				
CCV	1.9950	2.9270	2.9320	9.7330	2.4320	5.4020	14.3630	2022-11-02_	11/2/22 17:00		IZ/MA				
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-11-02_	11/2/22 17:30		IZ/MA				
N5420-02DLX2	0.0000	4.7480	0.0000	0.0000	0.1960	0.0000	4.2870	2022-11-02_	11/2/22 18:01		IZ/MA				
N5420-03DLX2	0.0000	4.5060	0.0000	0.0000	0.0000	0.0000	3.5220	2022-11-02_	11/2/22 18:32		IZ/MA				
N5420-04DLX2	0.0000	4.7010	0.0000	0.0000	0.0000	0.0000	4.3130	2022-11-02_	11/2/22 19:02		IZ/MA				
N5420-05DLX2	0.0000	4.7440	0.0000	0.0000	0.0000	0.0000	3.7770	2022-11-02_	11/2/22 19:33		IZ/MA				
CCV	2.0080	2.9300	2.9180	9.7330	2.4250	5.2550	14.4050	2022-11-02_	11/2/22 20:04		IZ/MA				
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2022-11-02_	11/2/22 20:34		IZ/MA				

Report date: 11/3/2022 12:00:35 PM
Printed by: wet


Ident: CCV
Analysis from: 11/2/2022 10:45:49 AM
File: _2022-11-02_

Last save: 11/2/2022 11:13:49 AM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32413

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

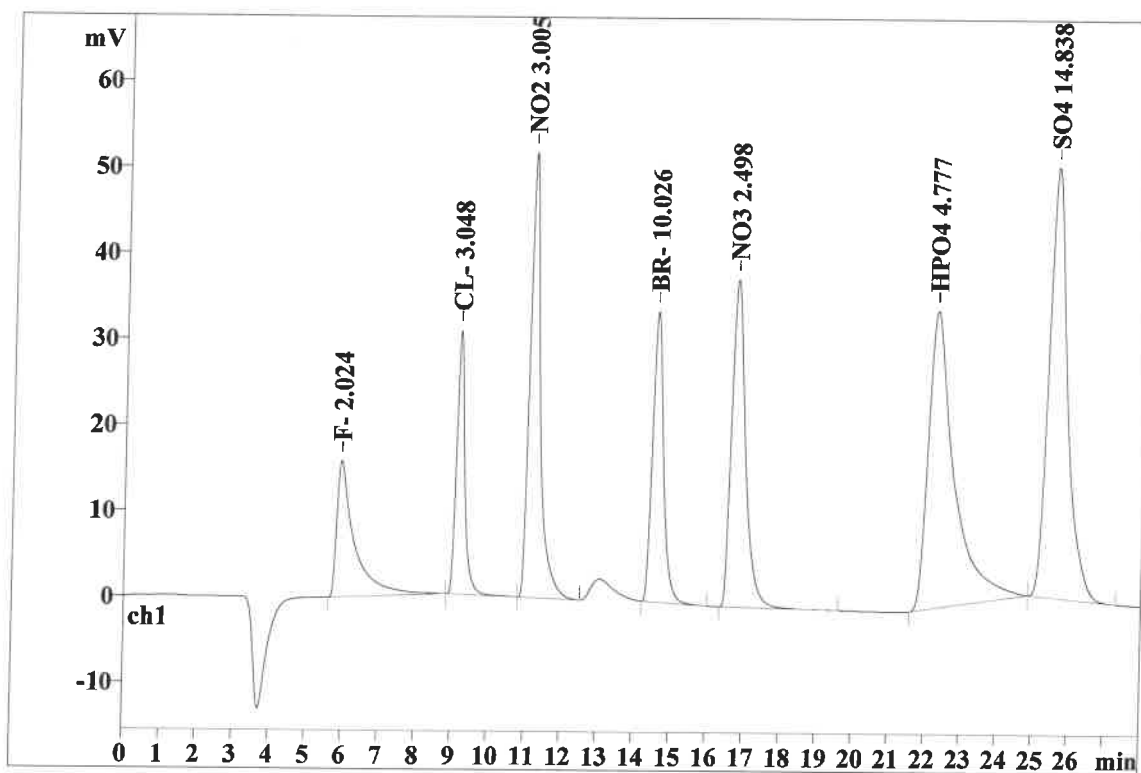

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.93	0.406	15.86	6.22	534.731	7.28
2	9.16	0.226	30.73	12.05	482.802	6.57
3	11.15	0.284	51.84	20.33	1056.492	14.38
4	14.57	0.314	33.81	13.26	708.308	9.64
5	16.74	0.390	38.10	14.94	1003.090	13.65
6	22.26	0.672	34.60	13.57	1738.373	23.65
7	25.56	0.531	50.07	19.63	1825.582	24.84
7	28.00	0.403	255.00	100.00	7349.377	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:01:36 PM
Printed by: wet


Ident: CCB
Analysis from: 11/2/2022 12:00:19 PM
File: _2022-11-02_

Last save: 11/3/2022 12:01:34 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32415

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

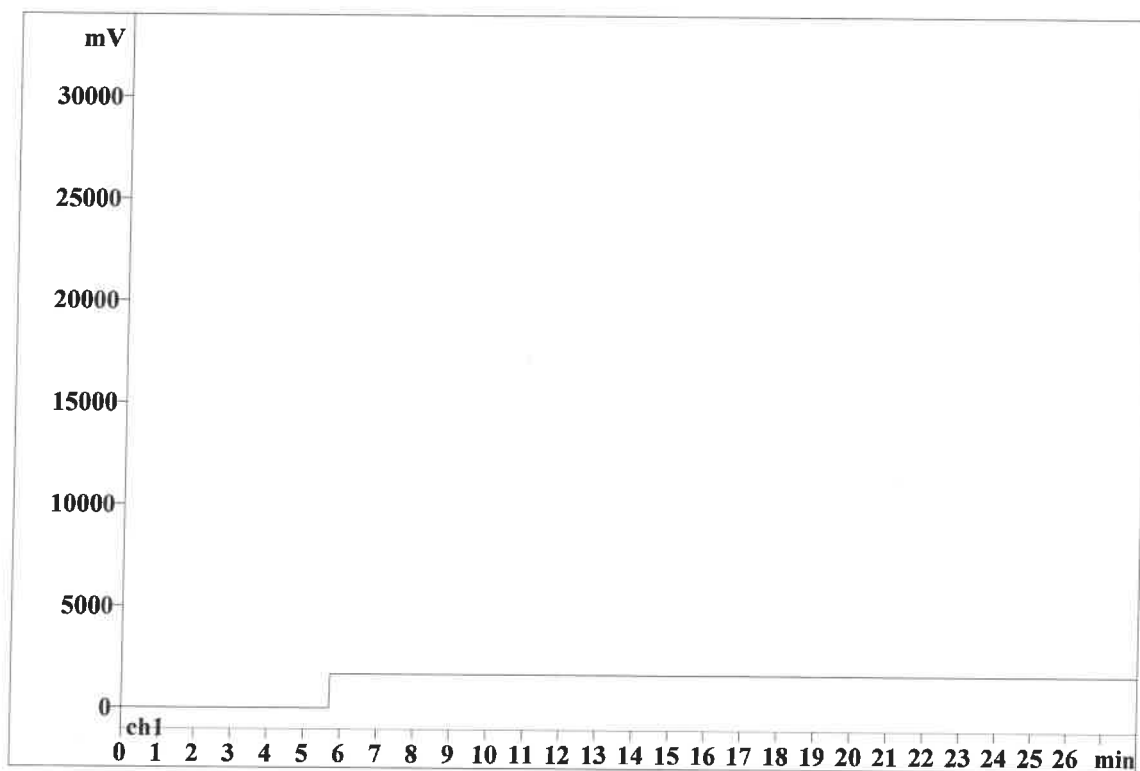

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:02:00 PM
Printed by: wet


Ident: LB122743BLW
Analysis from: 11/2/2022 12:08:44 PM
File: _2022-11-02_

Last save: 11/3/2022 12:00:27 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32416

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 13
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

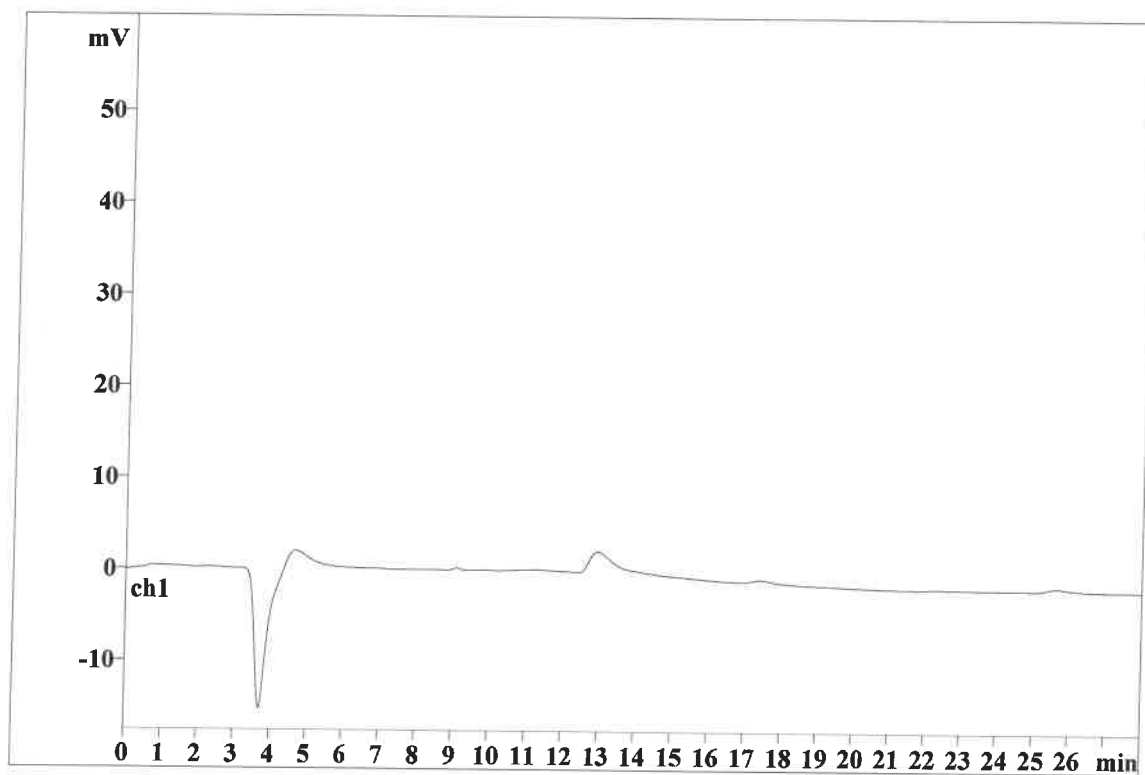

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:02:07 PM
Printed by: wet


Ident: LB122743BSW
Analysis from: 11/2/2022 1:15:09 PM
File: _2022-11-02_

Last save: 11/3/2022 12:00:27 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32418

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

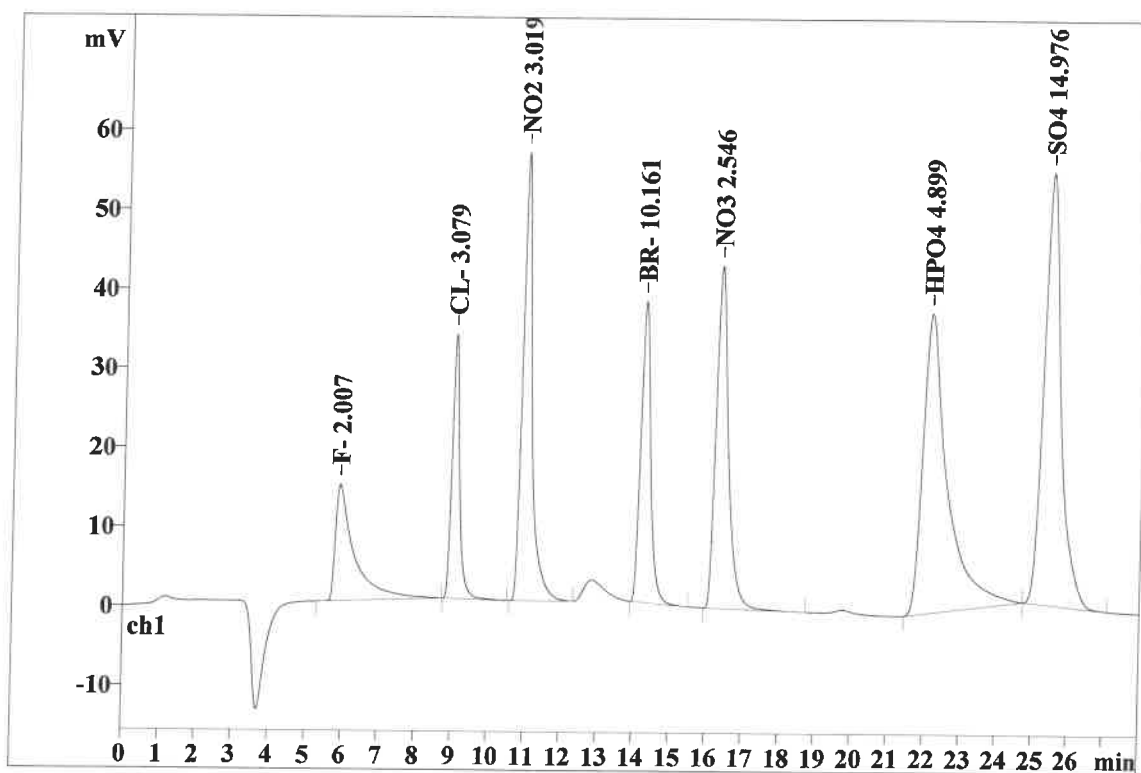

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.90	0.437	14.68	5.28	529.673	7.11
2	9.03	0.210	33.36	12.00	487.973	6.55
3	10.95	0.260	56.46	20.32	1061.593	14.26
4	14.24	0.282	37.99	13.67	718.512	9.65
5	16.31	0.347	43.16	15.53	1023.741	13.75
6	22.11	0.616	37.78	13.60	1781.382	23.92
7	25.41	0.488	54.43	19.59	1844.005	24.76
7	28.00	0.377	277.86	100.00	7446.879	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:02:24 PM
Printed by: wet


Ident: N5420-02
Analysis from: 11/2/2022 1:56:25 PM
File: _2022-11-02_

Last save: 11/2/2022 2:24:25 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32419

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

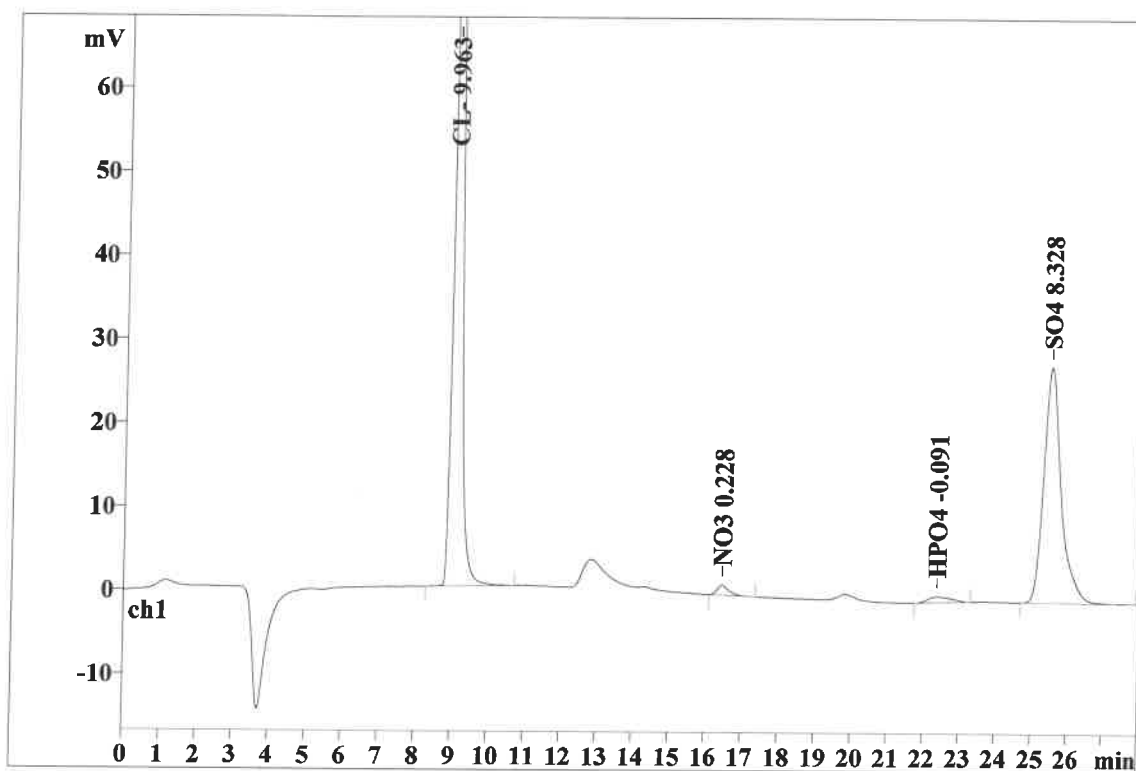

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.02	0.201	116.64	79.56	1639.355	61.65
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.46	0.353	1.15	0.79	27.129	1.02
6	22.36	0.785	0.68	0.46	31.203	1.17
7	25.48	0.489	28.12	19.18	961.532	36.16
7	28.00	0.261	146.59	100.00	2659.220	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:02:36 PM
Printed by: wet


Ident: N5420-03
Analysis from: 11/2/2022 2:27:03 PM
File: _2022-11-02_

Last save: 11/2/2022 2:55:03 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32420

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

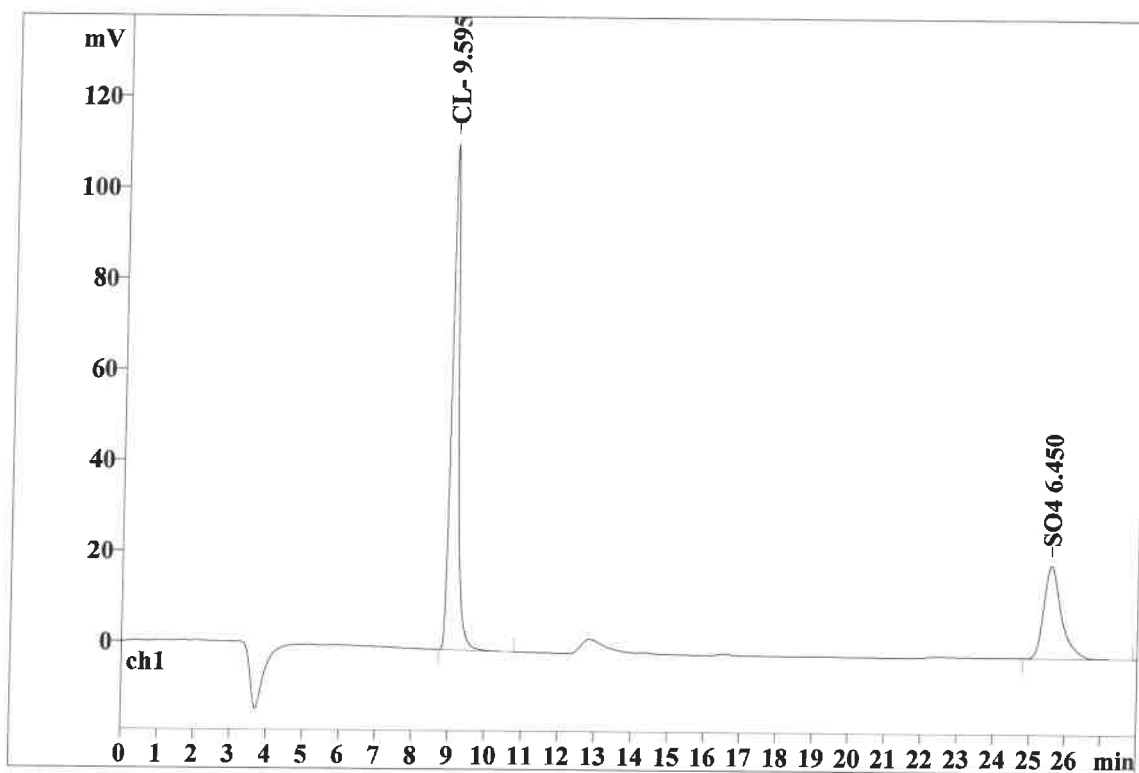

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.04	0.203	111.41	84.48	1577.812	68.90
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.58	0.501	20.46	15.52	712.313	31.10
7	28.00	0.101	131.88	100.00	2290.125	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:02:47 PM
Printed by: wet


Ident: N5420-04
Analysis from: 11/2/2022 2:57:41 PM
File: _2022-11-02_

Last save: 11/2/2022 3:25:41 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32421

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 20
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

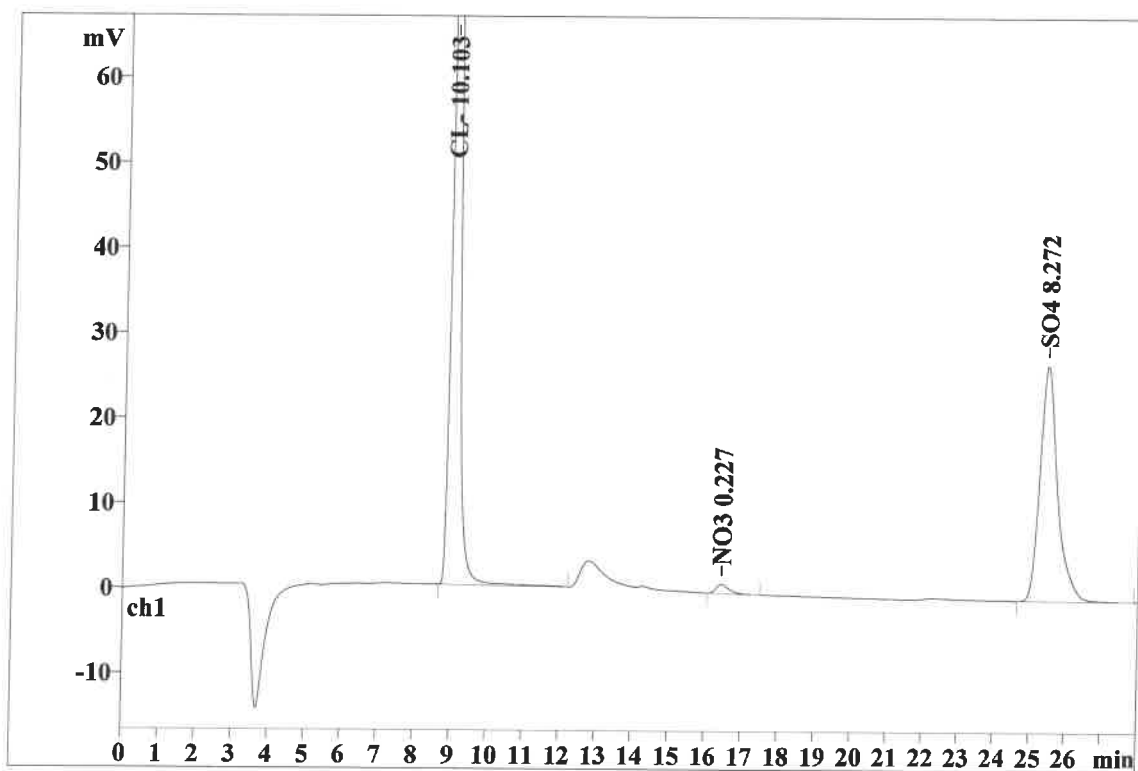

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.99	0.202	116.53	80.23	1662.767	62.90
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.44	0.362	1.08	0.75	26.608	1.01
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.43	0.497	27.63	19.02	954.113	36.09
7	28.00	0.152	145.24	100.00	2643.489	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:02:55 PM
Printed by: wet


Ident: N5420-05
Analysis from: 11/2/2022 3:28:19 PM
File: _2022-11-02_

Last save: 11/2/2022 3:56:19 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32422

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 21
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

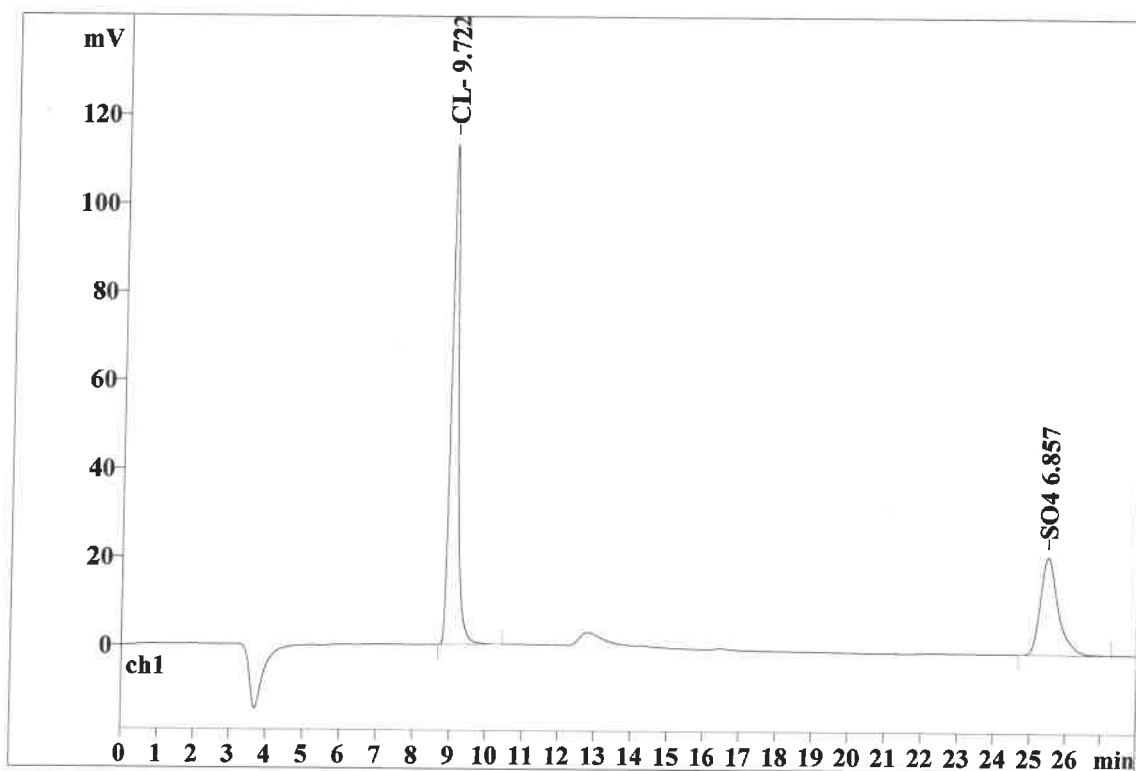

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.00	0.203	113.33	83.73	1599.053	67.60
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.47	0.501	22.03	16.27	766.303	32.40
7	28.00	0.101	135.36	100.00	2365.355	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:14 PM
Printed by: wet


Ident: N5420-05MS
Analysis from: 11/2/2022 3:58:57 PM
File: _2022-11-02_

Last save: 11/2/2022 4:26:57 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32423

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 22
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

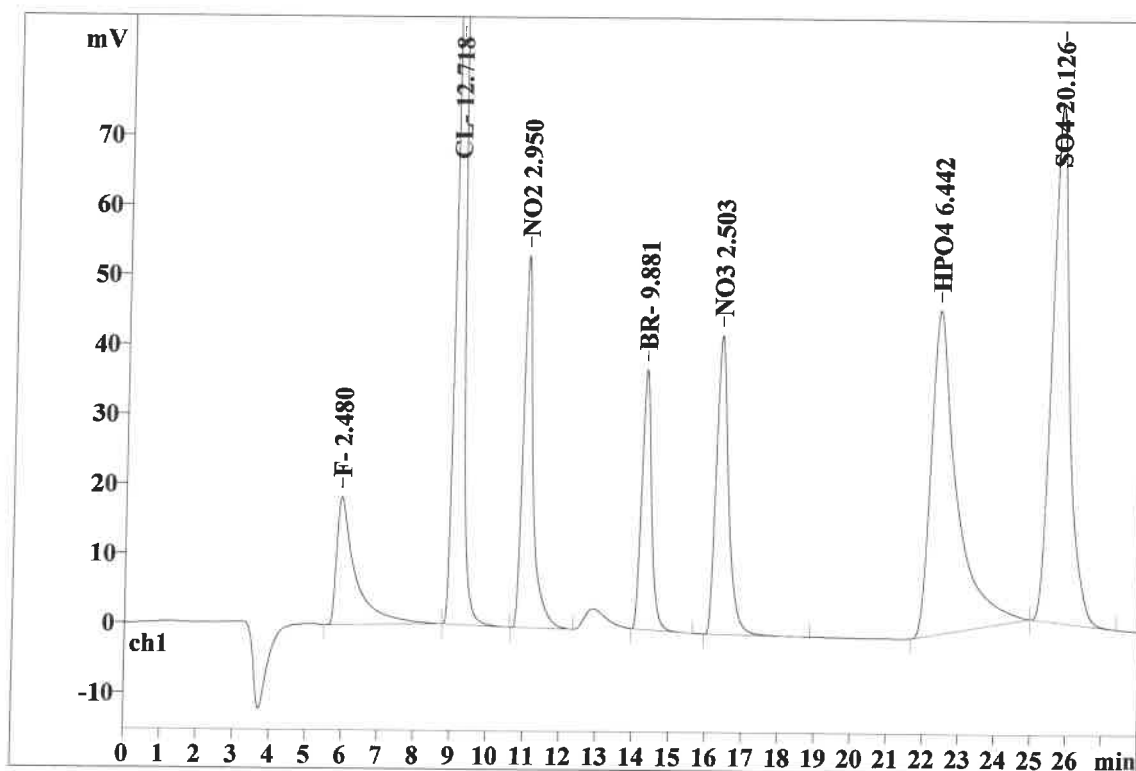

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.93	0.451	18.32	4.35	668.834	6.46
2	9.08	0.204	147.83	35.15	2100.165	20.28
3	10.99	0.266	53.42	12.70	1035.731	10.00
4	14.27	0.280	37.32	8.87	697.323	6.73
5	16.32	0.346	42.84	10.19	1005.446	9.71
6	22.34	0.660	46.53	11.06	2322.353	22.42
7	25.64	0.493	74.30	17.67	2527.500	24.40
7	28.00	0.386	420.55	100.00	10357.353	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:21 PM
Printed by: wet


Ident: N5420-05MSD
Analysis from: 11/2/2022 4:29:34 PM
File: _2022-11-02_

Last save: 11/2/2022 4:57:35 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32424

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

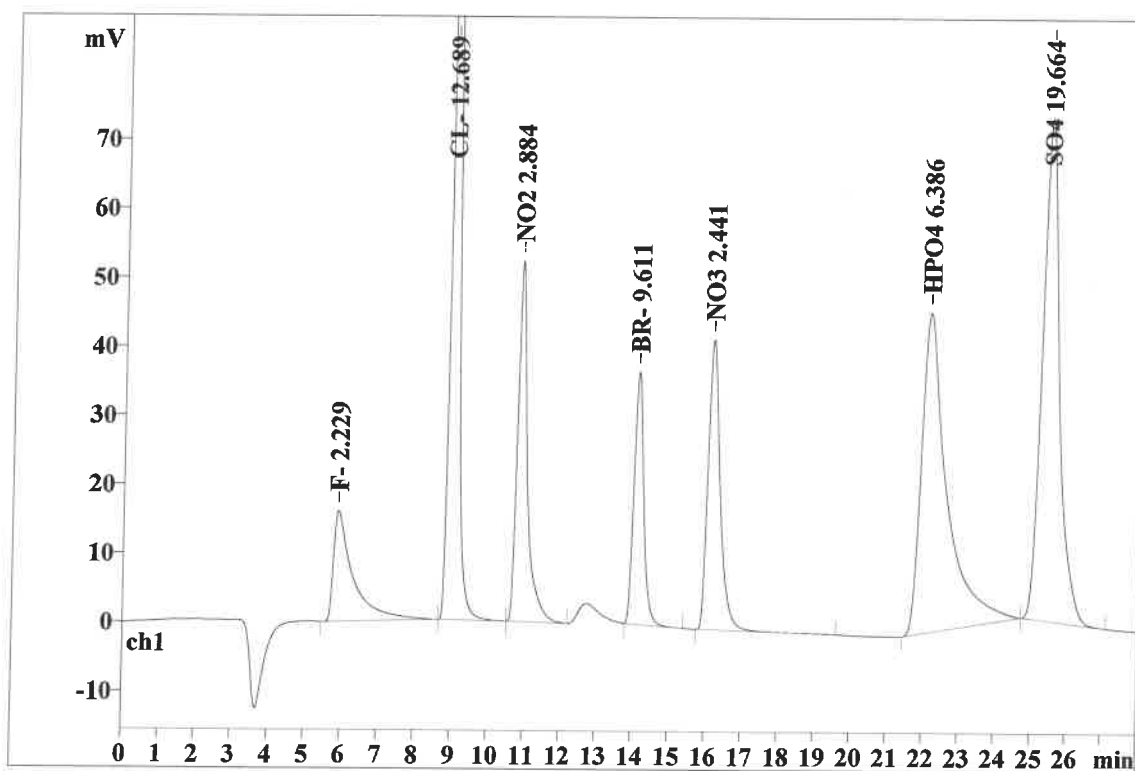

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.89	0.457	16.03	3.86	594.905	5.88
2	8.97	0.202	148.90	35.86	2095.235	20.69
3	10.86	0.264	52.32	12.60	1010.753	9.98
4	14.11	0.277	36.58	8.81	676.909	6.69
5	16.14	0.343	42.05	10.13	978.594	9.66
6	22.11	0.655	46.40	11.18	2302.897	22.74
7	25.40	0.490	72.88	17.56	2466.225	24.36
7	28.00	0.384	415.17	100.00	10125.517	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:28 PM
Printed by: wet


Ident: CCV
Analysis from: 11/2/2022 5:00:18 PM
File: _2022-11-02_

Last save: 11/2/2022 5:28:18 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32425

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

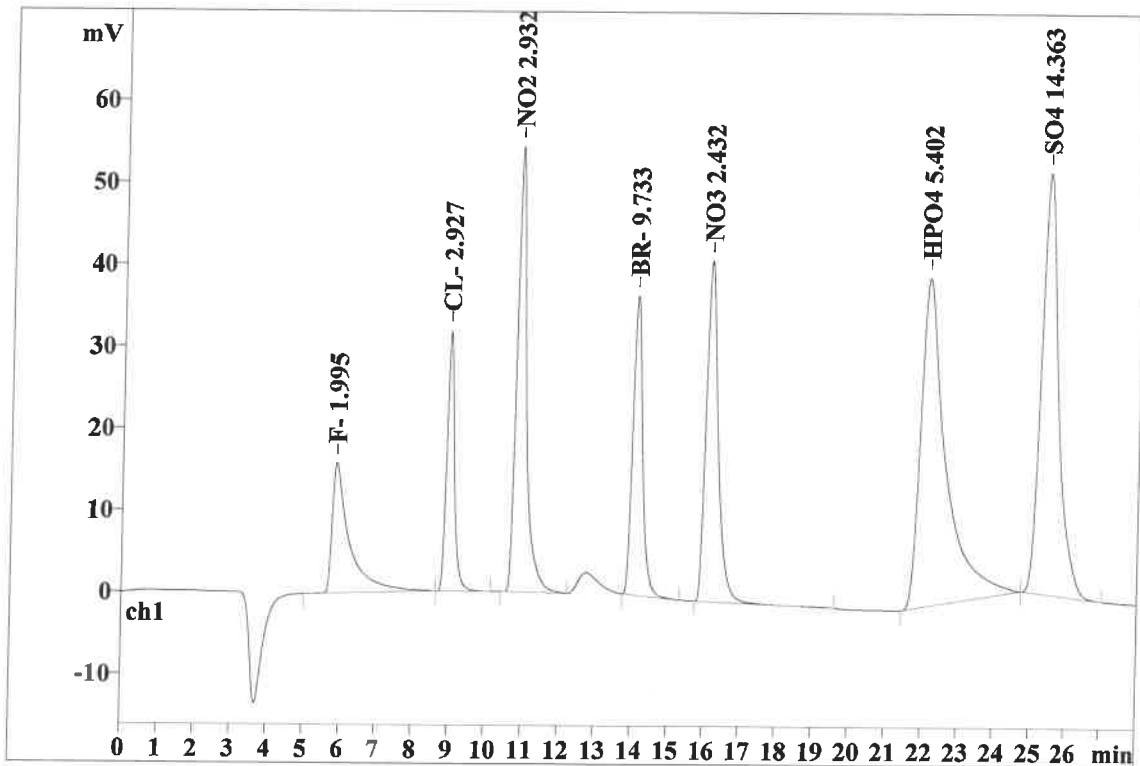

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.87	0.398	15.96	5.88	526.236	7.11
2	8.97	0.213	31.73	11.68	462.578	6.25
3	10.86	0.265	54.36	20.01	1029.002	13.91
4	14.08	0.281	36.51	13.44	686.124	9.27
5	16.11	0.344	41.63	15.32	974.666	13.17
6	22.12	0.643	40.05	14.74	1957.718	26.46
7	25.43	0.497	51.44	18.93	1762.546	23.82
7	28.00	0.377	271.69	100.00	7398.870	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:35 PM
Printed by: wet


Ident: CCB
Analysis from: 11/2/2022 5:30:55 PM
File: _2022-11-02_

Last save: 11/2/2022 5:58:55 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32426

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

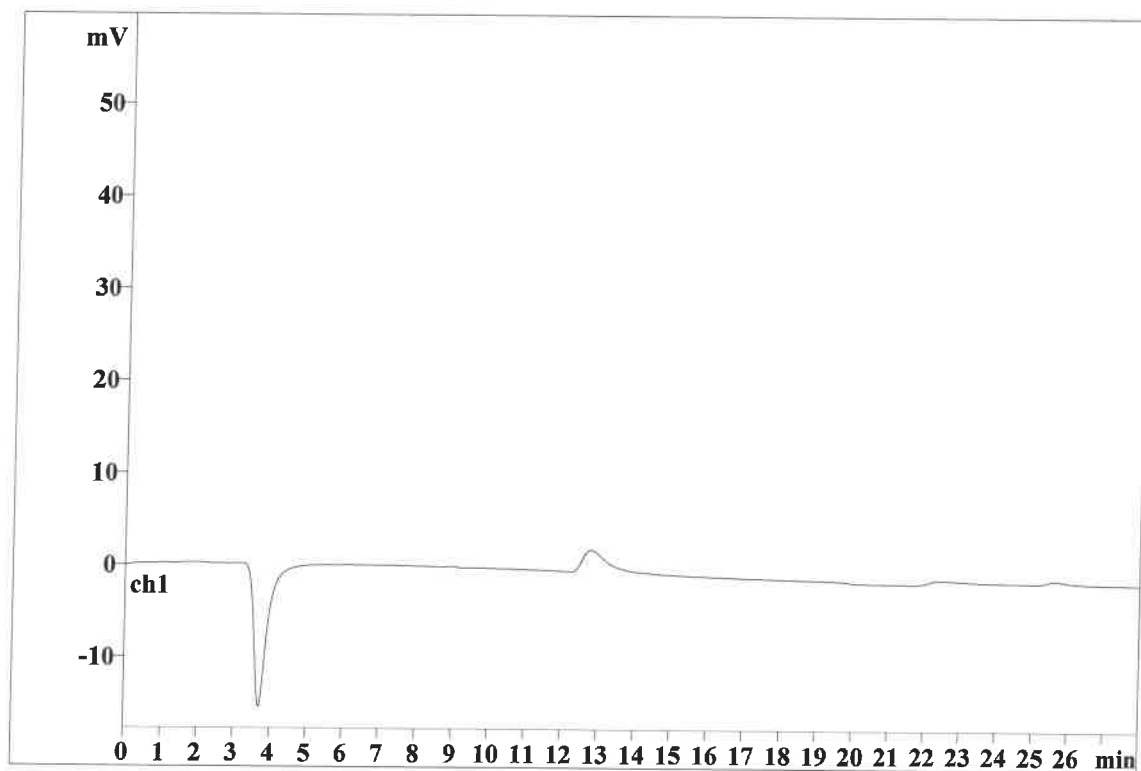

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:43 PM
Printed by: wet


Ident: N5420-02DLX2
Analysis from: 11/2/2022 6:01:37 PM
File: _2022-11-02_

Last save: 11/2/2022 6:29:37 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32427

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 24
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

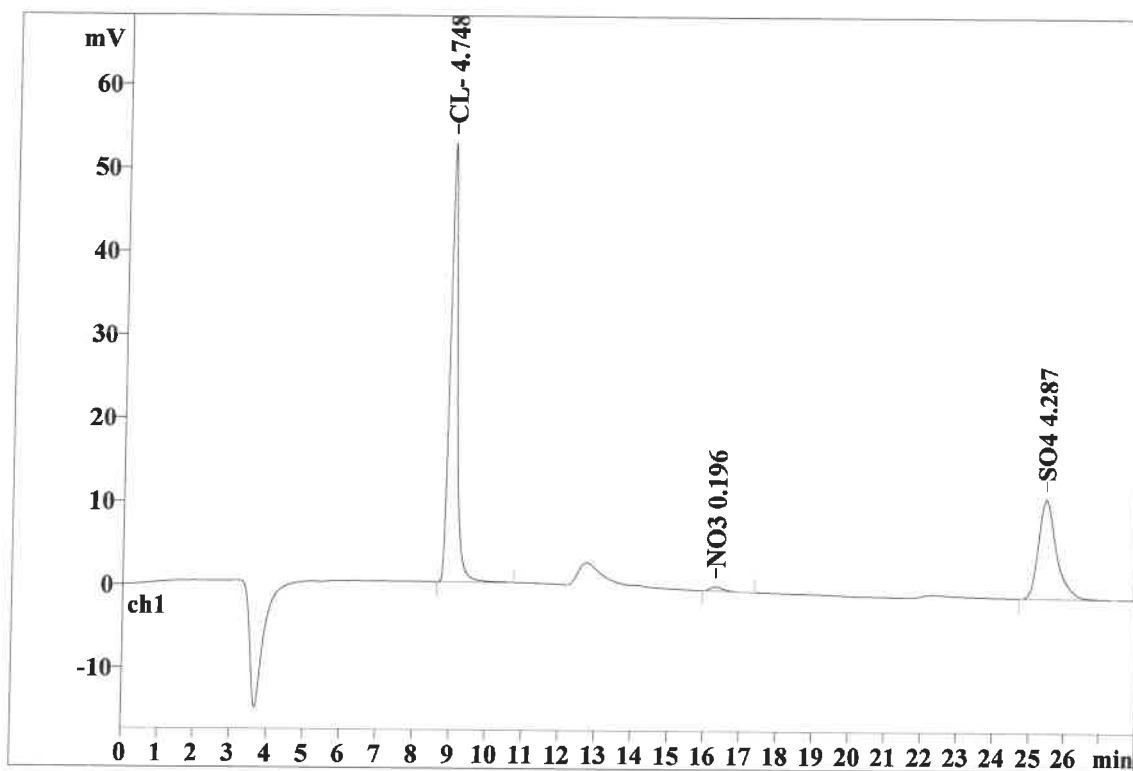

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.96	0.210	52.62	80.89	767.073	63.63
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	16.29	0.369	0.52	0.80	13.200	1.10
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.42	0.515	11.91	18.30	425.203	35.27
7	28.00	0.156	65.05	99.99	1205.476	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:50 PM
Printed by: wet


Ident: N5420-03DLX2
Analysis from: 11/2/2022 6:32:16 PM
File: _2022-11-02_

Last save: 11/2/2022 7:00:16 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32428

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 25
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

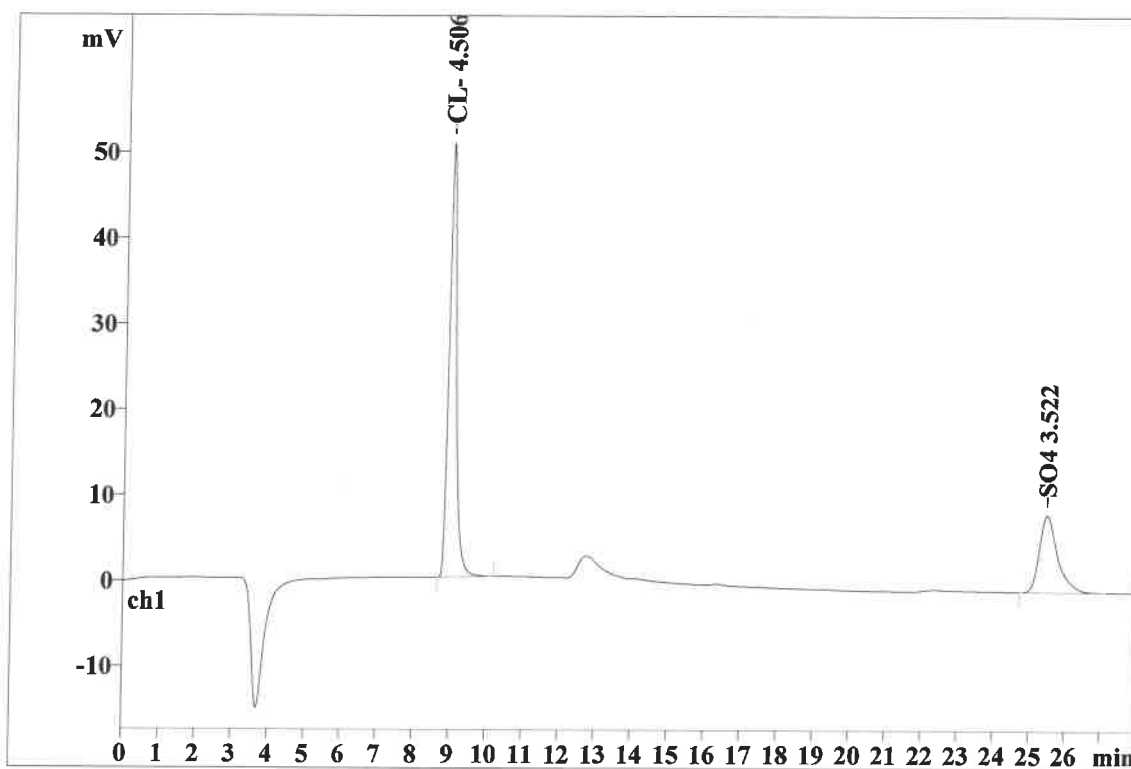

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.97	0.209	50.71	84.93	726.592	69.19
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.46	0.518	8.99	15.06	323.559	30.81
7	28.00	0.104	59.70	100.00	1050.151	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:03:56 PM
Printed by: wet


Ident: N5420-04DLX2
Analysis from: 11/2/2022 7:02:53 PM
File: _2022-11-02_

Last save: 11/2/2022 7:30:54 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32429

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 26
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

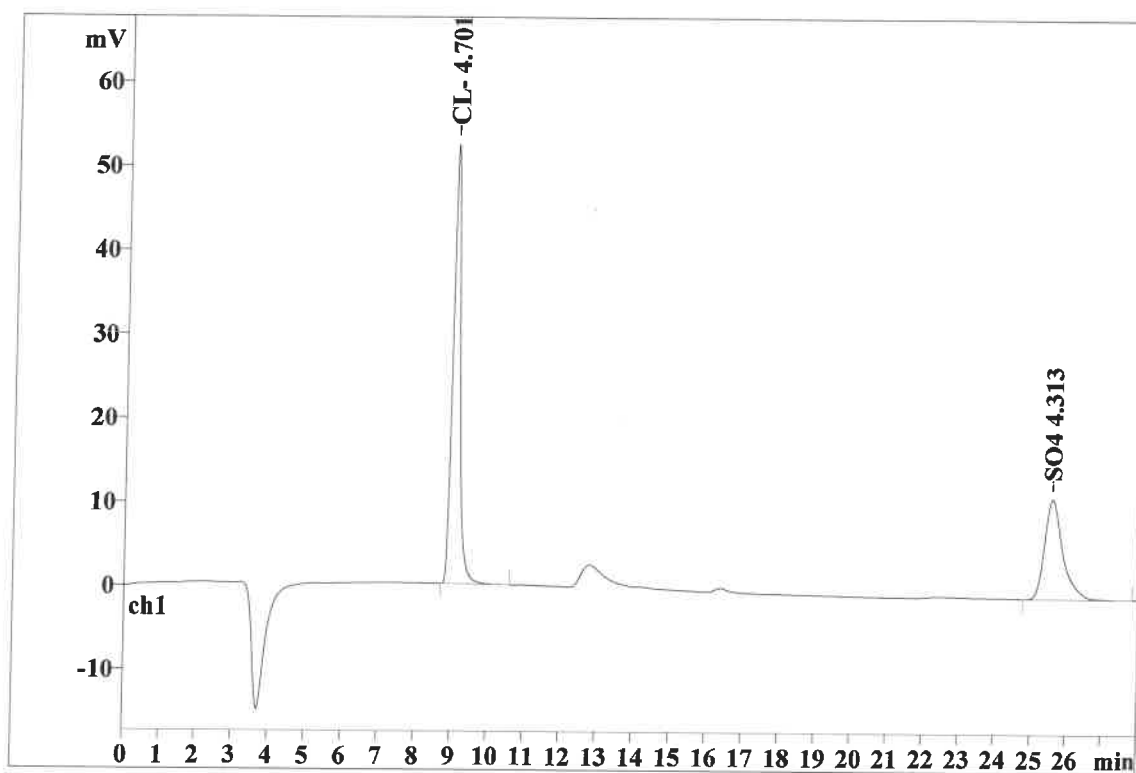

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	9.01	0.211	52.33	81.47	759.189	63.91
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.56	0.519	11.90	18.53	428.644	36.09
7	28.00	0.104	64.23	100.00	1187.833	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:04:03 PM
Printed by: wet


Ident: N5420-05DLX2
Analysis from: 11/2/2022 7:33:31 PM
File: _2022-11-02_

Last save: 11/2/2022 8:01:32 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32430

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 27
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

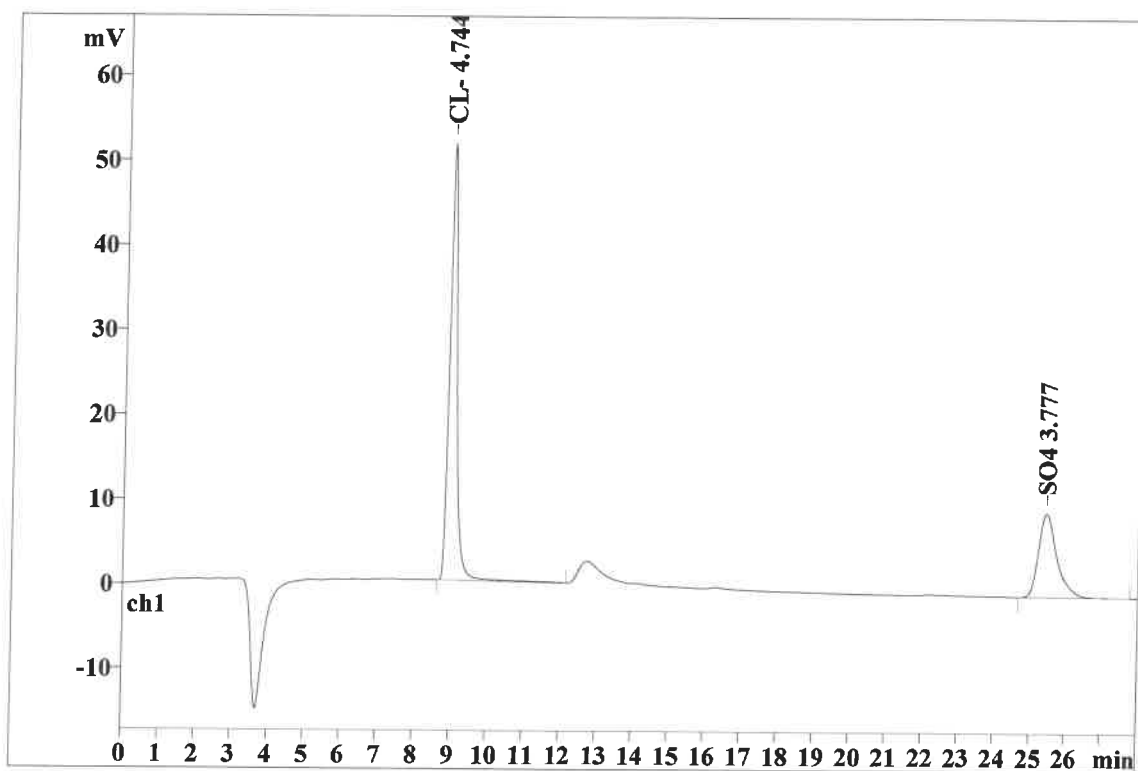

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.96	0.211	51.55	83.89	766.375	68.20
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.43	0.520	9.90	16.11	357.408	31.80
7	28.00	0.104	61.45	100.00	1123.783	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:04:11 PM
Printed by: wet


Ident: CCV
Analysis from: 11/2/2022 8:04:15 PM
File: _2022-11-02_

Last save: 11/2/2022 8:32:15 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32431

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

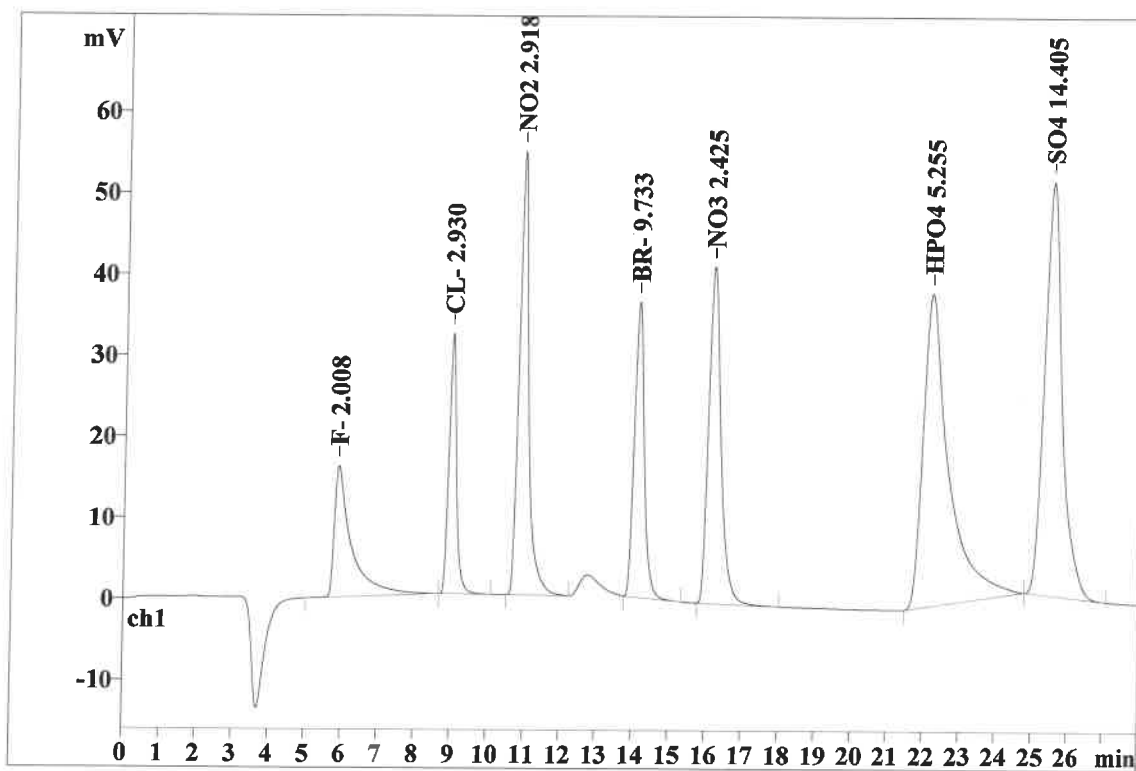

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.88	0.392	16.18	5.99	530.122	7.21
2	8.98	0.212	32.12	11.89	462.982	6.30
3	10.87	0.265	54.61	20.22	1023.726	13.93
4	14.09	0.283	36.36	13.46	686.120	9.34
5	16.13	0.347	41.48	15.35	971.641	13.22
6	22.14	0.653	38.51	14.25	1906.082	25.94
7	25.45	0.504	50.87	18.83	1768.233	24.06
7	28.00	0.379	270.13	100.00	7348.905	100.00

This report has been created by IC Net
METROHM LTD

Report date: 11/3/2022 12:04:18 PM
Printed by: wet


Ident: CCB
Analysis from: 11/2/2022 8:34:53 PM
File: _2022-11-02_

Last save: 11/2/2022 9:02:53 PM

Method: AnionsIC2-101722.mtw
Run operator: wet
Analysis number: 32432

Last save: 10/27/2022 9:16

SAMPLE:
: IZ/MA
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

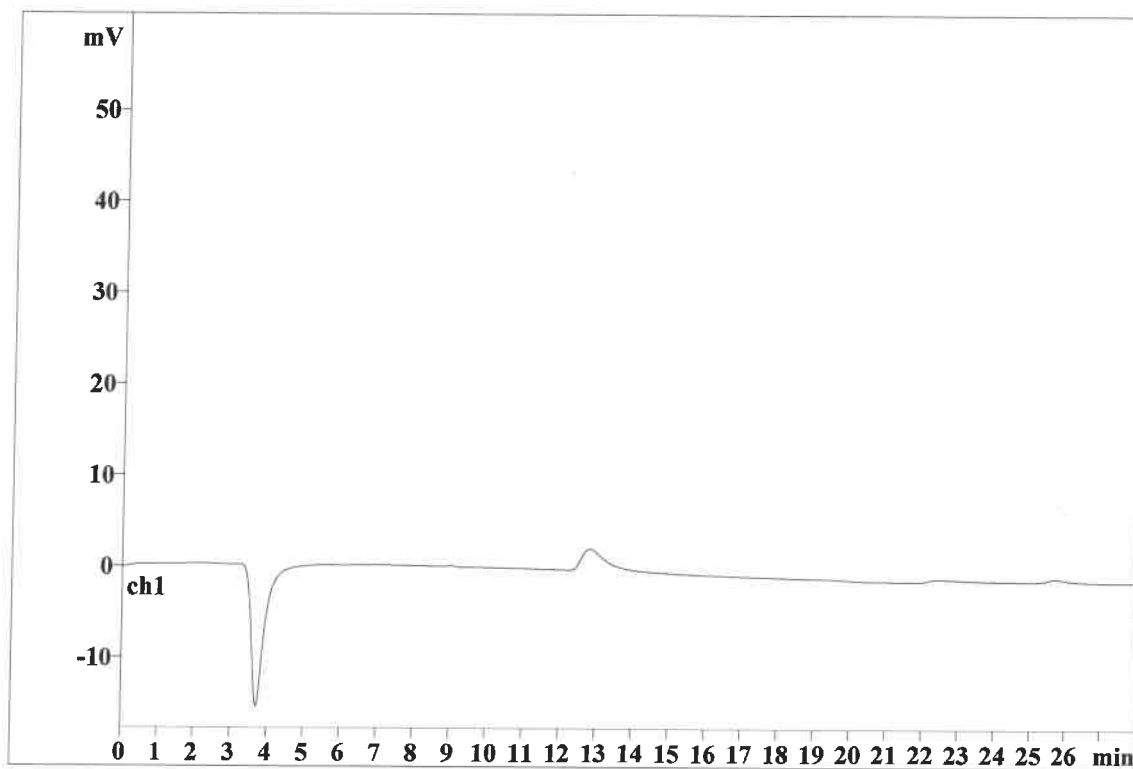

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

WORKLIST(Hardcopy Internal Chain)

LB122743

WorkList Name : Anions-110222 WorkList ID : 164619 Department : Wet-Chemistry Date : 11-02-2022 09:21:45

Due Date	Matrix	Sample	Test	Preservative	Customer	Raw Sample Storage Location	Customer Sample	Collect Date	Method
11/03/2022	Water	N5420-02	Anions Group1	Cool 4 deg C	TETR06	F11	RW8-PT-IN01-11012022	11/01/2022	300.0
11/03/2022	Water	N5420-03	Anions Group1	Cool 4 deg C	TETR06	F11	RW8-PT-OUT01-11012022	11/01/2022	300.0
11/03/2022	Water	N5420-04	Anions Group1	Cool 4 deg C	TETR06	F11	RW8-PT-IN02-11012022	11/01/2022	300.0
11/03/2022	Water	N5420-05	Anions Group1	Cool 4 deg C	TETR06	F11	RW8-PT-OUT-02-11012022	11/01/2022	300.0

Date/Time 11/02/22 14:00
 Raw Sample Received by: 12 (SC)
 Raw Sample Relinquished by: 12 (SC)

Date/Time 11/02/22 15:20
 Raw Sample Received by: 12 (SC)
 Raw Sample Relinquished by: 12 (SC)